
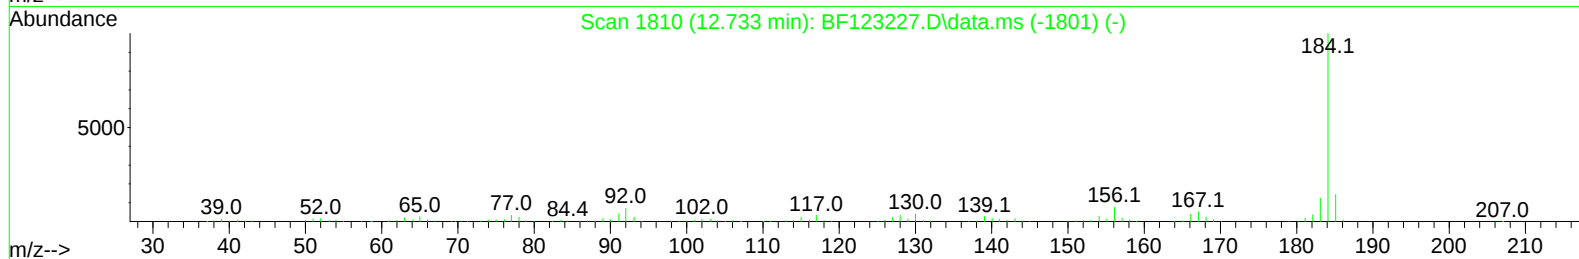
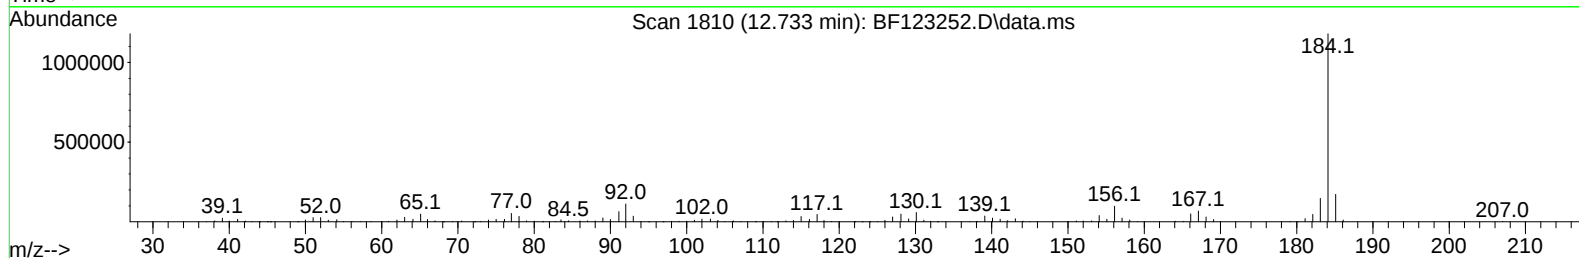


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022221\
Data File : BF123252.D
Acq On : 22 Feb 2021 10:10
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 22 11:30:40 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 19 16:08:53 2021
Response via : Initial Calibration

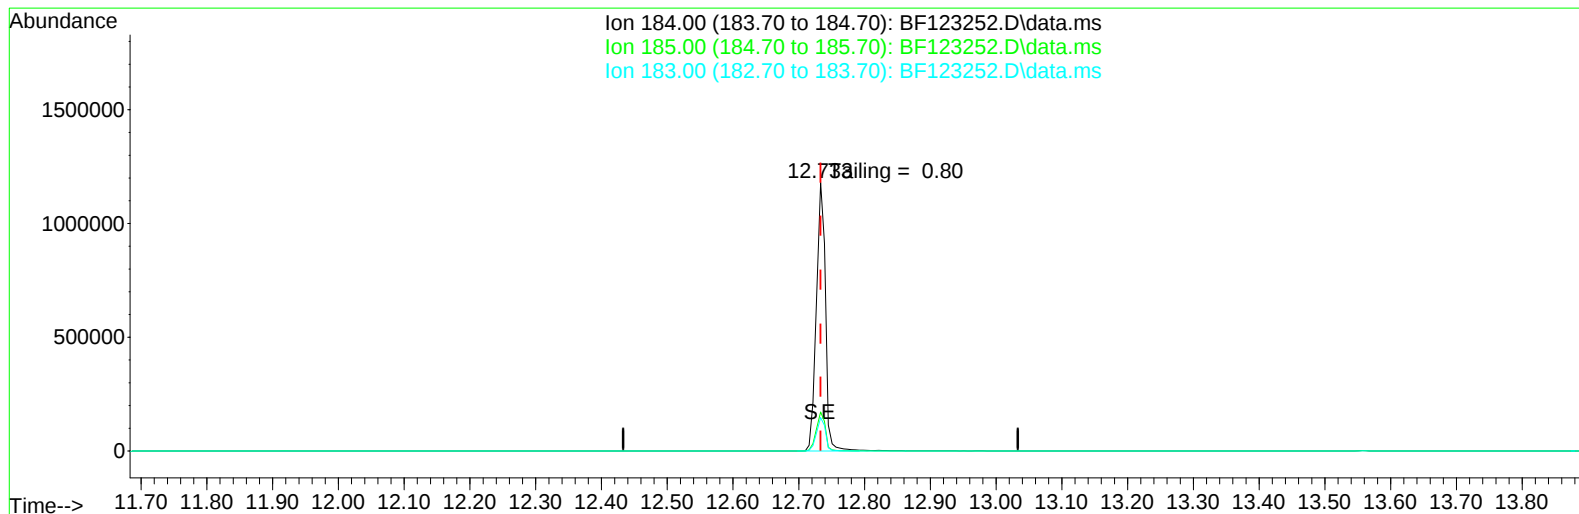

TIC: BF123252.D\data.ms

(77) Benzidine




12.733min (+ 0.000) 0.00 ng

response 1153159

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.55
183.00	12.10	12.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022221\
Data File : BF123252.D
Acq On : 22 Feb 2021 10:10
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 22 11:30:40 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 19 16:08:53 2021
Response via : Initial Calibration

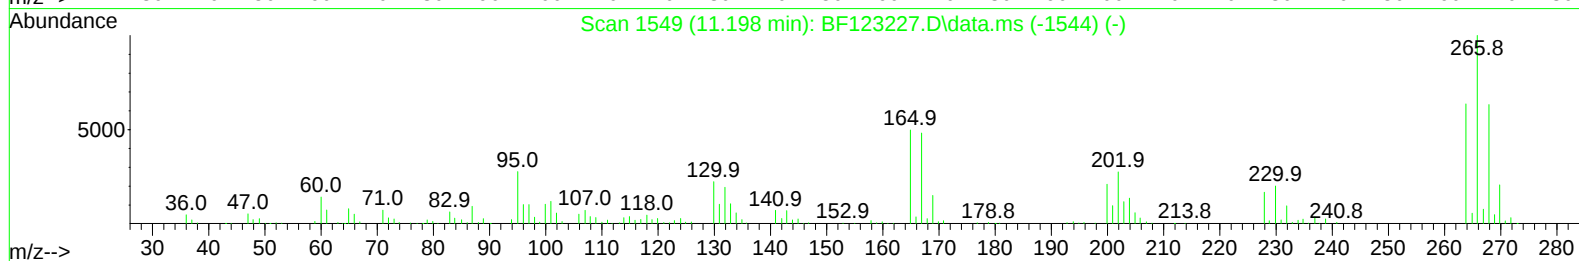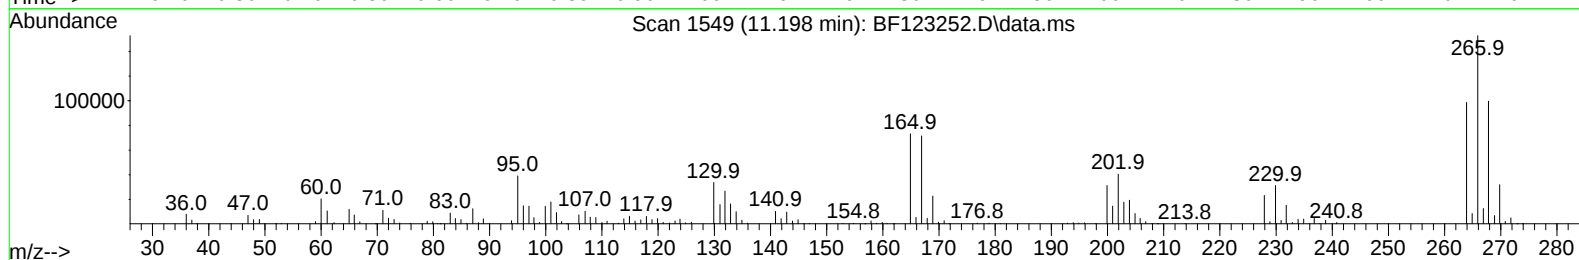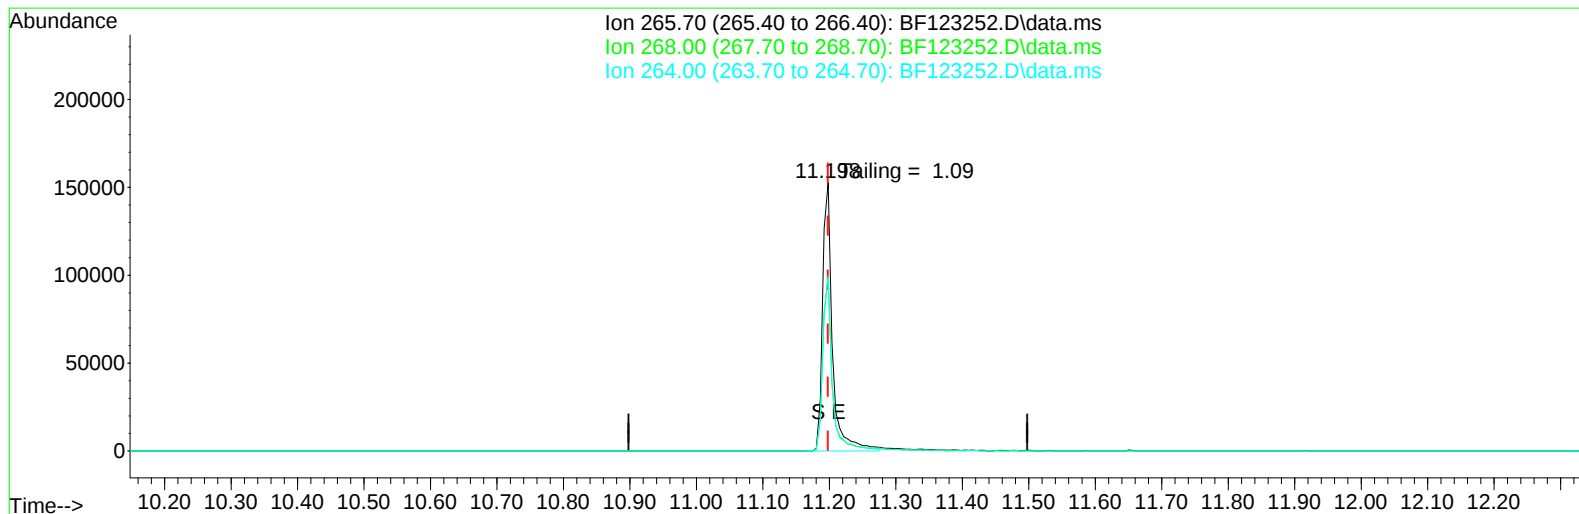

TIC: BF123252.D\data.ms

(70) Pentachlorophenol (C)

11.198min (+ 0.000) 29875.80 ng

response 162482

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	65.26
264.00	62.30	64.61
0.00	0.00	0.00