

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022221\
 Data File : BF123257.D
 Acq On : 22 Feb 2021 14:06
 Operator : JU/CG
 Sample : PB134758BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB134758BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF123257.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.492	574	579	582	rBV	3783893	3765631	79.02%	13.571%
2	6.492	743	749	752	rBV	3703986	3764578	79.00%	13.568%
3	6.857	807	811	814	rBV	851325	737587	15.48%	2.658%
4	7.416	901	906	909	rBV	2319105	2468928	51.81%	8.898%
5	8.139	1024	1029	1033	rBV	1042725	978518	20.53%	3.527%
6	9.216	1207	1212	1216	rBV	3881108	4232800	88.82%	15.255%
7	9.898	1323	1328	1332	rBV	1240419	1107023	23.23%	3.990%
8	10.692	1457	1463	1466	rBV	2782353	2611209	54.79%	9.411%
9	11.392	1576	1582	1585	rBV	1220306	1166316	24.47%	4.203%
10	12.986	1846	1853	1856	rBV	5113348	4765461	100.00%	17.175%
11	14.039	2028	2032	2035	rBV	1322455	1093863	22.95%	3.942%
12	15.515	2277	2283	2295	rBV	793808	1054827	22.13%	3.802%




Sum of corrected areas: 27746741

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022221\
Data File : BF123257.D
Acq On : 22 Feb 2021 14:06
Operator : JU/CG
Sample : PB134758BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB134758BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

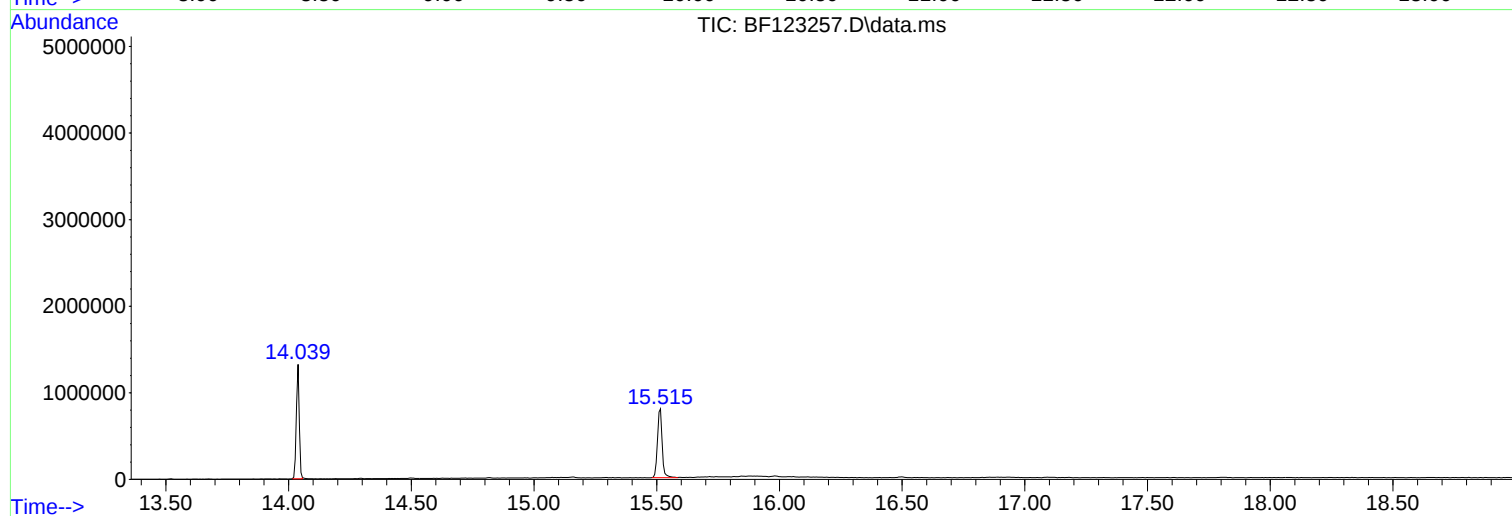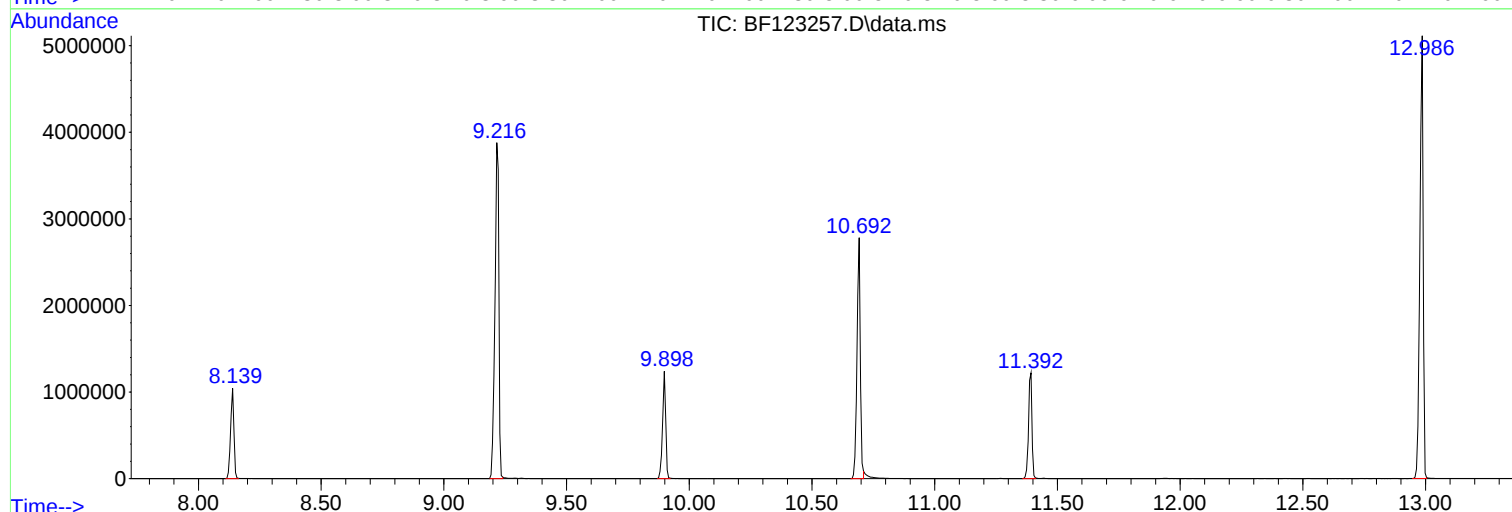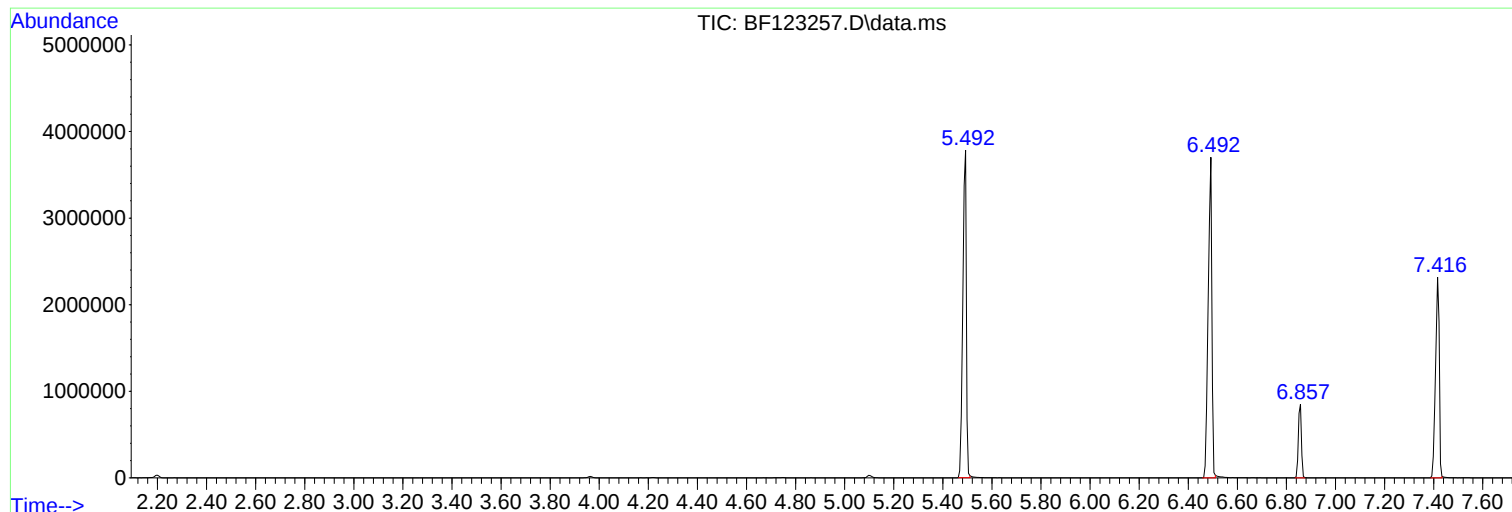

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022221\
Data File : BF123257.D
Acq On : 22 Feb 2021 14:06
Operator : JU/CG
Sample : PB134758BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB134758BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022221\
Data File : BF123257.D
Acq On : 22 Feb 2021 14:06
Operator : JU/CG
Sample : PB134758BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB134758BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------