

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022221\
 Data File : BF123261.D
 Acq On : 22 Feb 2021 16:30
 Operator : JU/CG
 Sample : M1452-08
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF123261.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.810	108	123	131	rVB	274623	394864	8.65%	1.345%
2	4.657	433	437	442	rBV	457935	467986	10.25%	1.595%
3	5.081	505	509	510	rBV	88442	98326	2.15%	0.335%
4	5.098	510	512	518	rVB	208705	195298	4.28%	0.665%
5	5.487	574	578	581	rBV	3003391	2755036	60.36%	9.388%
6	6.492	744	749	762	rBV	2822698	2732256	59.86%	9.310%
7	6.857	807	811	814	rBV	994547	738877	16.19%	2.518%
8	7.416	901	906	909	rBV	2045469	1974032	43.25%	6.726%
9	8.139	1025	1029	1032	rBV	1234567	981908	21.51%	3.346%
10	9.216	1207	1212	1216	rBV	3747227	3566644	78.14%	12.153%
11	9.610	1276	1279	1282	rBV	108716	81456	1.78%	0.278%
12	9.898	1322	1328	1332	rBV	1417211	1157077	25.35%	3.943%
13	10.692	1457	1463	1466	rBV	2729883	2636977	57.77%	8.985%
14	11.386	1577	1581	1585	rBV	1343812	1228089	26.90%	4.185%
15	11.927	1665	1673	1684	rBV	1321440	1612276	35.32%	5.494%
16	12.368	1745	1748	1751	rBV	351997	291166	6.38%	0.992%
17	12.427	1754	1758	1762	rBV	69576	66763	1.46%	0.227%
18	12.621	1787	1791	1801	rBV4	85663	144650	3.17%	0.493%
19	12.710	1803	1806	1815	rBV	932524	1101253	24.13%	3.752%
20	12.986	1847	1853	1856	rBV	4845114	4564681	100.00%	15.554%
21	13.910	2004	2010	2027	rBV3	107728	371105	8.13%	1.265%
22	14.039	2027	2032	2035	rVB	1256558	1128931	24.73%	3.847%
23	15.509	2277	2282	2292	rBV	804530	1058121	23.18%	3.605%




Sum of corrected areas: 29347772

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022221\
Data File : BF123261.D
Acq On : 22 Feb 2021 16:30
Operator : JU/CG
Sample : M1452-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

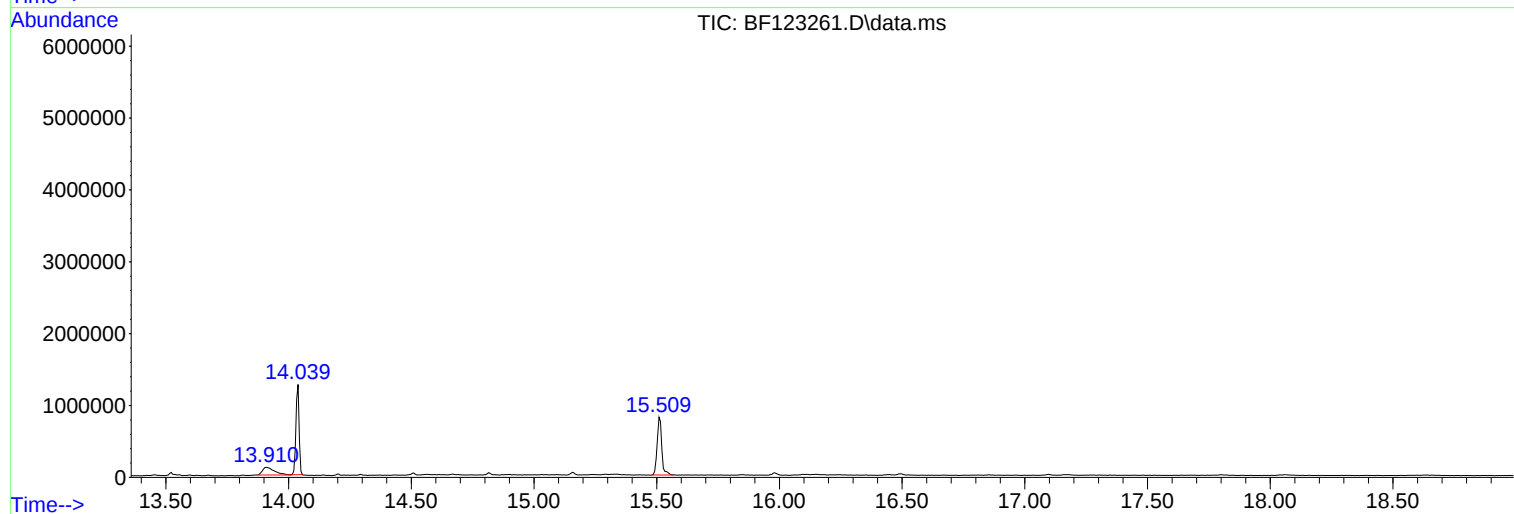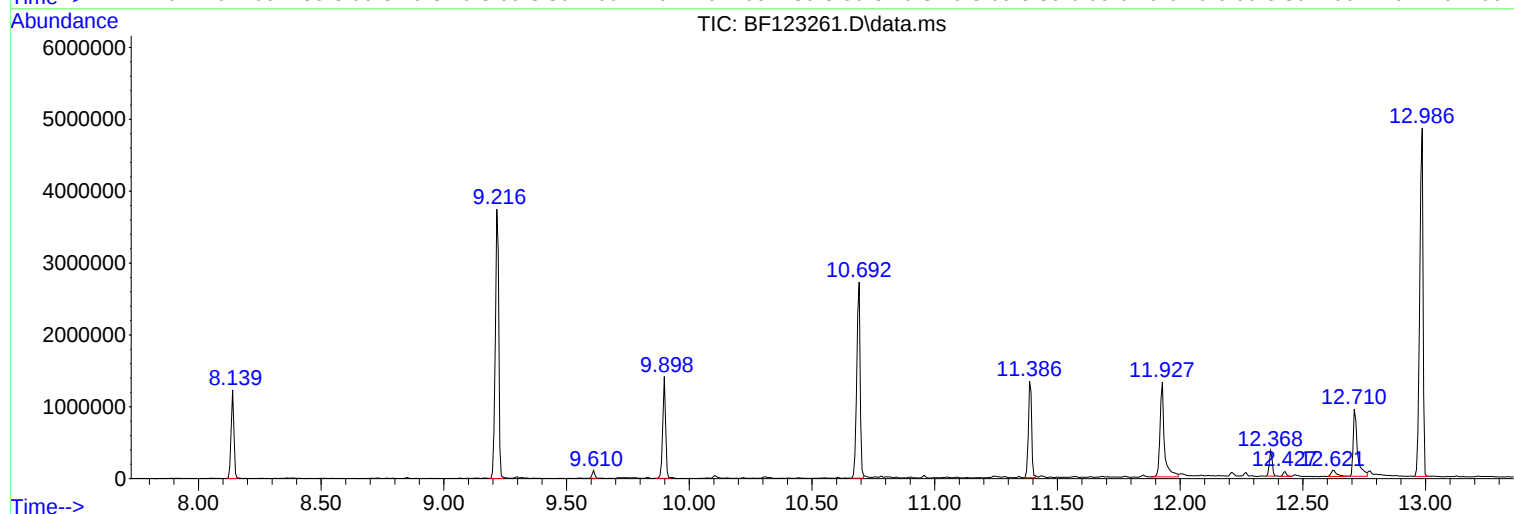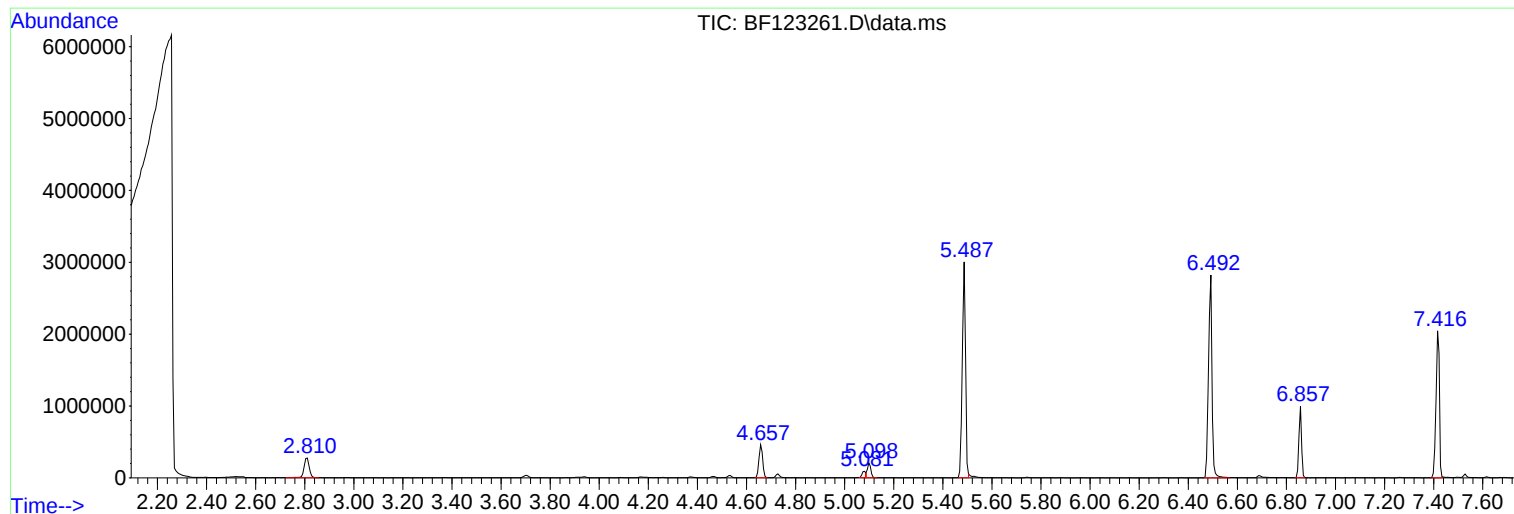

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022221\
Data File : BF123261.D
Acq On : 22 Feb 2021 16:30
Operator : JU/CG
Sample : M1452-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022221\
Data File : BF123261.D
Acq On : 22 Feb 2021 16:30
Operator : JU/CG
Sample : M1452-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------