


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022221\
 Data File : BF123252.D
 Acq On : 22 Feb 2021 10:10
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 19 16:08:53 2021

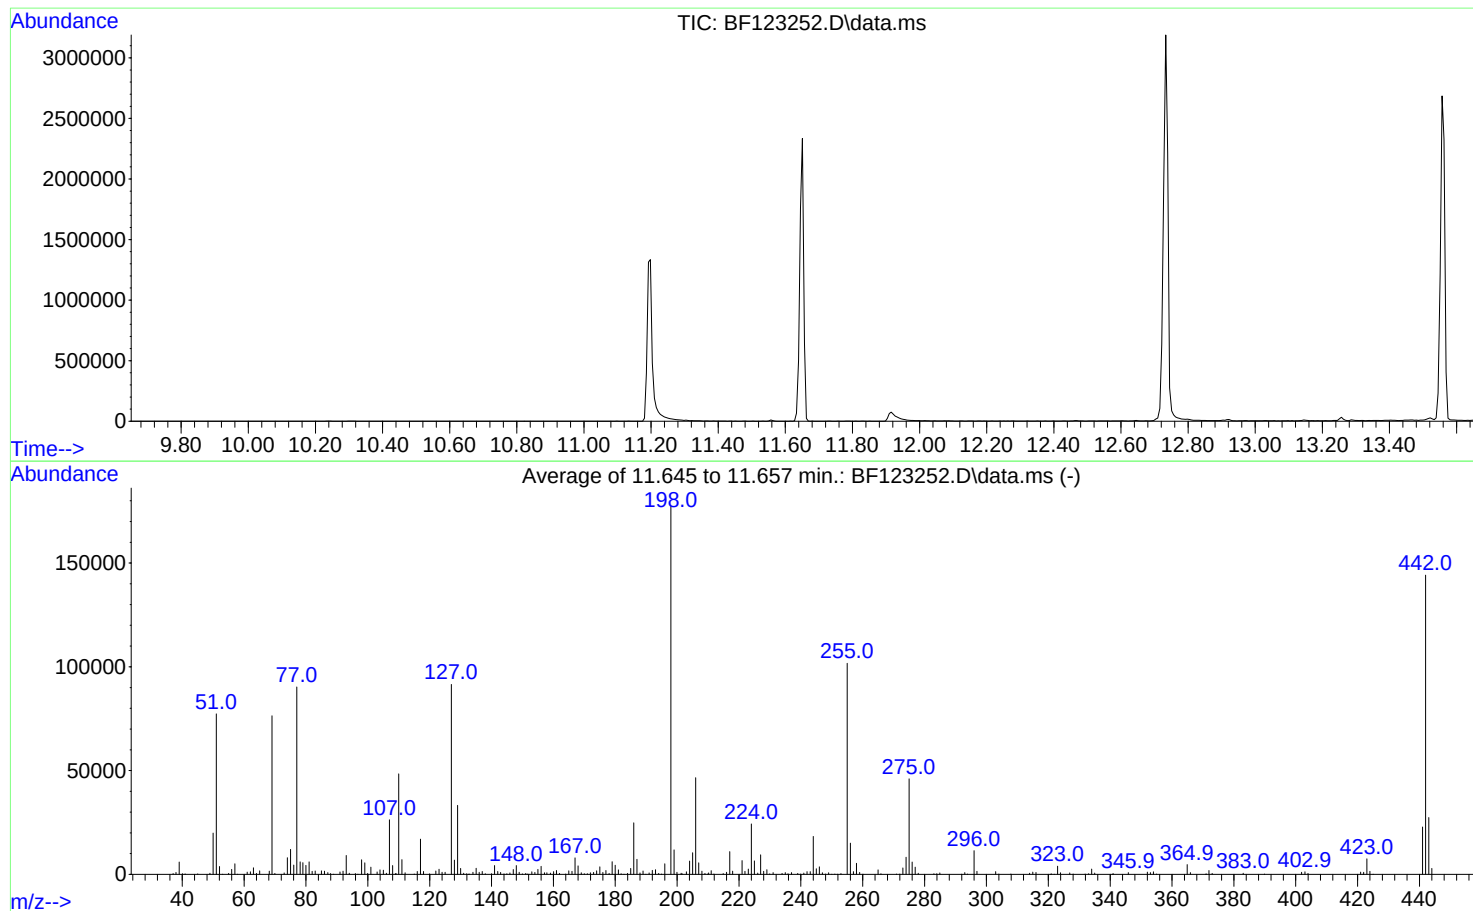




AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.6	77309	PASS
68	69	0.00	2	2.0	1521	PASS
69	198	0.00	100	43.1	76435	PASS
70	69	0.00	2	0.6	440	PASS
127	198	10	80	51.6	91533	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	177243	PASS
199	198	5	9	6.7	11797	PASS
275	198	10	60	26.0	46027	PASS
365	198	1	100	2.7	4697	PASS
441	198	0.01	100	12.9	22831	PASS
442	442	50	100	100.0	144195	PASS
443	442	15	24	19.0	27397	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022221\
Data File : BF123252.D
Acq On : 22 Feb 2021 10:10
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 22 11:30:40 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 19 16:08:53 2021
Response via : Initial Calibration

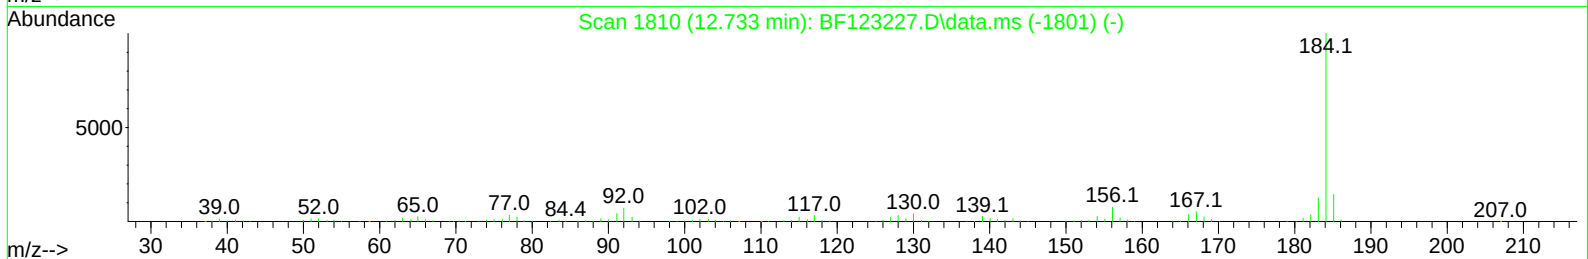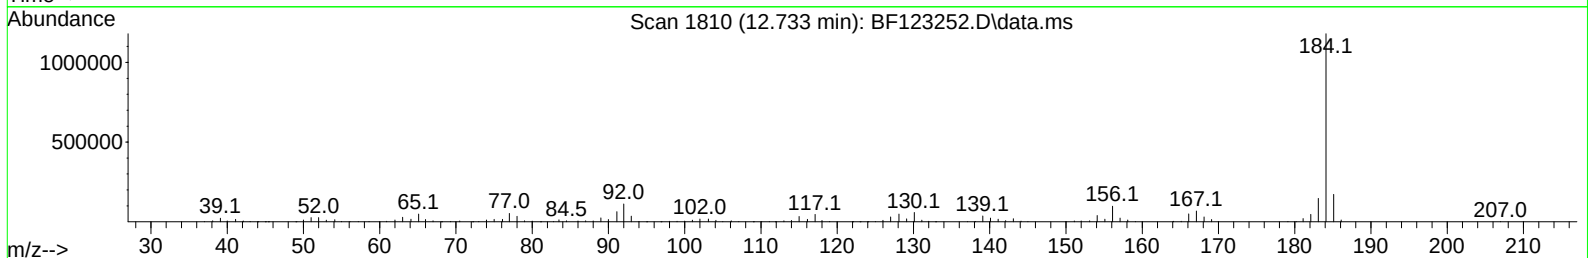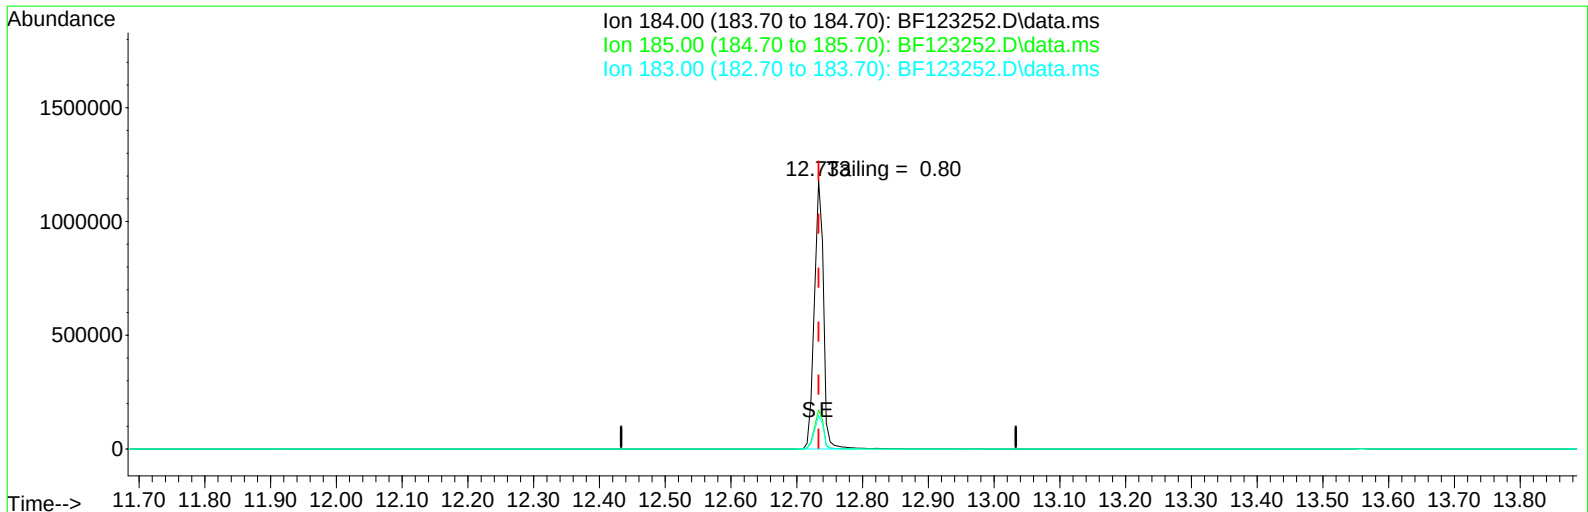

TIC: BF123252.D\data.ms

(77) Benzidine

12.733min (+ 0.000) 0.00 ng




response 1153159

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.55
183.00	12.10	12.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022221\
Data File : BF123252.D
Acq On : 22 Feb 2021 10:10
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 22 11:30:40 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 19 16:08:53 2021
Response via : Initial Calibration

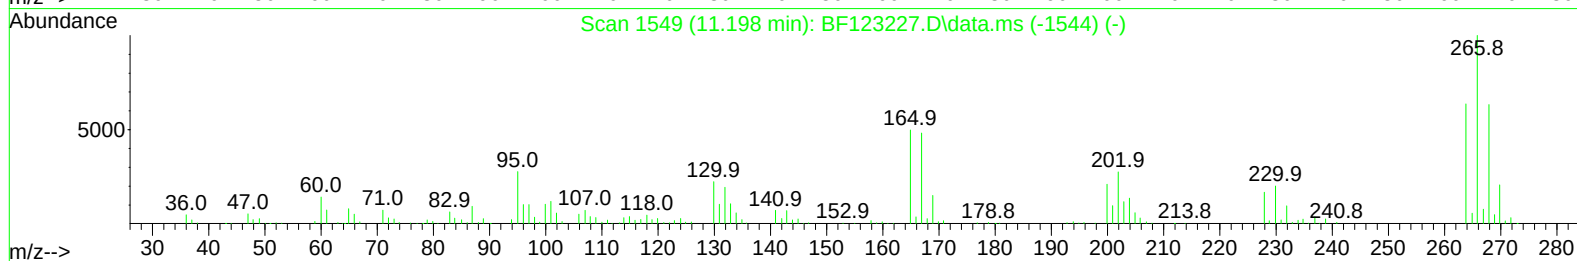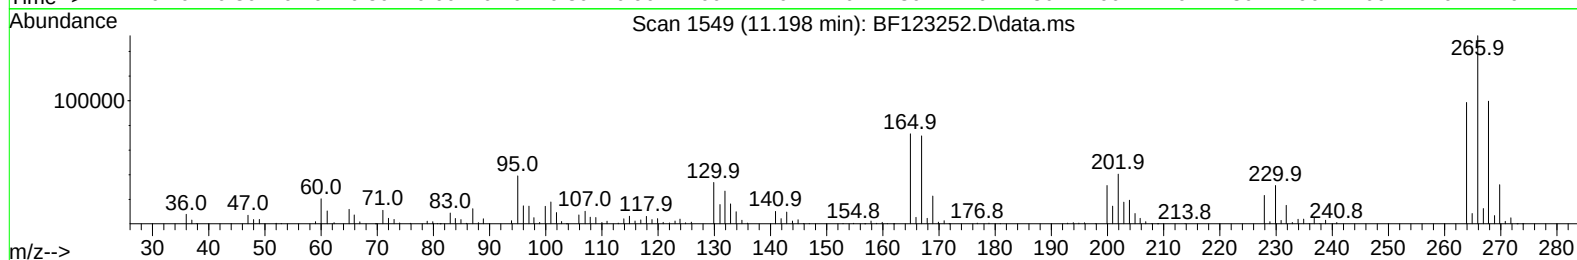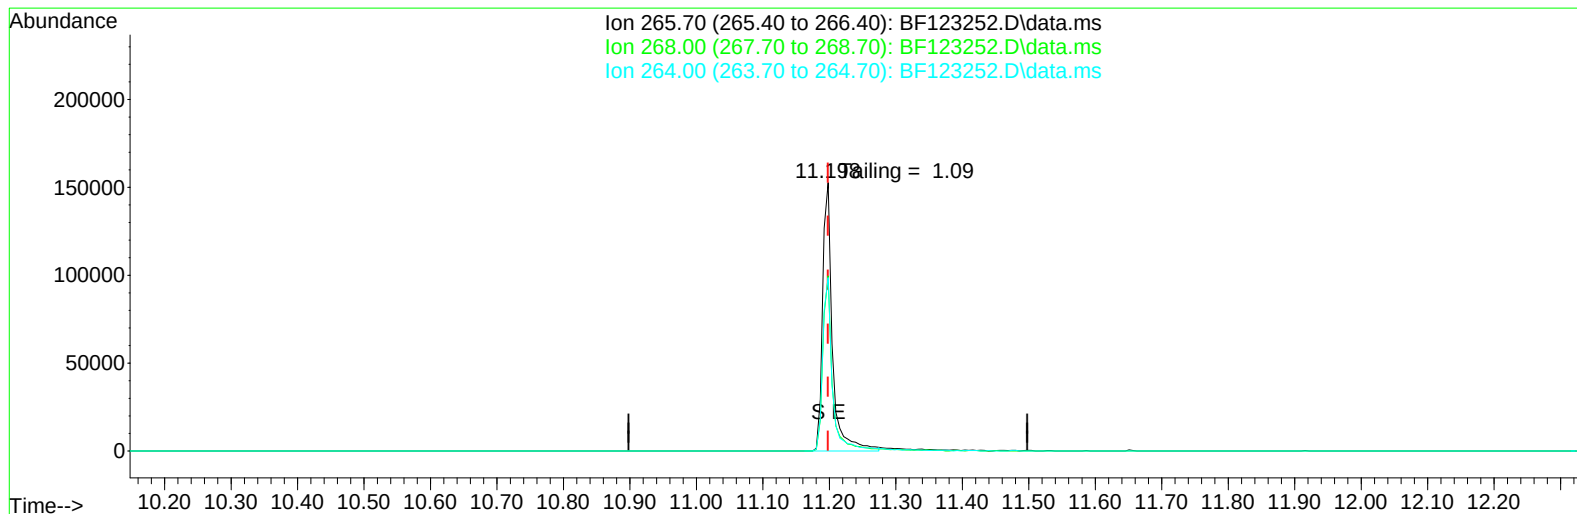

TIC: BF123252.D\data.ms

(70) Pentachlorophenol (C)

11.198min (+ 0.000) 29875.80 ng

response 162482

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	65.26
264.00	62.30	64.61
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
02/22/2021	BNA_F	<u>BF123252.D</u>
Compound Name	Response	Retention Time
DDT	441242	13.55
DDD	5002	13.25
DDE	1605	12.92
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6607	447849	1.48

Instrument :
BNA_F
ClientSampleId :
DFTPP