


Data Path : Z:\HPCHEM1\BNA\_F\Data\BF022315\  
 Data File : BF077395.D  
 Acq On : 23 Feb 2015 10:11  
 Operator : TP/IZ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF021915.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Thu Feb 19 16:57:32 2015

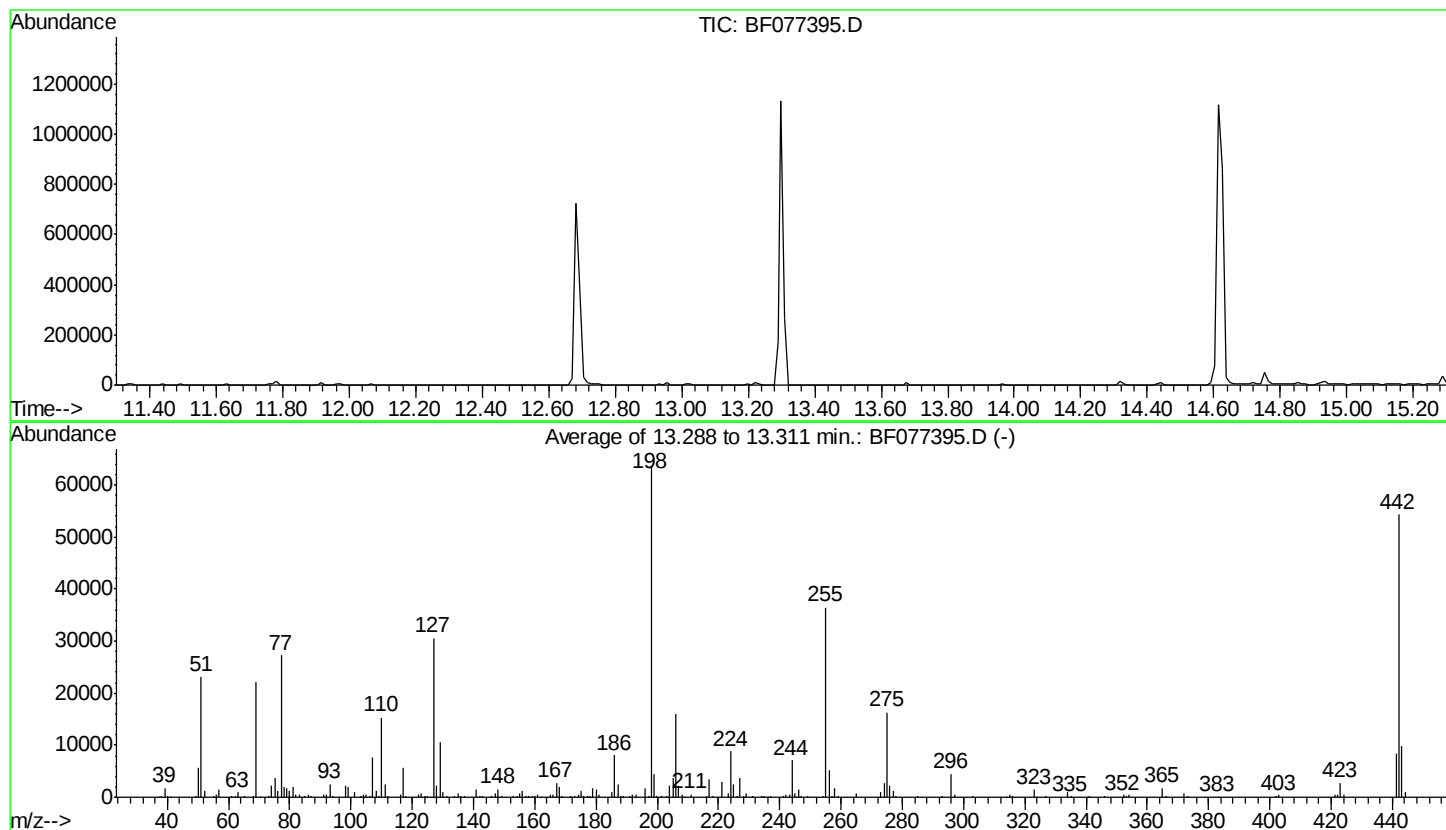

AutoFind: Scans 1085, 1086, 1087; Background Corrected with Scan 1082

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 36.3      | 23154   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.5       | 342     | PASS             |
| 69          | 198          | 0.00         | 100          | 34.8      | 22194   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.5       | 115     | PASS             |
| 127         | 198          | 10           | 80           | 47.9      | 30518   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.5       | 324     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 63712   | PASS             |
| 199         | 198          | 5            | 9            | 6.9       | 4398    | PASS             |
| 275         | 198          | 10           | 60           | 25.7      | 16356   | PASS             |
| 365         | 198          | 1            | 100          | 2.7       | 1750    | PASS             |
| 441         | 442          | 0.01         | 24           | 15.3      | 8315    | PASS             |
| 442         | 198          | 50           | 100          | 85.2      | 54256   | PASS             |
| 443         | 442          | 15           | 24           | 18.2      | 9853    | PASS             |