


Data Path : Z:\HPCHEM1\BNA F\Data\BF022315\
 Data File : BF077395.D
 Acq On : 23 Feb 2015 10:11
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Feb 19 16:57:32 2015

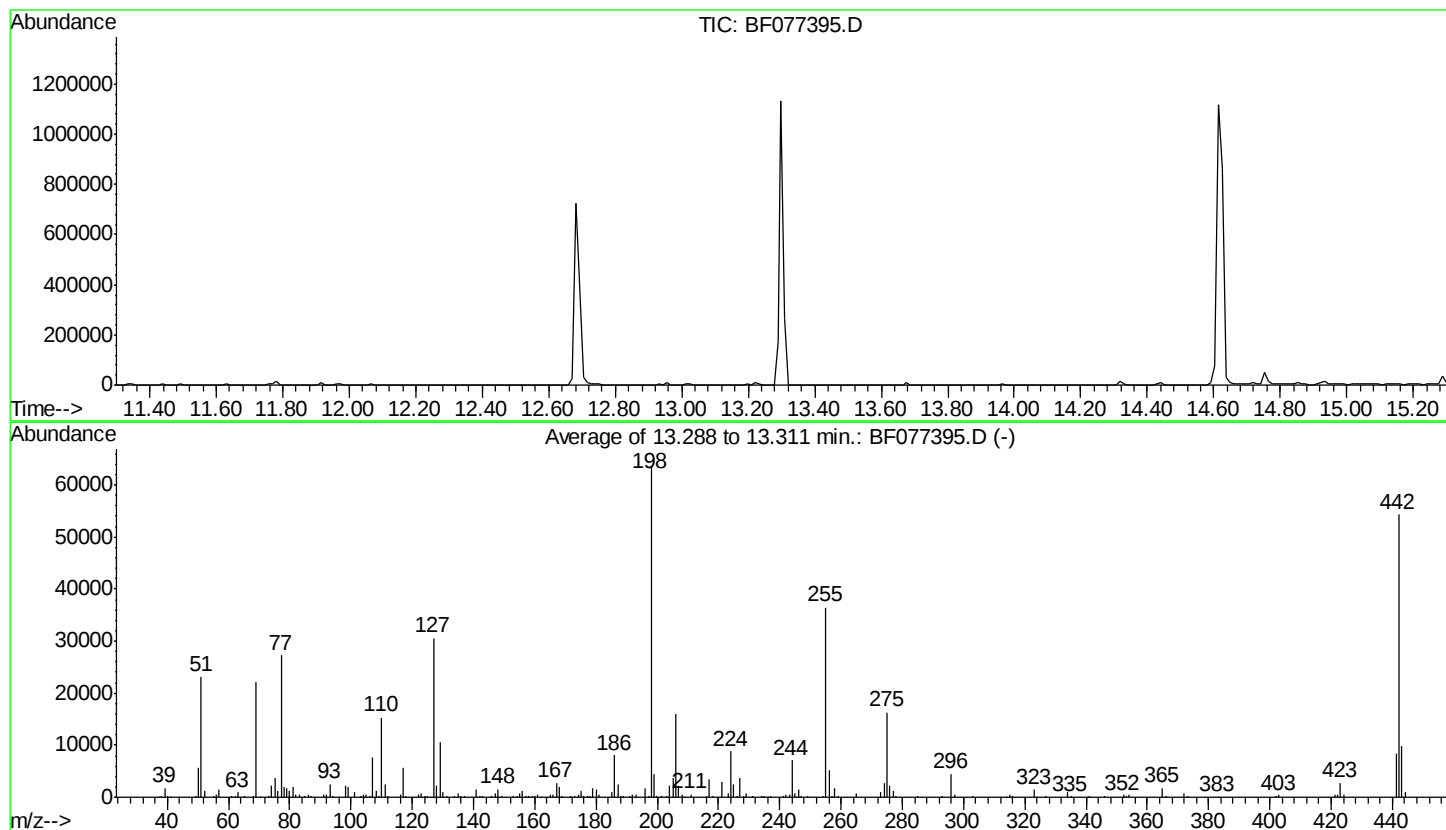

AutoFind: Scans 1085, 1086, 1087; Background Corrected with Scan 1082

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.3	23154	PASS
68	69	0.00	2	1.5	342	PASS
69	198	0.00	100	34.8	22194	PASS
70	69	0.00	2	0.5	115	PASS
127	198	10	80	47.9	30518	PASS
197	198	0.00	2	0.5	324	PASS
198	198	100	100	100.0	63712	PASS
199	198	5	9	6.9	4398	PASS
275	198	10	60	25.7	16356	PASS
365	198	1	100	2.7	1750	PASS
441	442	0.01	24	15.3	8315	PASS
442	198	50	100	85.2	54256	PASS
443	442	15	24	18.2	9853	PASS