
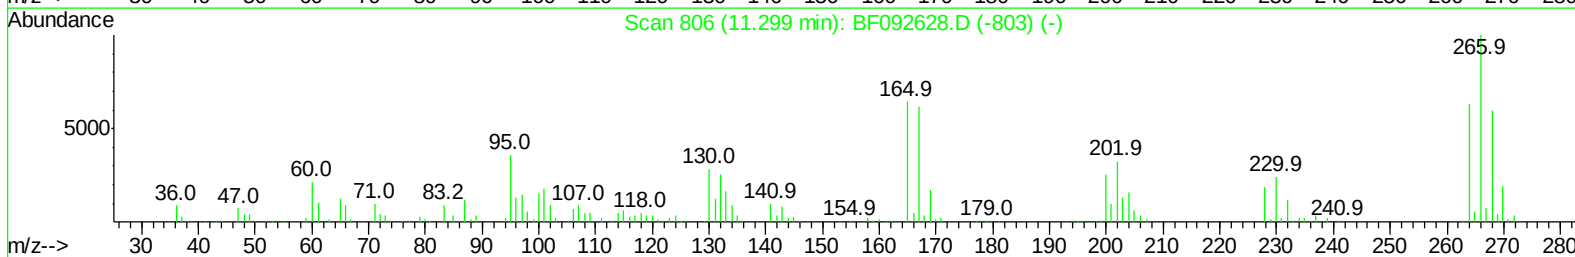
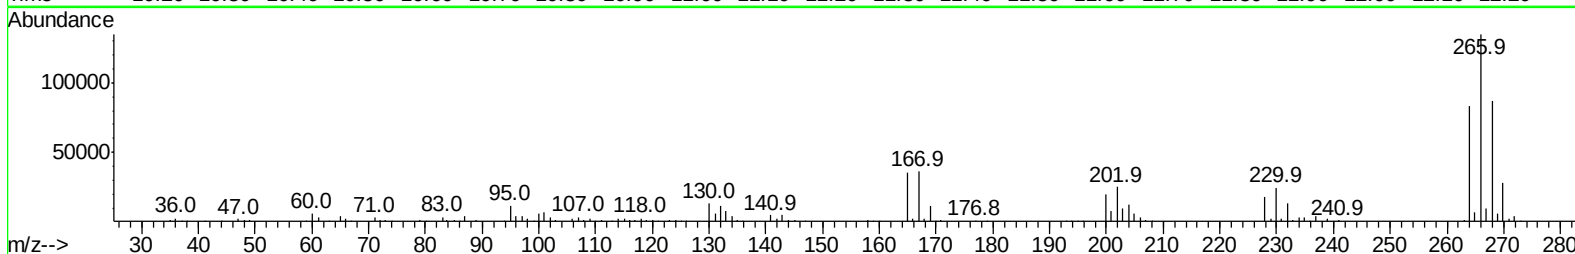


Data Path : Z:\HPCHEM1\BNA F\Data\BF022317\
Data File : BF093097.D
Acq On : 23 Feb 2017 9:16
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 23 15:38:28 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 17:31:55 2017
Response via : Initial Calibration

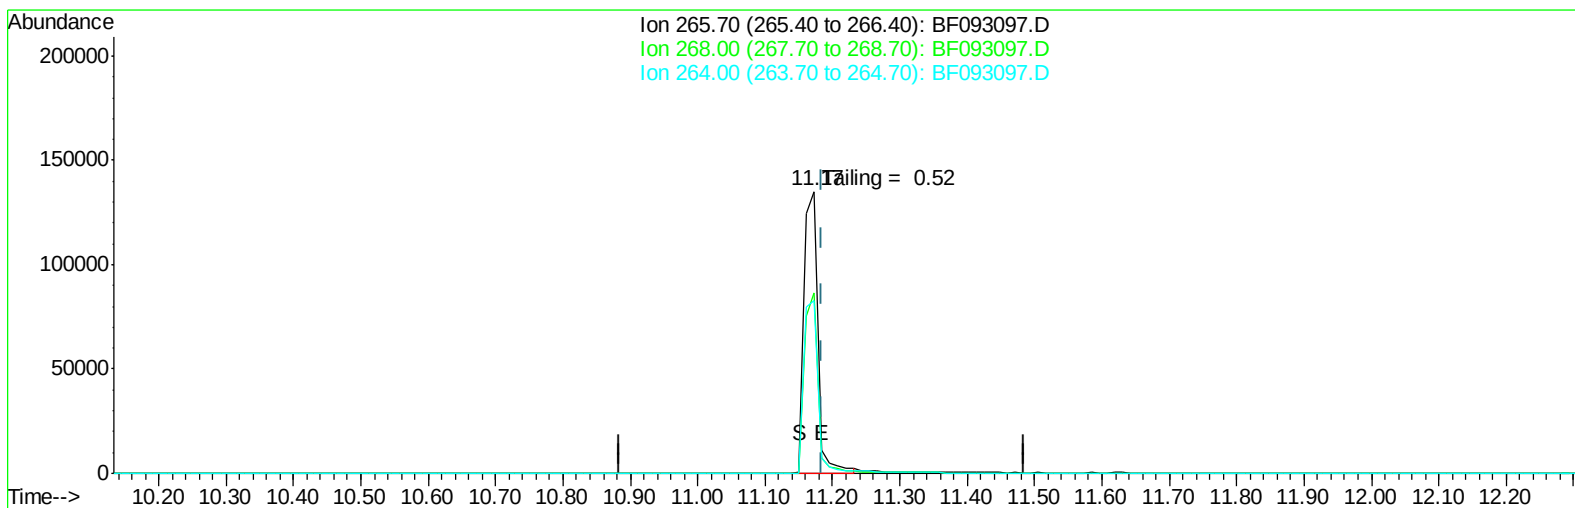

TIC: BF093097.D

(69) Pentachlorophenol (C)




11.173min (-0.012) 29108.64ng

response 199081

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	64.21
264.00	62.90	61.42
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF022317\
Data File : BF093097.D
Acq On : 23 Feb 2017 9:16
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 23 15:38:28 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 17:31:55 2017
Response via : Initial Calibration

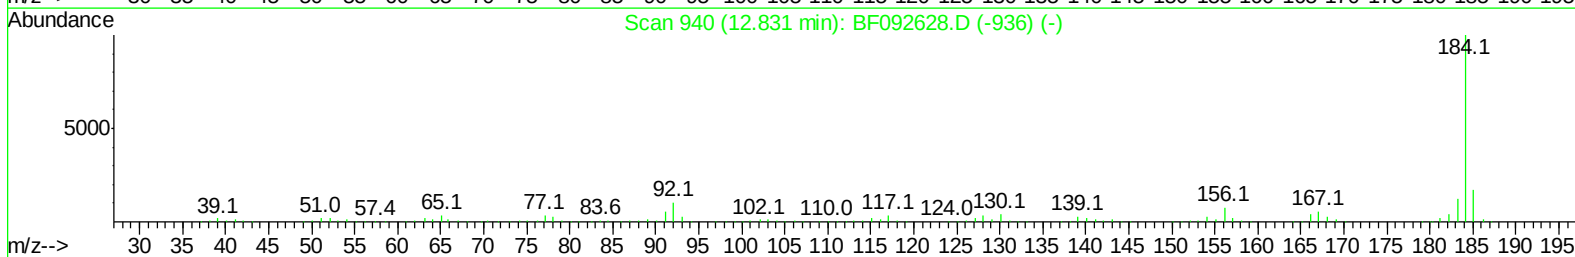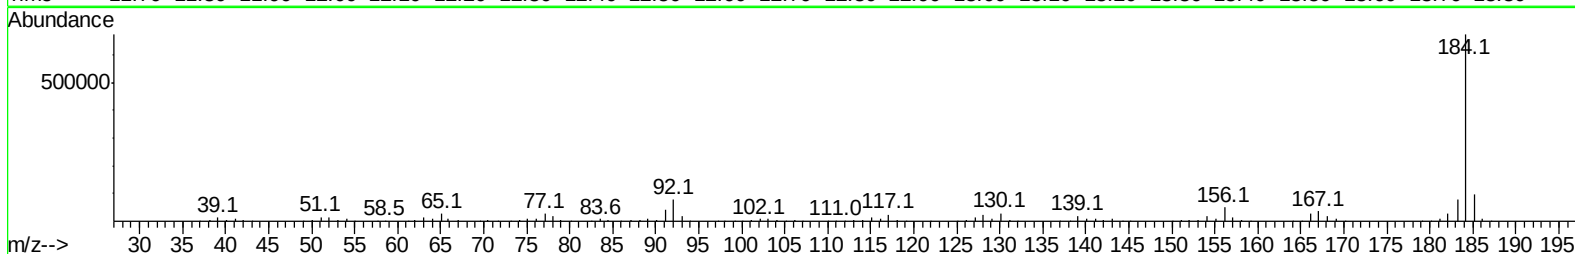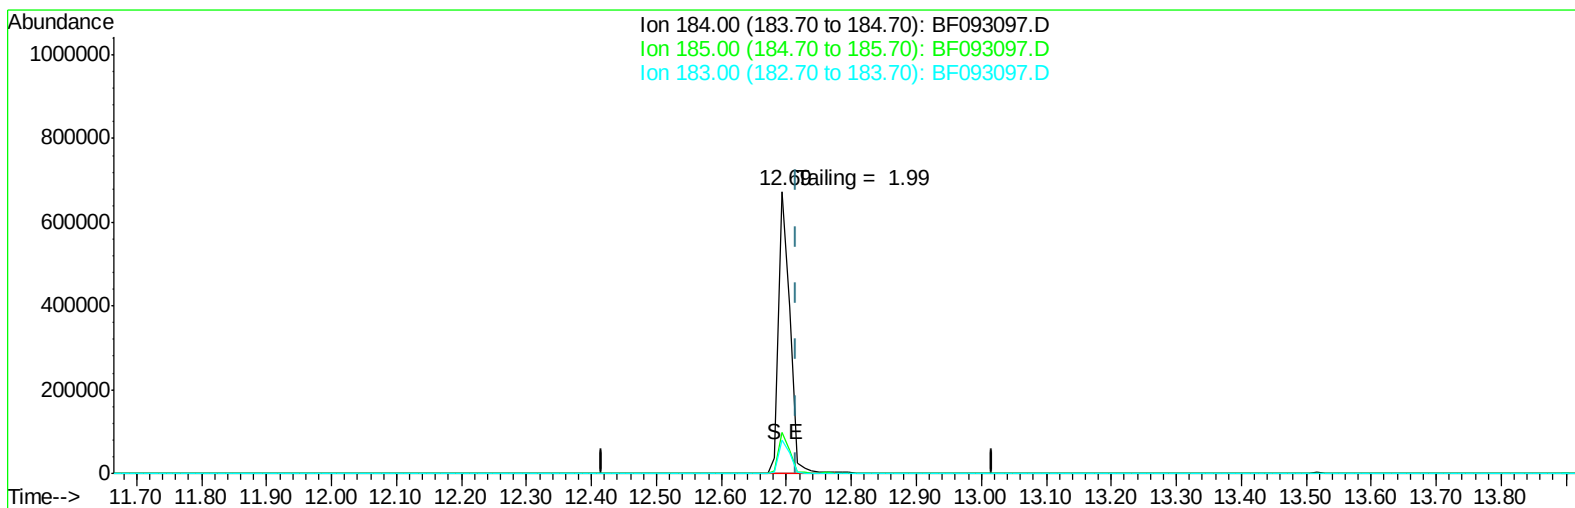

TIC: BF093097.D

(76) Benzidine

12.694min (-0.023) 5082.11ng

response 807562

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.60
183.00	11.50	11.86
0.00	0.00	0.00