

Data File : BF093103.D

Acq On : 23 Feb 2017 14:33

Operator : SJ/MA

Sample : DFTPP

Misc :

ALS Vial : 1 Sample Multiplier: 1




Quant Time: Feb 24 03:12:39 2017

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Feb 17 17:31:55 2017

Response via : Initial Calibration

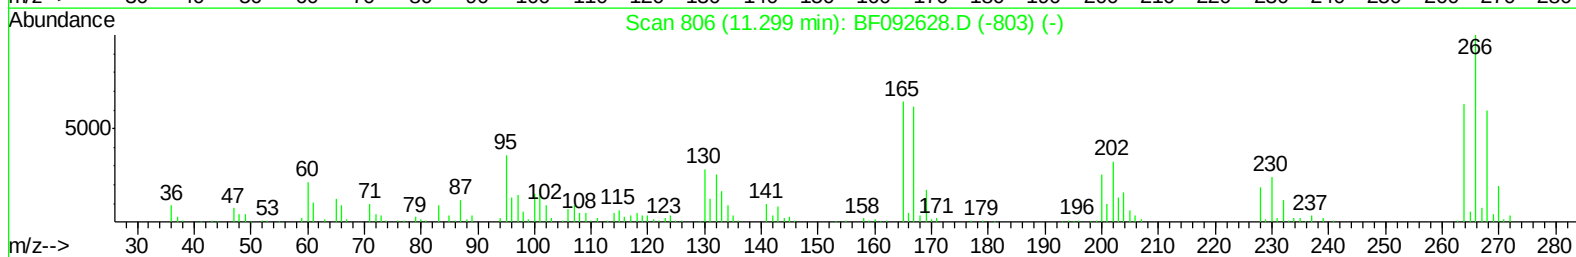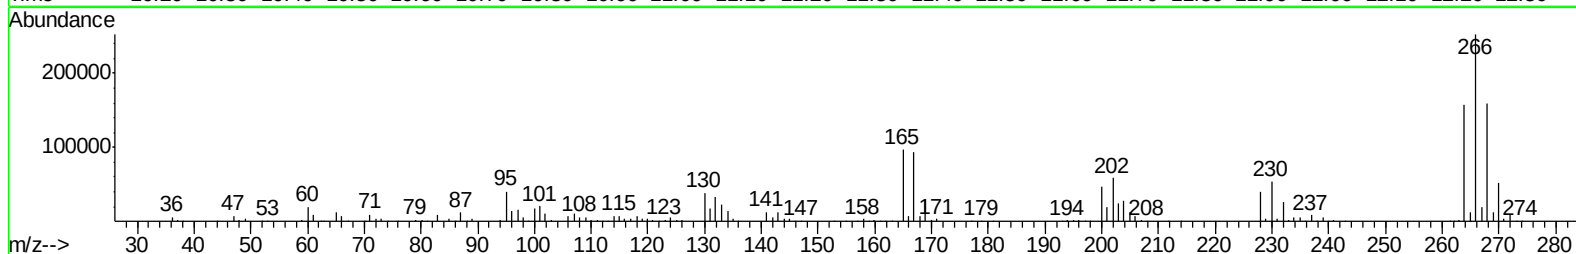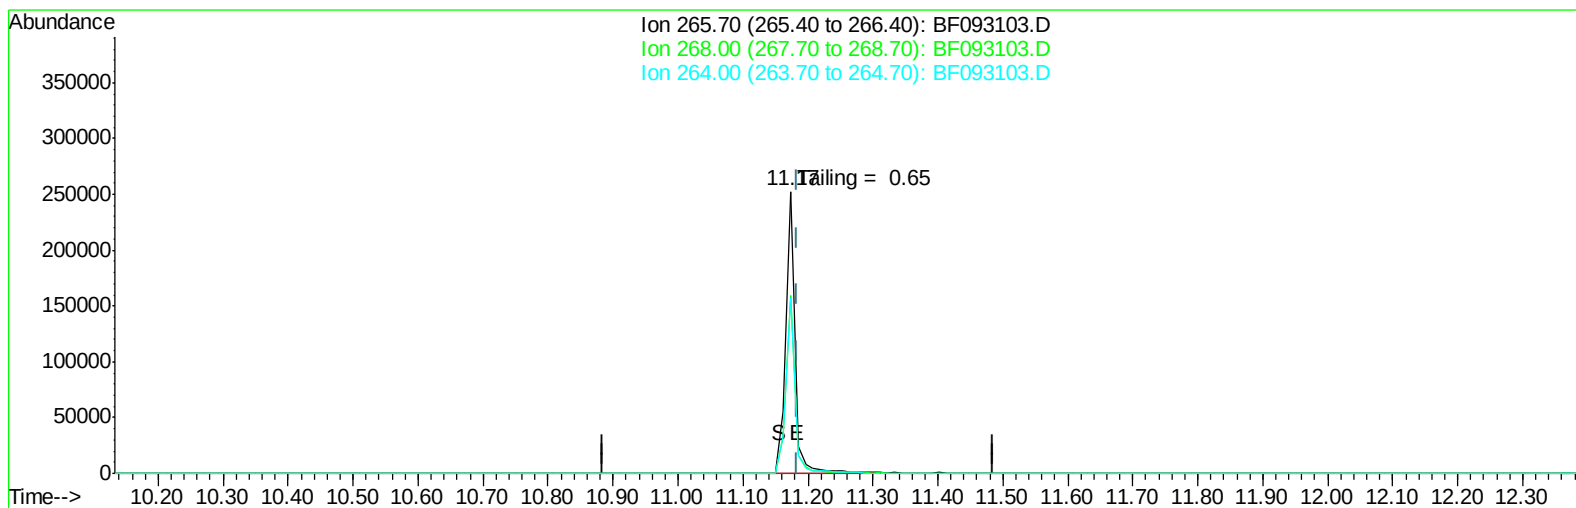

TIC: BF093103.D

(69) Pentachlorophenol (C)




11.173min (-0.012) 50870.01ng

response 248450

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	63.37
264.00	62.90	62.23
0.00	0.00	0.00

Data File : BF093103.D
Acq On : 23 Feb 2017 14:33
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 24 03:12:39 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 17:31:55 2017
Response via : Initial Calibration

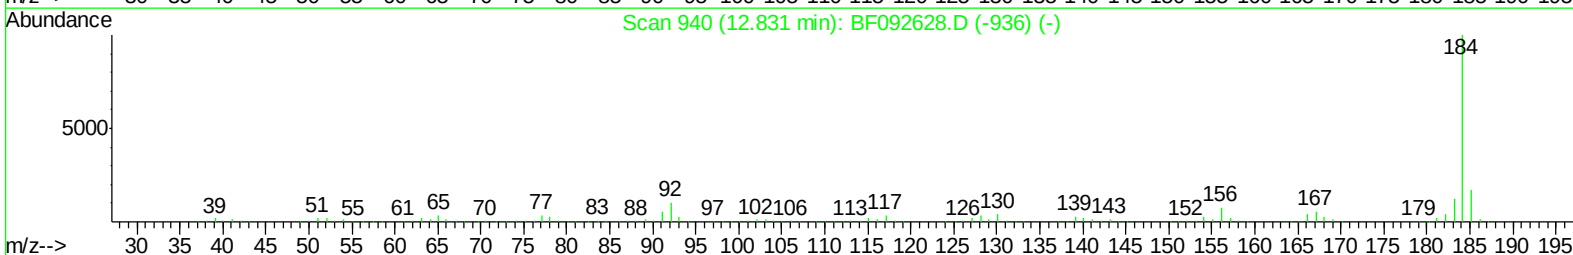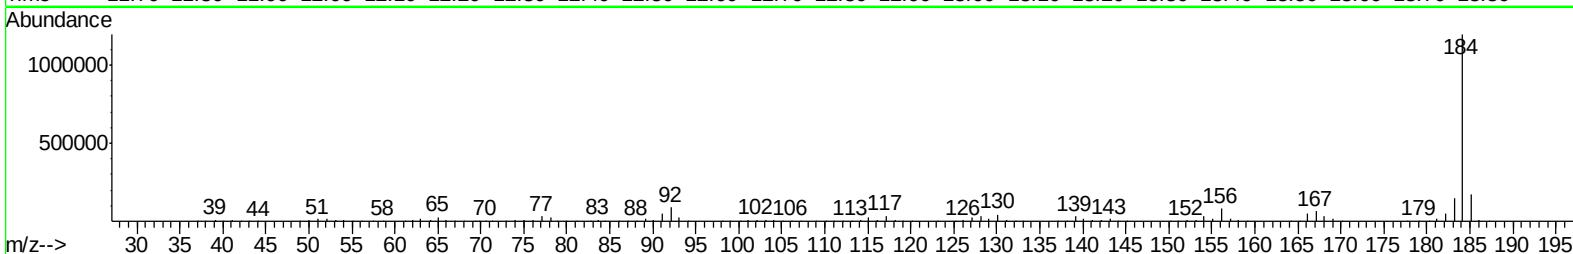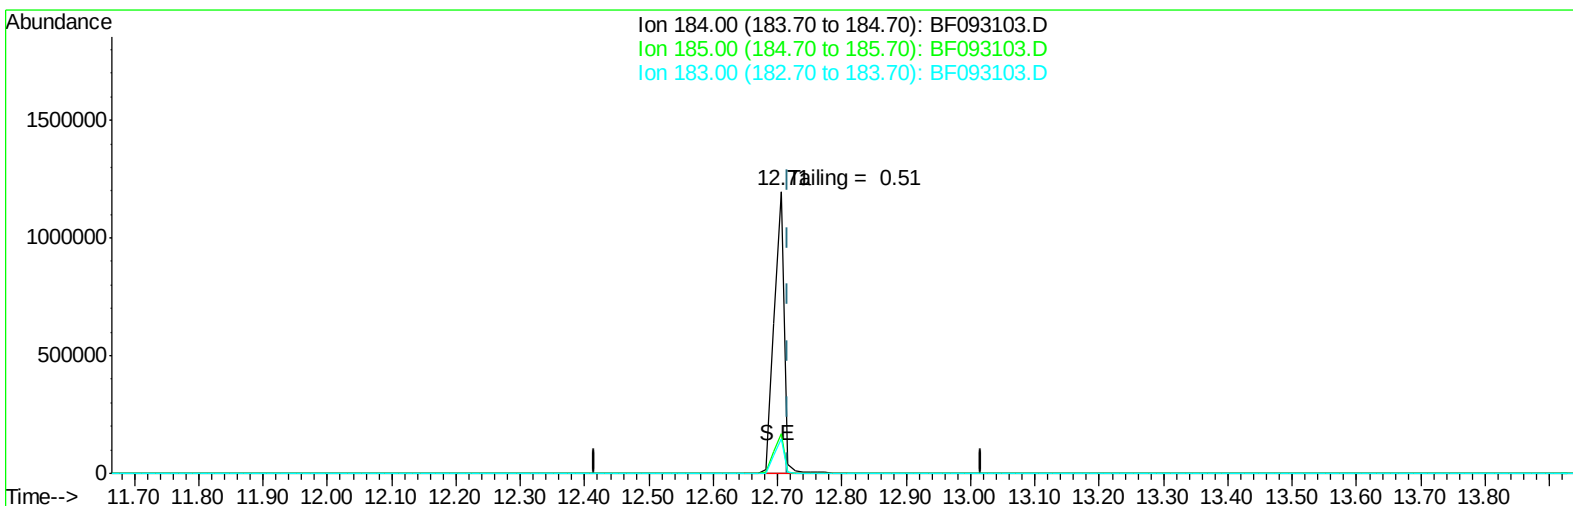

TIC: BF093103.D

(76) Benzidine

12.705min (-0.012) 8430.84ng

response 1332858

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.22
183.00	11.50	12.26
0.00	0.00	0.00