

Data Path : Z:\HPCHEM1\BNA F\DATA\BF022317\
 Data File : BF093117.D
 Acq On : 23 Feb 2017 21:13
 Operator : SJ/MA
 Sample : I1954-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CLP-S-04(5-10)

Quant Time: Feb 24 00:24:39 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF013017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 17 17:31:55 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.84	152	154886	20.00	ng	-0.01
21) Naphthalene-d8	8.12	136	652542	20.00	ng	-0.02
38) Acenaphthene-d10	9.87	164	301691	20.00	ng	-0.02
63) Phenanthrene-d10	11.36	188	584798	20.00	ng	-0.02
75) Chrysene-d12	14.00	240	512486	20.00	ng	-0.02
86) Perylene-d12	15.41	264	368360	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.44	112	1076062	119.19	ng	-0.01
7) Phenol-d6	6.48	99	1308555	112.65	ng	-0.01
23) Nitrobenzene-d5	7.40	82	821910	70.14	ng	-0.02
41) 2,4,6-Tribromophenol	10.67	330	296637	135.95	ng	-0.01
44) 2-Fluorobiphenyl	9.20	172	1436909	86.29	ng	-0.02
78) Terphenyl-d14	12.94	244	1281291	58.75	ng	-0.02
Target Compounds						
10) Phenol	6.49	94	60486	4.45	ng	97
49) Dimethylphthalate	9.60	163	159844	7.87	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF022317\
Data File : BF093117.D
Acq On : 23 Feb 2017 21:13
Operator : SJ/MA
Sample : I1954-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CLP-S-04(5-10)

Quant Time: Feb 24 00:24:39 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 17:31:55 2017
Response via : Initial Calibration

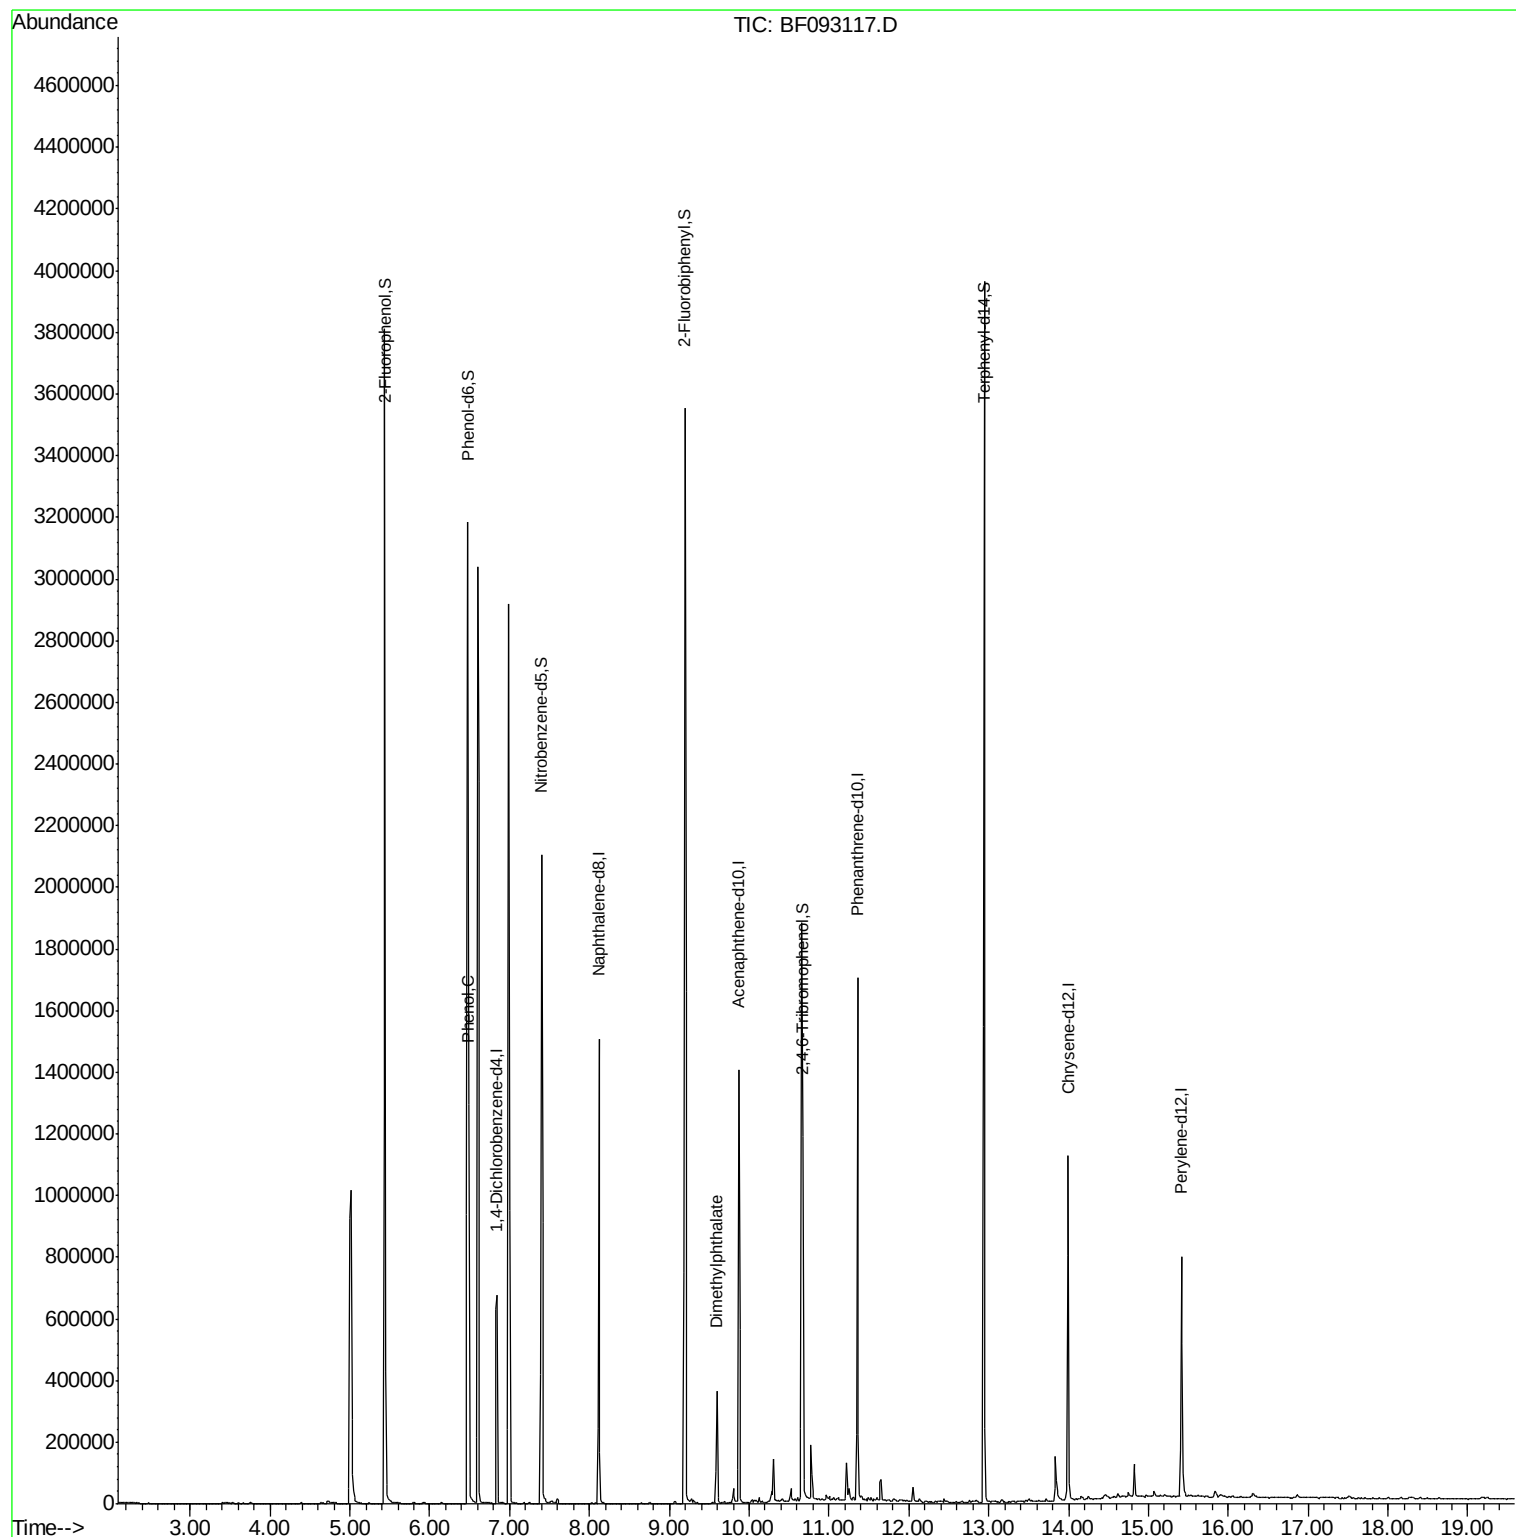

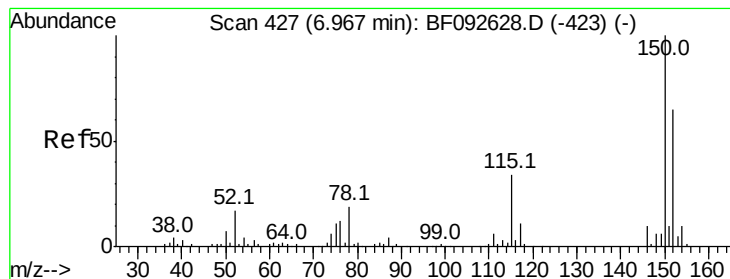

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.84 min Scan# 416

Delta R.T. -0.01 min

Lab File: BF093117.D

Acq: 23 Feb 2017 21:13

Instrument :

BNA_F

ClientSampleId :

CLP-S-04(5-10)


Tot Ion:152 Resp: 154886

Ion Ratio Lower Upper

152 100

150 151.6 124.9 187.3




115 50.9 46.0 69.0

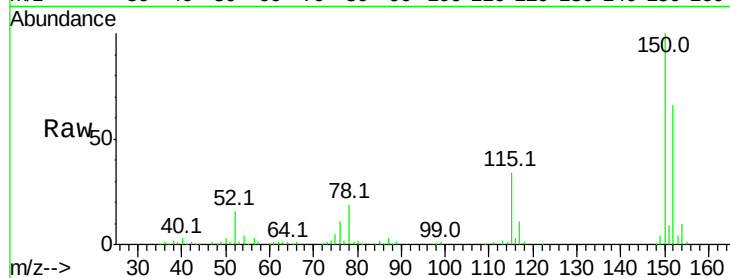

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

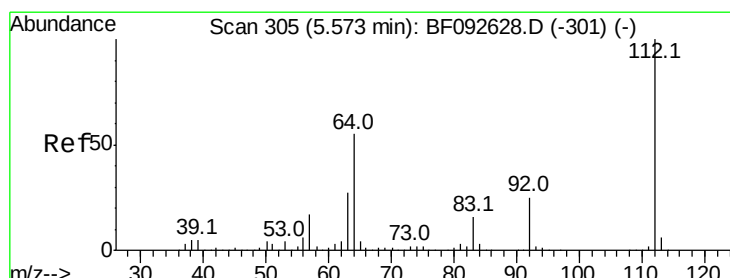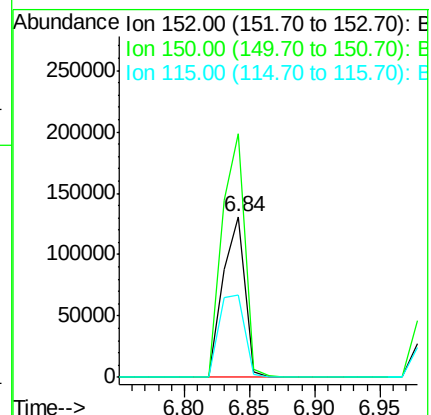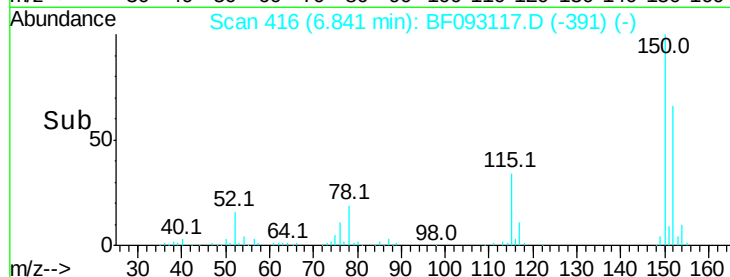

#5

2-Fluorophenol

Concen: 119.19 ng

RT: 5.44 min Scan# 293

Delta R.T. -0.01 min

Lab File: BF093117.D

Acq: 23 Feb 2017 21:13


Tgt Ion:112 Resp: 1076062

Ion Ratio Lower Upper

112 100

64 65.0 46.1 69.1



63 32.5 23.8 35.6

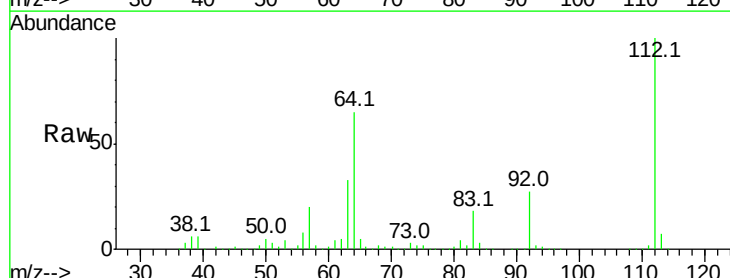


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

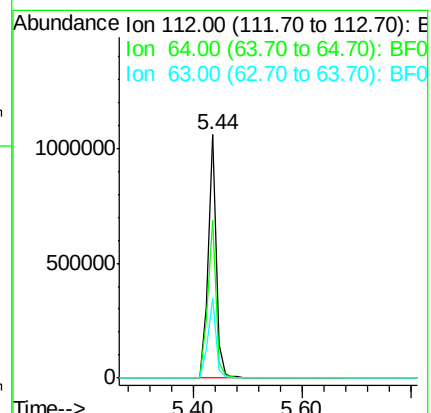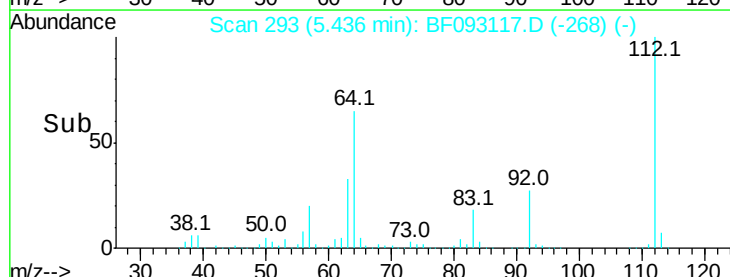

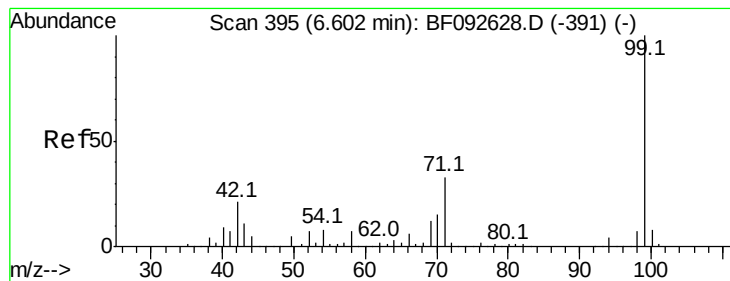

#7

Phenol-d6

Concen: 112.65 ng

RT: 6.48 min Scan# 384

Delta R.T. -0.01 min

Lab File: BF093117.D

Acq: 23 Feb 2017 21:13

Instrument :

BNA_F

ClientSampleId :

CLP-S-04(5-10)


Tot Ion: 99 Resp: 1308555

Ion Ratio Lower Upper

99 100

42 20.3 15.6 23.4




71 33.0 27.5 41.3

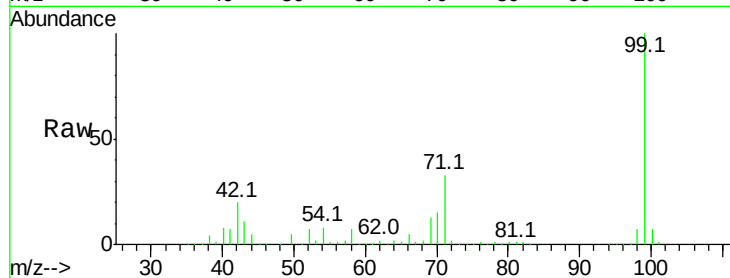

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

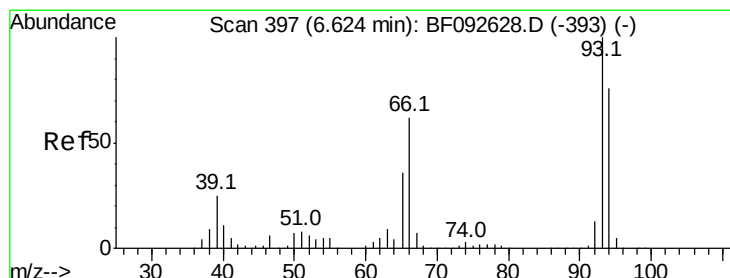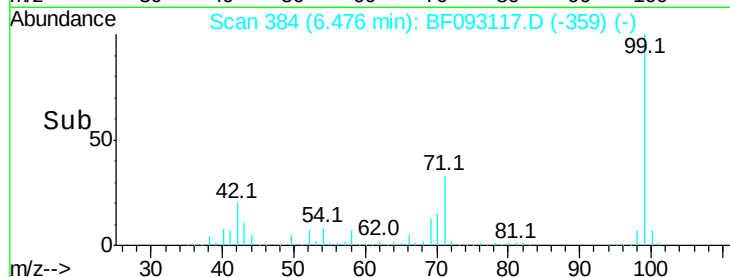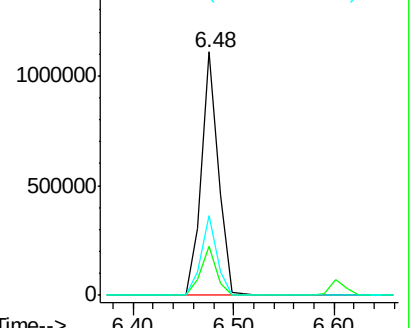

#10

Phenol

Concen: 4.45 ng

RT: 6.49 min Scan# 385

Delta R.T. -0.02 min

Lab File: BF093117.D

Acq: 23 Feb 2017 21:13


Tgt Ion: 94 Resp: 60486

Ion Ratio Lower Upper

94 100

65 36.5 21.4 61.4



66 63.9 44.0 84.0

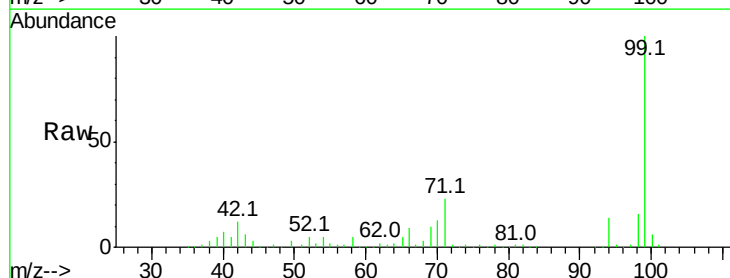


Abundance Ion 94.00 (93.70 to 94.70): BF0

Ion 65.00 (64.70 to 65.70): BF0

Ion 66.00 (65.70 to 66.70): BF0

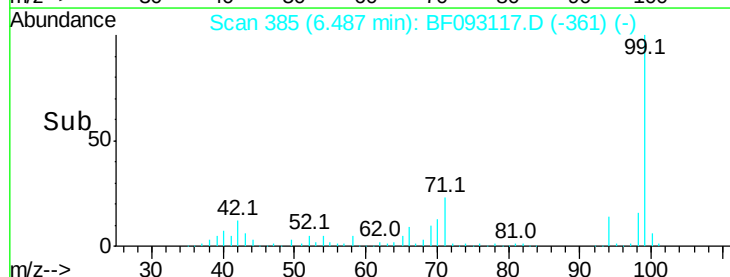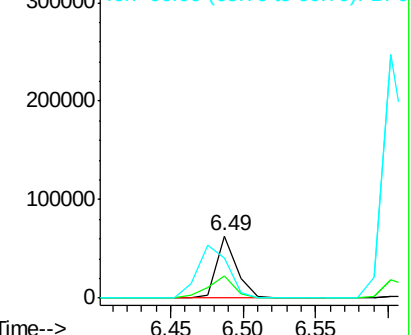


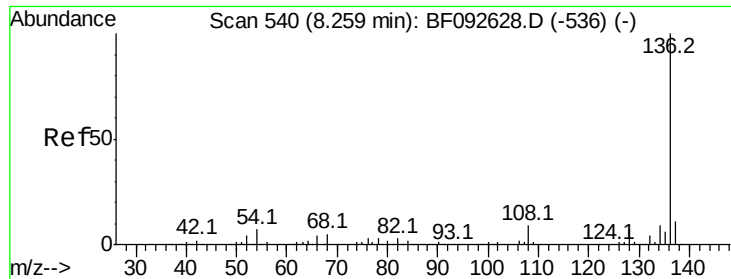




#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.12 min Scan# 528
Delta R.T. -0.02 min
Lab File: BF093117.D
Acq: 23 Feb 2017 21:13

Instrument :
BNA_F
ClientSampleId :
CLP-S-04(5-10)

Tot Ion:	136	Resp:	652542
Ion	Ratio	Lower	Upper
136	100		
137	11.0	8.4	12.6
54	10.0	4.5	6.7#
68	7.2	3.6	5.4#




Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0

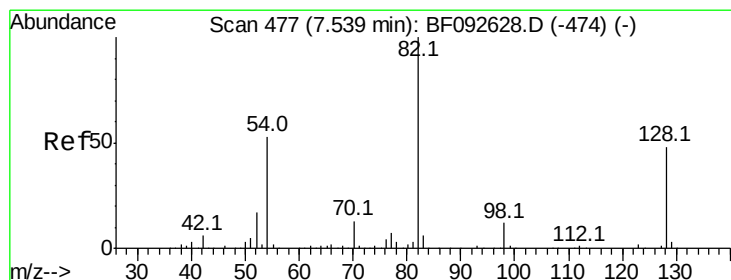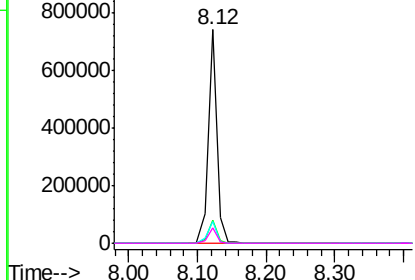




#23
Nitrobenzene-d5
Concen: 70.14 ng
RT: 7.40 min Scan# 465
Delta R.T. -0.02 min
Lab File: BF093117.D
Acq: 23 Feb 2017 21:13

Tgt Ion:	82	Resp:	821910
Ion	Ratio	Lower	Upper
82	100		
128	40.7	34.6	52.0
54	57.9	39.5	59.3



Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0

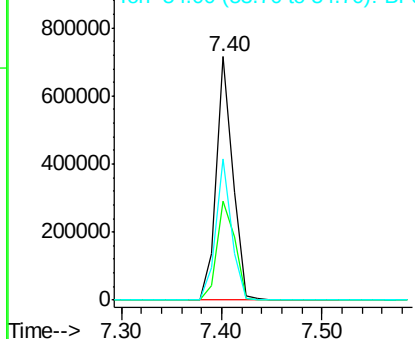







#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.87 min Scan# 681
Delta R.T. -0.02 min
Lab File: BF093117.D
Acq: 23 Feb 2017 21:13

Instrument :
BNA_F
ClientSampleId :
CLP-S-04(5-10)

Tot Ion:164 Resp: 301691
Ion Ratio Lower Upper
164 100
162 103.7 80.2 120.2
160 44.6 36.9 55.3

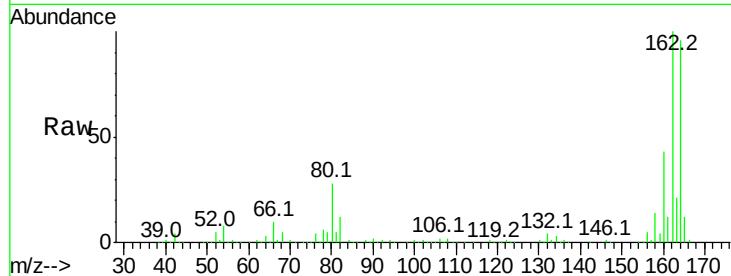


Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

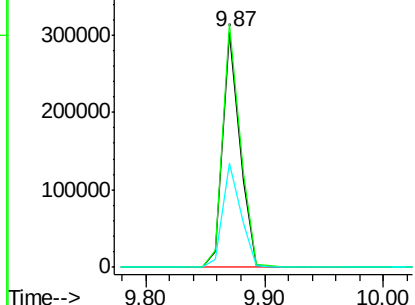
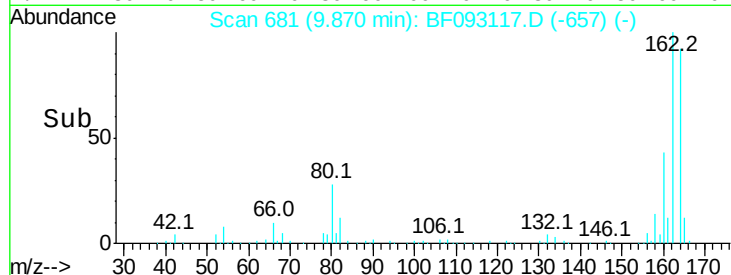



#41
2,4,6-Tribromophenol
Concen: 135.95 ng
RT: 10.67 min Scan# 751
Delta R.T. -0.01 min
Lab File: BF093117.D
Acq: 23 Feb 2017 21:13

Tgt Ion:330 Resp: 296637
Ion Ratio Lower Upper
330 100
332 96.6 77.4 116.2
141 32.5 34.1 51.1#



Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

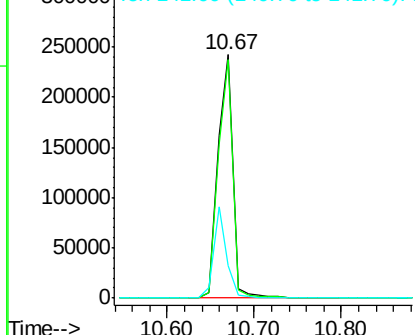




#44
 2-Fluorobiphenyl
 Concen: 86.29 ng
 RT: 9.20 min Scan# 622
 Delta R.T. -0.02 min
 Lab File: BF093117.D
 Acq: 23 Feb 2017 21:13




Instrument :
 BNA_F
 ClientSampleId :
 CLP-S-04(5-10)

Tot Ion:172 Resp: 1436909

Ion	Ratio	Lower	Upper
172	100		
171	36.5	29.4	44.0
170	24.9	20.2	30.4




Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

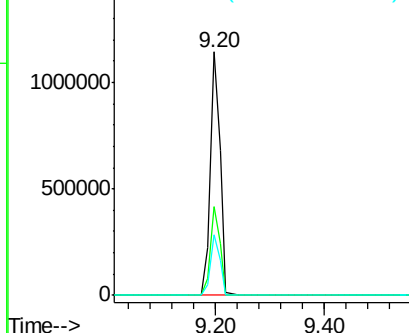



#49
 Dimethylphthalate
 Concen: 7.87 ng
 RT: 9.60 min Scan# 657
 Delta R.T. -0.02 min
 Lab File: BF093117.D
 Acq: 23 Feb 2017 21:13


Tgt Ion:163 Resp: 159844

Ion	Ratio	Lower	Upper
163	100		
194	3.6	3.0	4.4
164	9.5	8.0	12.0



Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

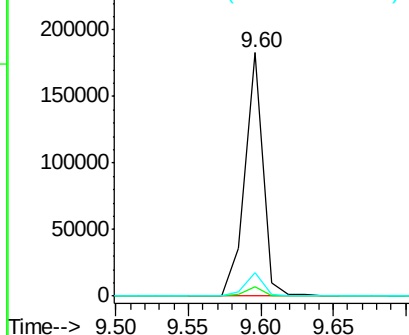







#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.36 min Scan# 811
Delta R.T. -0.02 min
Lab File: BF093117.D
Acq: 23 Feb 2017 21:13

Instrument :
BNA_F
ClientSampleId :
CLP-S-04(5-10)

Tot Ion:188 Resp: 584798
Ion Ratio Lower Upper
188 100
94 11.4 10.0 15.0
80 12.0 11.2 16.8

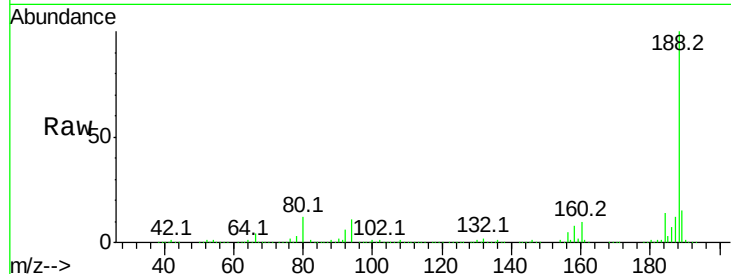


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

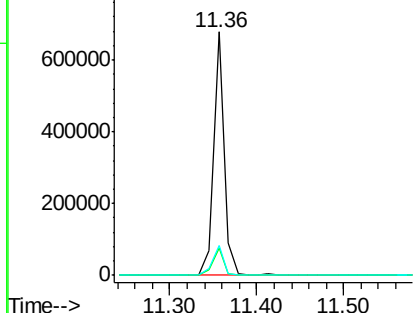




#75
Chrysene-d12
Concen: 20.00 ng
RT: 14.00 min Scan# 1042
Delta R.T. -0.02 min
Lab File: BF093117.D
Acq: 23 Feb 2017 21:13

Tgt Ion:240 Resp: 512486
Ion Ratio Lower Upper
240 100
120 9.4 12.9 19.3#
236 25.3 20.9 31.3



Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

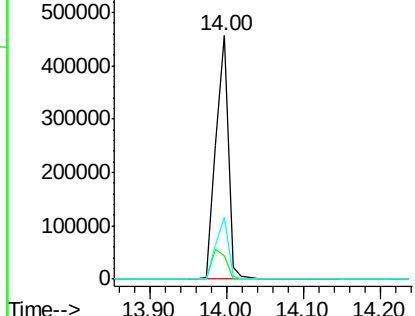



#78

Terphenyl-d14

Concen: 58.75 ng

RT: 12.94 min Scan# 950

Delta R.T. -0.02 min

Lab File: BF093117.D

Acq: 23 Feb 2017 21:13

Instrument :

BNA_F

ClientSampleId :

CLP-S-04(5-10)


Tot Ion:244 Resp: 1281291

Ion Ratio Lower Upper

244 100

212 7.6 6.2 9.2




122 12.8 11.4 17.2



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

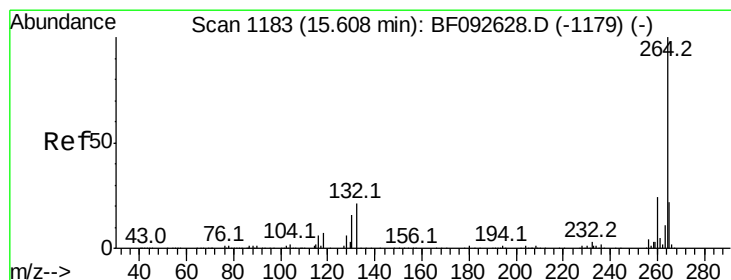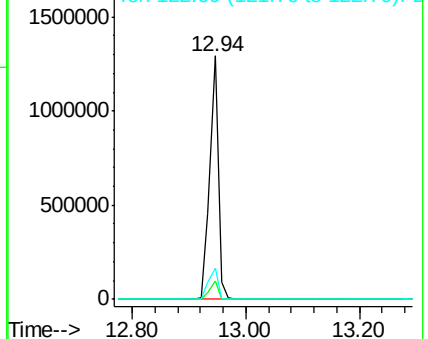

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.41 min Scan# 1166

Delta R.T. -0.03 min

Lab File: BF093117.D

Acq: 23 Feb 2017 21:13


Tgt Ion:264 Resp: 368360

Ion Ratio Lower Upper

264 100

260 24.4 19.2 28.8

265 21.8 17.4 26.0



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

