


Data Path : Z:\HPCHEM1\BNA F\DATA\BF022317\
 Data File : BF093097.D
 Acq On : 23 Feb 2017 9:16
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 17 17:31:55 2017

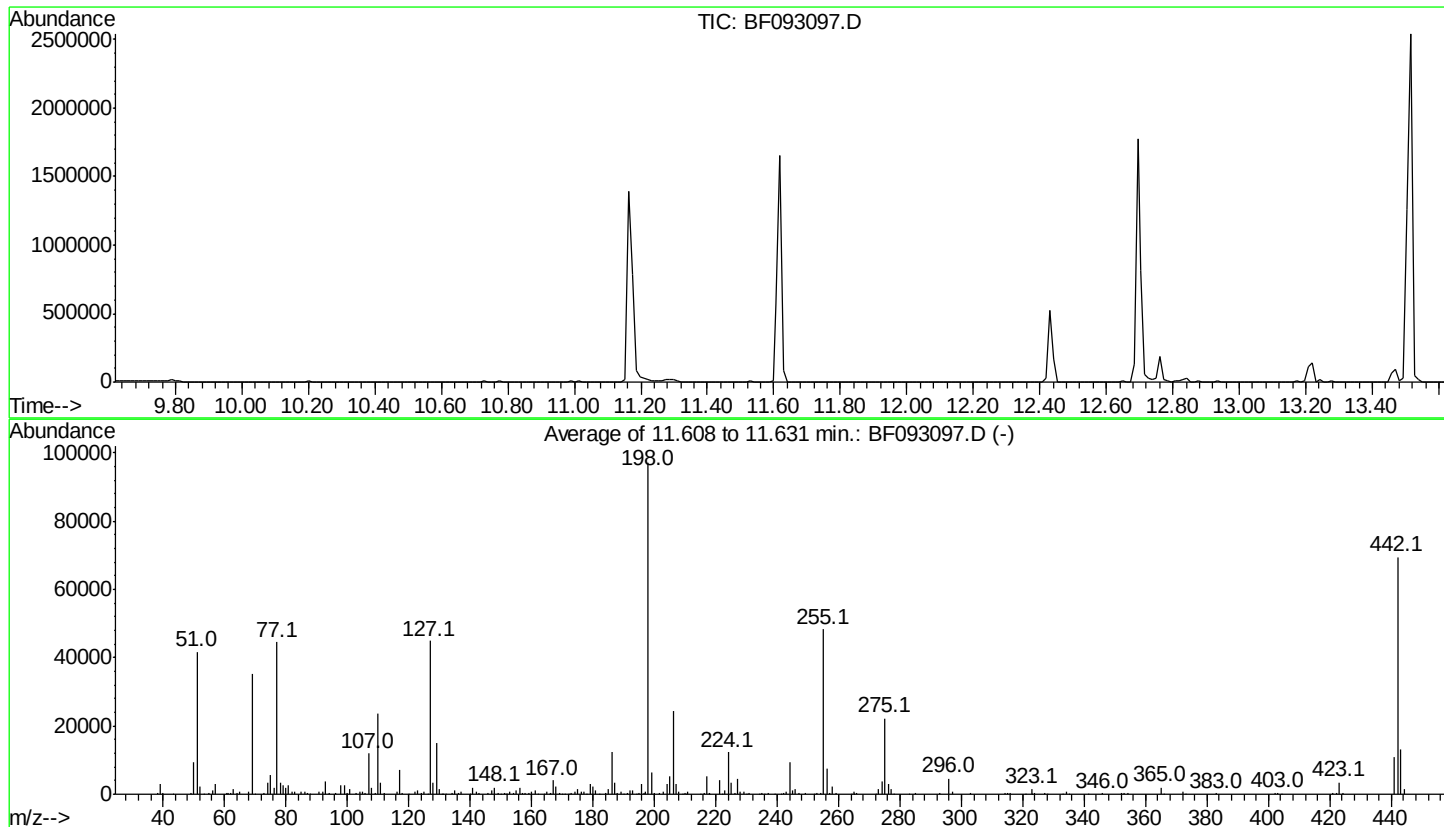

AutoFind: Scans 833, 834, 835; Background Corrected with Scan 829

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.9	41659	PASS
68	69	0.00	2	1.7	602	PASS
69	198	0.00	100	36.5	35423	PASS
70	69	0.00	2	0.3	119	PASS
127	198	10	80	46.2	44919	PASS
197	198	0.00	2	0.9	898	PASS
198	198	100	100	100.0	97166	PASS
199	198	5	9	6.7	6477	PASS
275	198	10	60	22.9	22220	PASS
365	198	1	100	1.9	1877	PASS
441	442	0.01	24	15.6	10824	PASS
442	198	50	100	71.6	69535	PASS
443	442	15	24	19.1	13273	PASS