


Data Path : Z:\HPCHEM1\BNA F\DATA\BF022317\
Data File : BF093103.D
Acq On : 23 Feb 2017 14:33
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Feb 17 17:31:55 2017

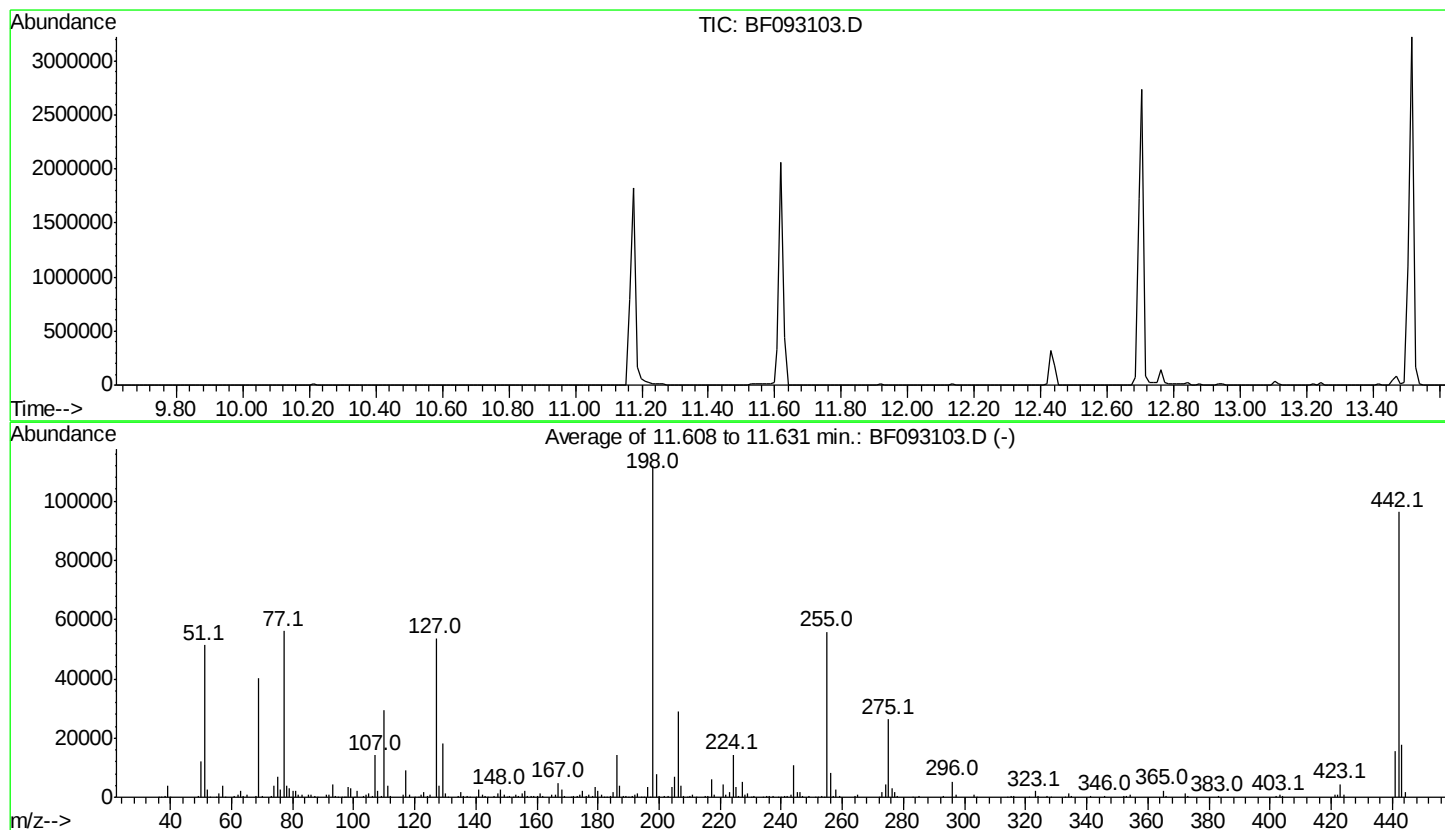

AutoFind: Scans 833, 834, 835; Background Corrected with Scan 829

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.9	51399	PASS
68	69	0.00	2	1.1	435	PASS
69	198	0.00	100	35.9	40246	PASS
70	69	0.00	2	0.8	342	PASS
127	198	10	80	47.8	53511	PASS
197	198	0.00	2	0.1	118	PASS
198	198	100	100	100.0	111989	PASS
199	198	5	9	6.8	7602	PASS
275	198	10	60	23.4	26218	PASS
365	198	1	100	2.0	2266	PASS
441	442	0.01	24	16.1	15466	PASS
442	198	50	100	86.0	96257	PASS
443	442	15	24	18.6	17912	PASS