


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF022317\
 Data File : BF093129.D
 Acq On : 24 Feb 2017 4:11
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 17 17:31:55 2017

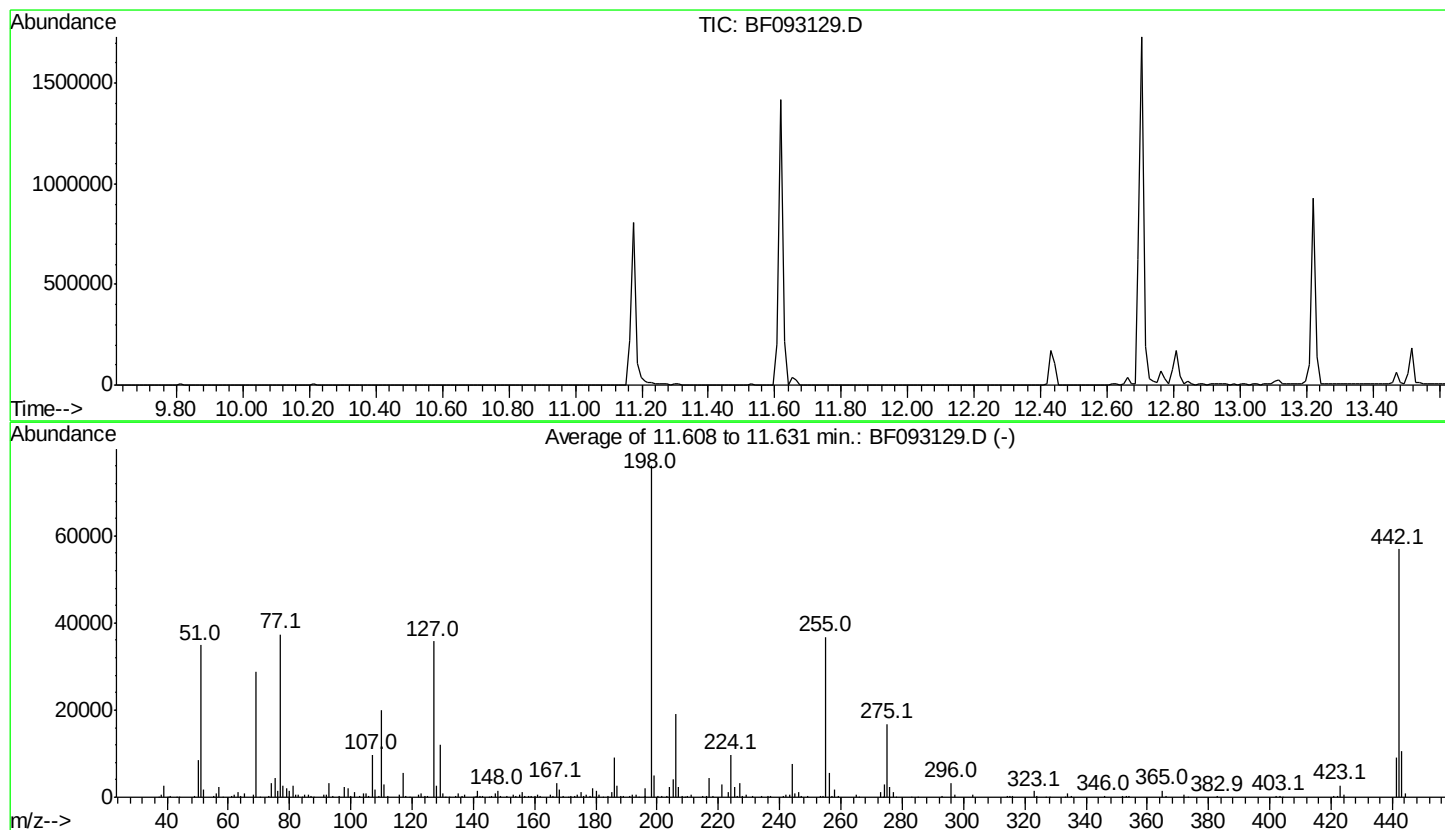

AutoFind: Scans 833, 834, 835; Background Corrected with Scan 830

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.9	34945	PASS
68	69	0.00	2	1.8	525	PASS
69	198	0.00	100	38.0	28938	PASS
70	69	0.00	2	0.4	114	PASS
127	198	10	80	47.1	35836	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	76104	PASS
199	198	5	9	6.6	5008	PASS
275	198	10	60	22.0	16748	PASS
365	198	1	100	2.0	1517	PASS
441	442	0.01	24	15.9	9063	PASS
442	198	50	100	74.8	56888	PASS
443	442	15	24	18.4	10454	PASS