
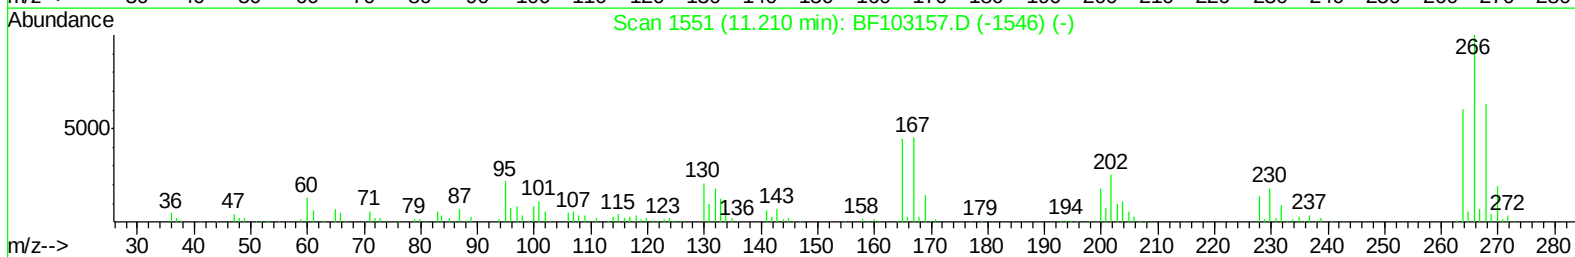
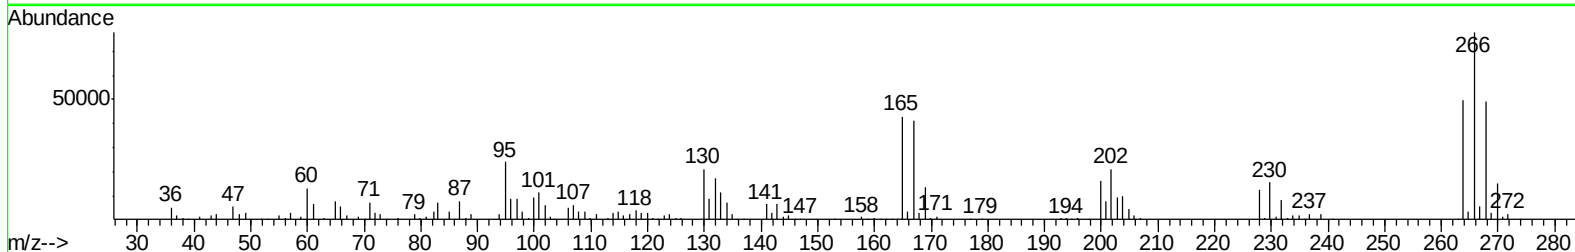


Data Path : Z:\HPCHEM1\BNA F\DATA\BF022318\
Data File : BF103183.D
Acq On : 23 Feb 2018 8:01
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 23 22:12:00 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 23 02:43:46 2018
Response via : Initial Calibration

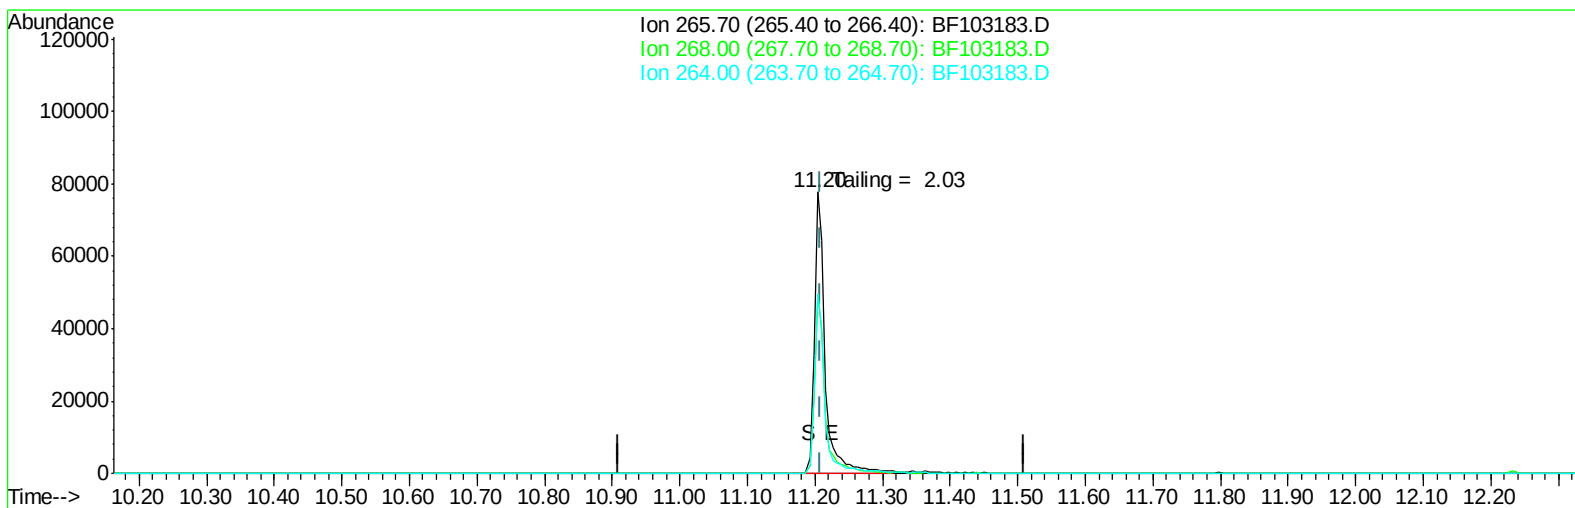

TIC: BF103183.D

(69) Pentachlorophenol (C)




11.204min (-0.006) 45801.68ng

response 87388

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.45
264.00	61.90	63.60
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF022318\
 Data File : BF103183.D
 Acq On : 23 Feb 2018 8:01
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 23 22:12:00 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 23 02:43:46 2018
 Response via : Initial Calibration

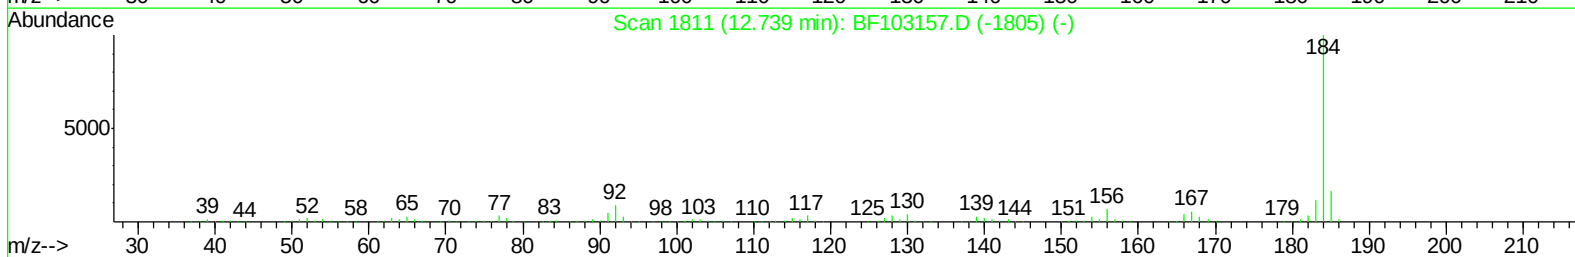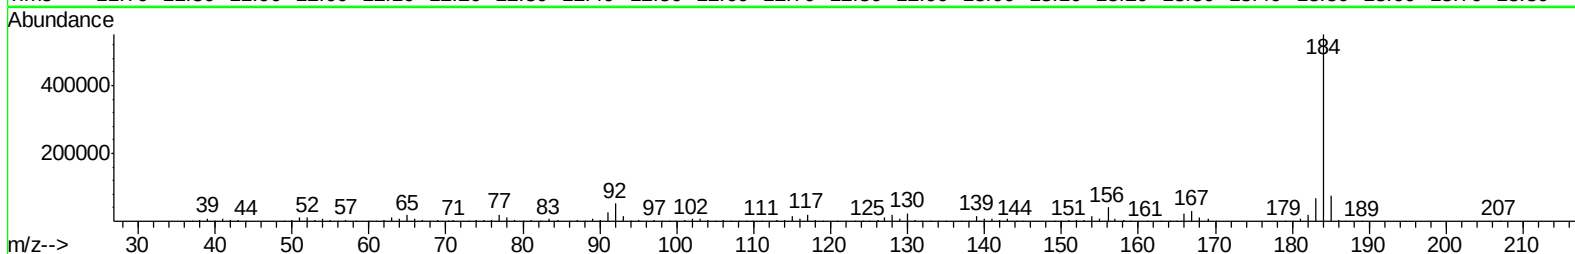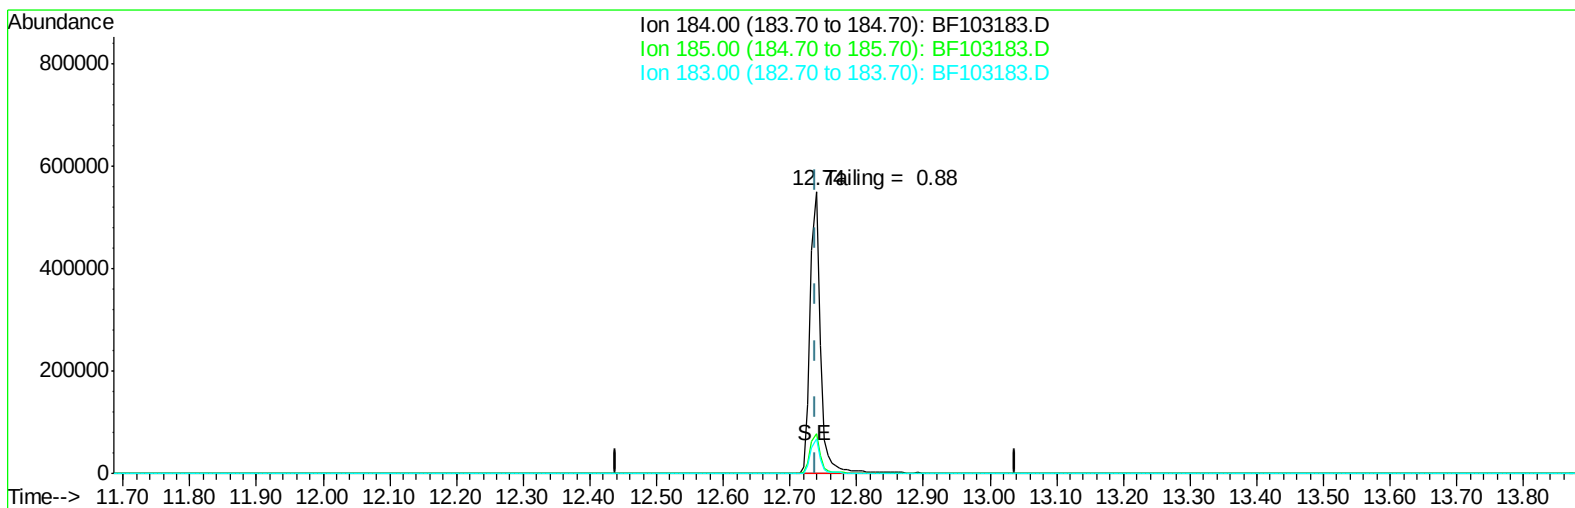

TIC: BF103183.D

(76) Benzidine

12.739min (-0.000) 0.00ng

response 560327

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.10
183.00	11.60	12.29
0.00	0.00	0.00