


Data Path : Z:\HPCHEM1\BNA F\Data\BF022318\
 Data File : BF103183.D
 Acq On : 23 Feb 2018 8:01
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF022218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 23 02:43:46 2018

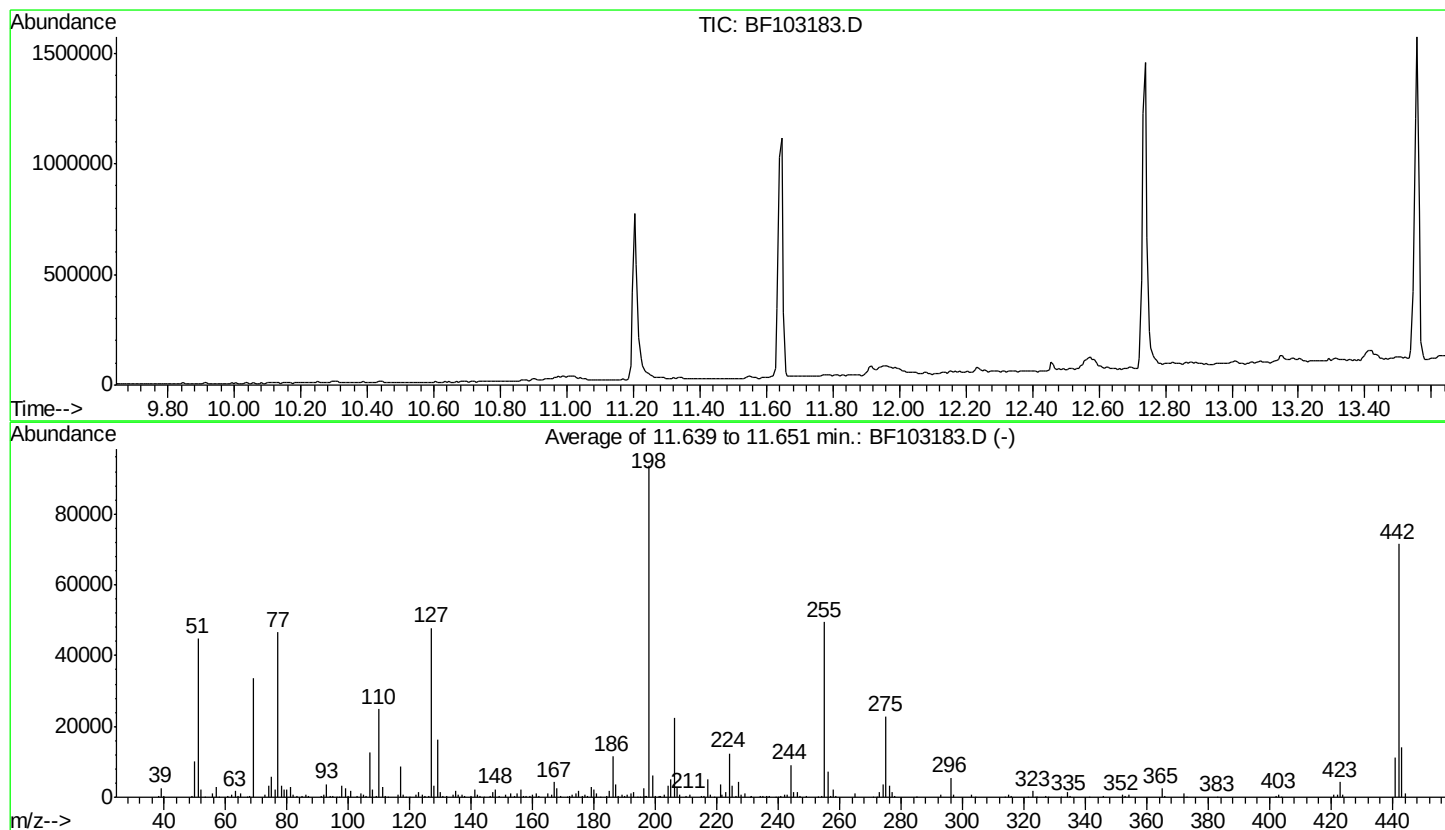

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.7	44671	PASS
68	69	0.00	2	1.4	474	PASS
69	198	0.00	100	35.8	33567	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.1	47895	PASS
197	198	0.00	2	0.4	364	PASS
198	198	100	100	100.0	93645	PASS
199	198	5	9	6.5	6042	PASS
275	198	10	60	24.3	22764	PASS
365	198	1	100	2.7	2511	PASS
441	443	0.01	100	81.6	11393	PASS
442	198	50	100	76.4	71501	PASS
443	442	15	24	19.5	13963	PASS