
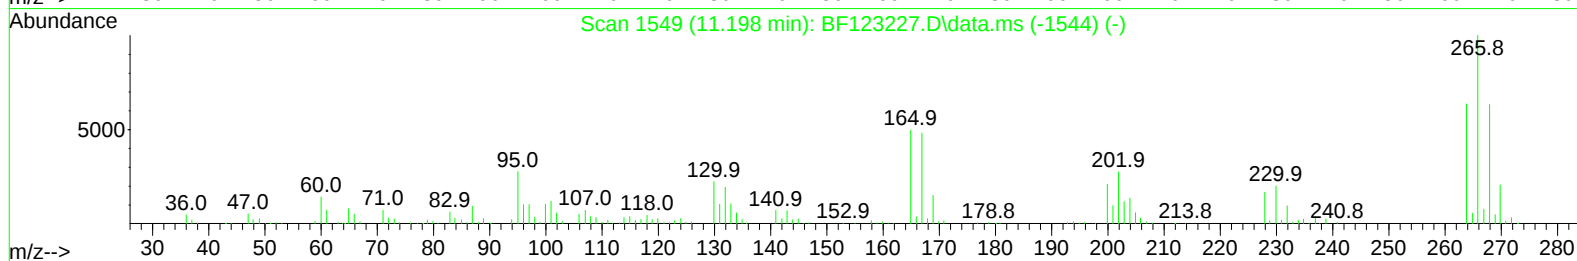
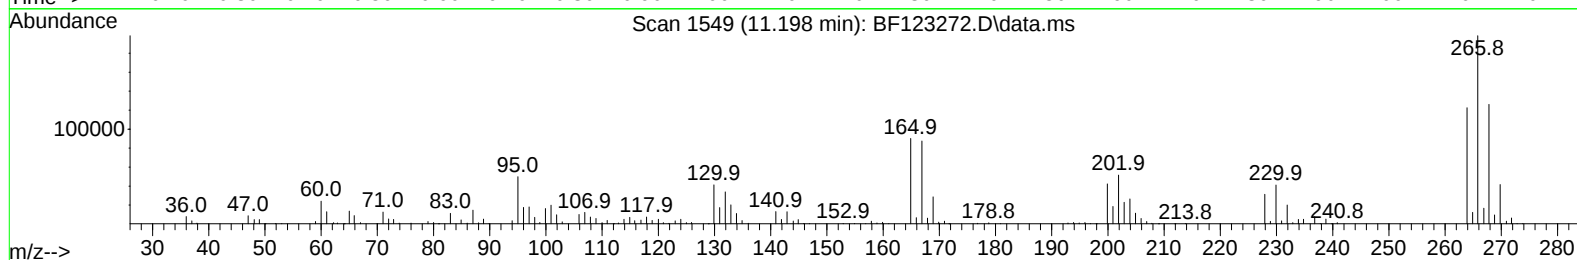


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022321\
 Data File : BF123272.D
 Acq On : 23 Feb 2021 9:47
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 23 10:51:45 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 19 16:08:53 2021
 Response via : Initial Calibration

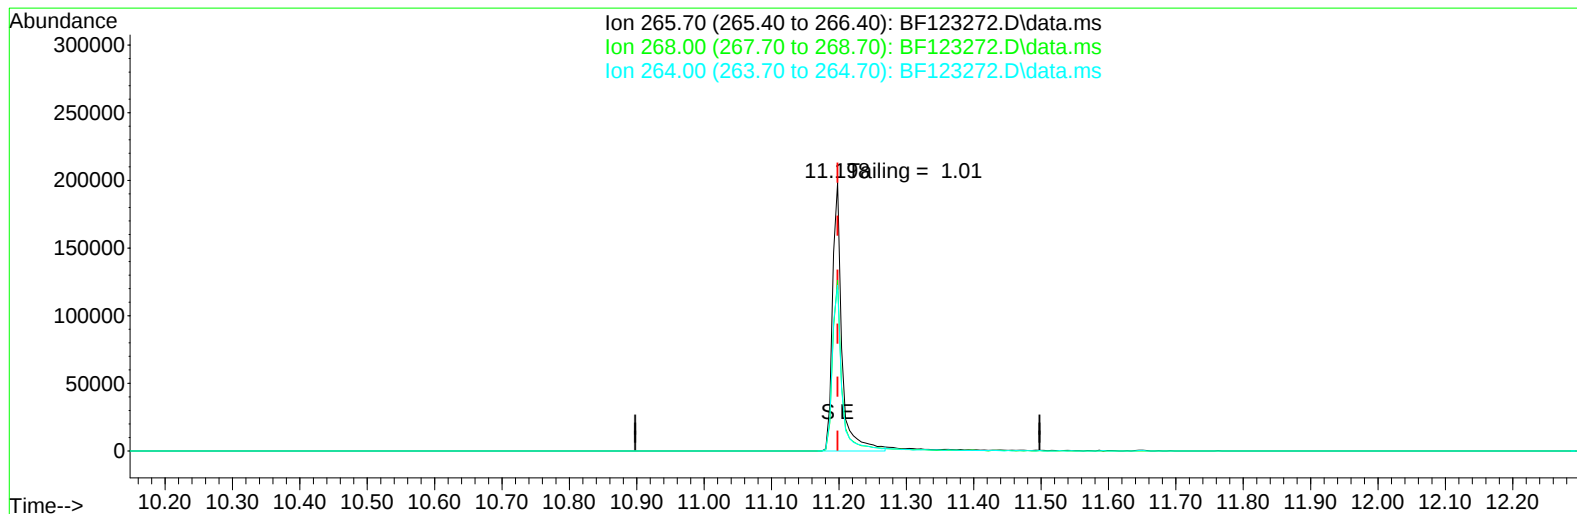

TIC: BF123272.D\data.ms

(70) Pentachlorophenol (C)




11.198min (+ 0.000) 25884.56 ng

response 196710

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.56
264.00	62.30	61.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022321\
Data File : BF123272.D
Acq On : 23 Feb 2021 9:47
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 23 10:51:45 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 19 16:08:53 2021
Response via : Initial Calibration

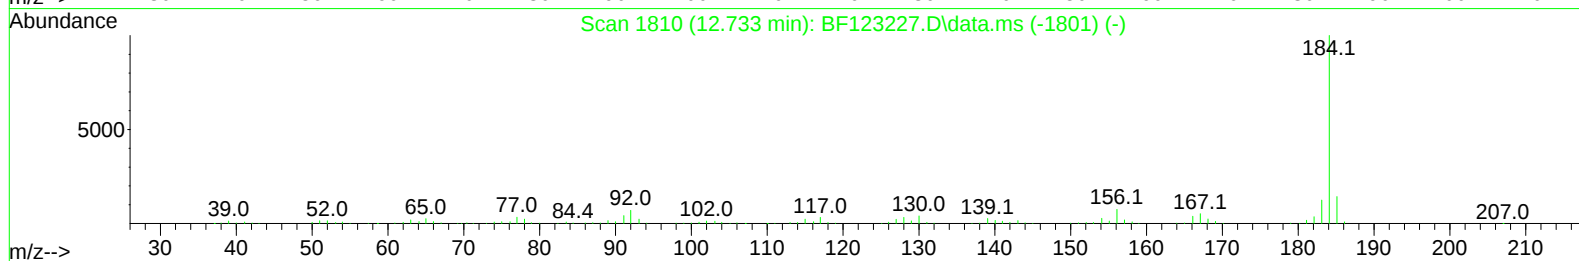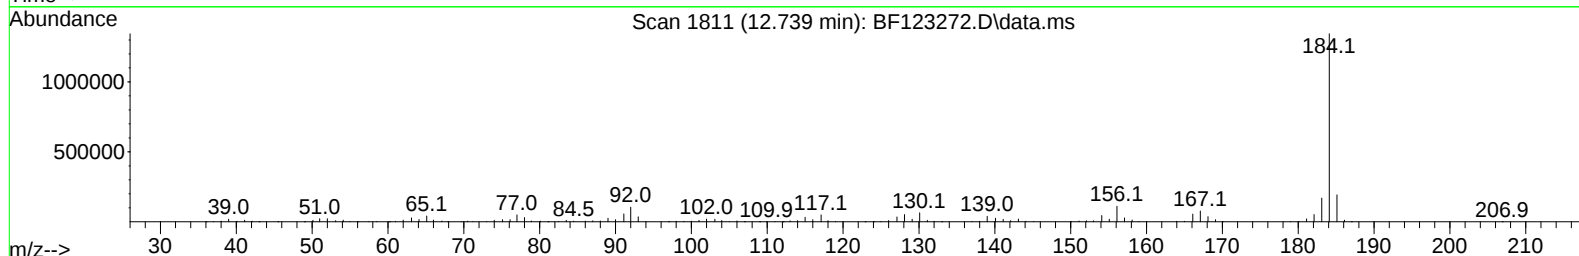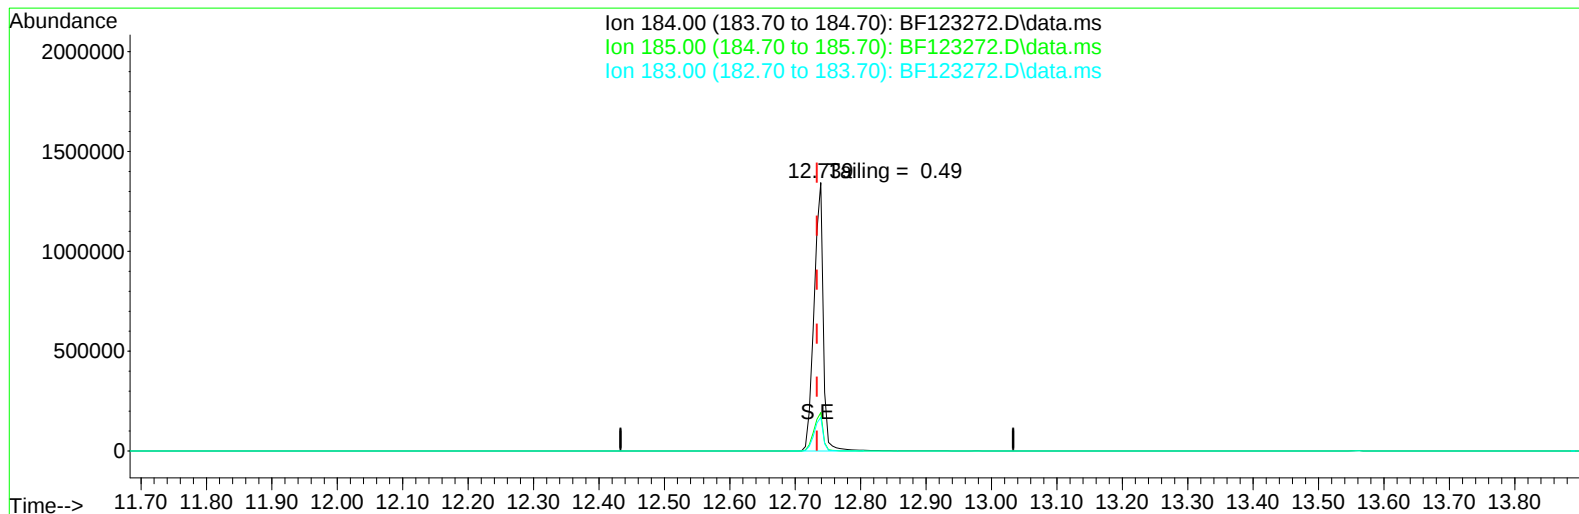

TIC: BF123272.D\data.ms

(77) Benzidine

12.739min (+ 0.006) 0.00 ng

response 1315008

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.33
183.00	12.10	12.62
0.00	0.00	0.00