

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022321\
 Data File : BF123274.D
 Acq On : 23 Feb 2021 11:04
 Operator : JU/CG
 Sample : PB134764BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB134764BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF123274.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.493	573	579	582	rBV	3865674	3949811	83.71%	13.701%
2	6.493	743	749	752	rBV	3660839	3941115	83.52%	13.671%
3	6.857	807	811	814	rBV	960000	828737	17.56%	2.875%
4	7.422	901	907	910	rBV	2334251	2594538	54.99%	9.000%
5	8.140	1024	1029	1032	rBV	1231617	1080365	22.90%	3.748%
6	9.222	1206	1213	1216	rBV	3996405	4355096	92.30%	15.107%
7	9.898	1322	1328	1331	rBV	1375809	1200876	25.45%	4.166%
8	10.692	1457	1463	1477	rBV	2795237	2777769	58.87%	9.635%
9	11.386	1576	1581	1585	rBV	1338496	1244886	26.38%	4.318%
10	12.986	1846	1853	1856	rBV	5081222	4718601	100.00%	16.368%
11	14.039	2027	2032	2041	rBV	1199676	1099631	23.30%	3.814%
12	15.510	2277	2282	2294	rBV	756771	1037352	21.98%	3.598%




Sum of corrected areas: 28828777

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022321\
Data File : BF123274.D
Acq On : 23 Feb 2021 11:04
Operator : JU/CG
Sample : PB134764BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB134764BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

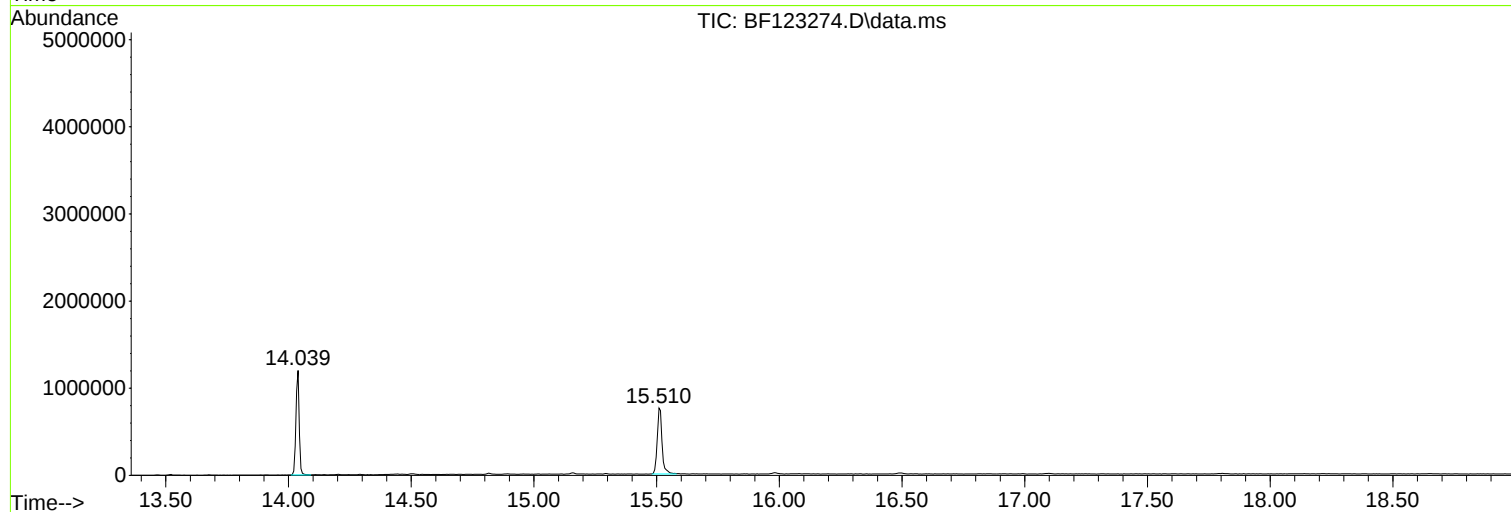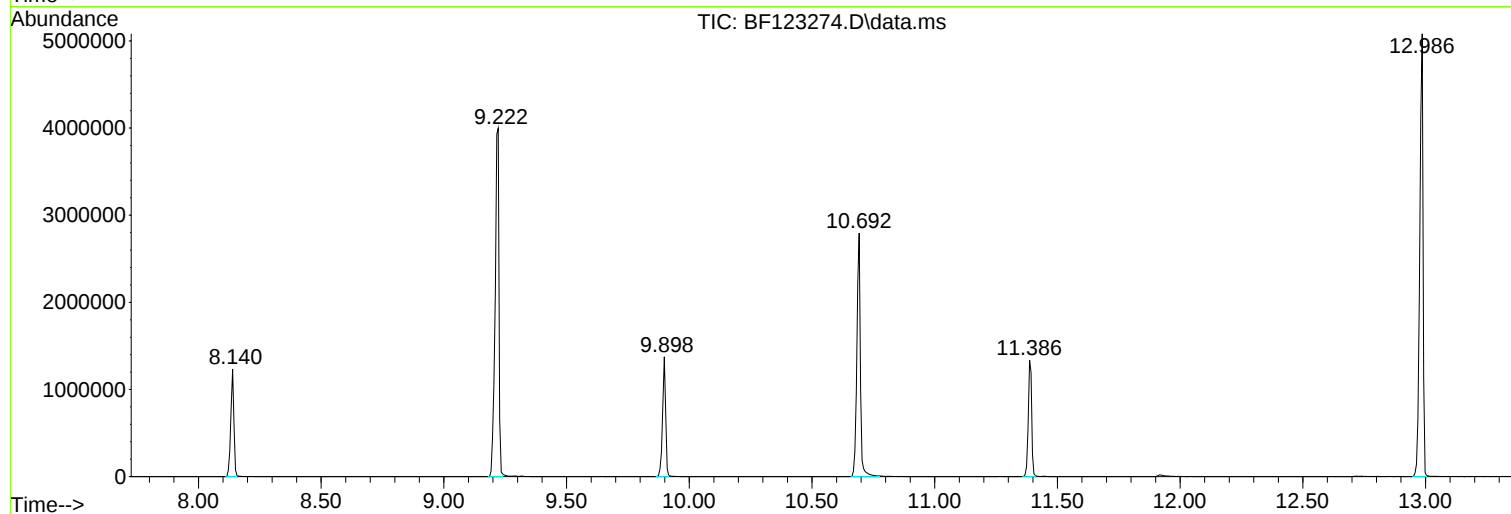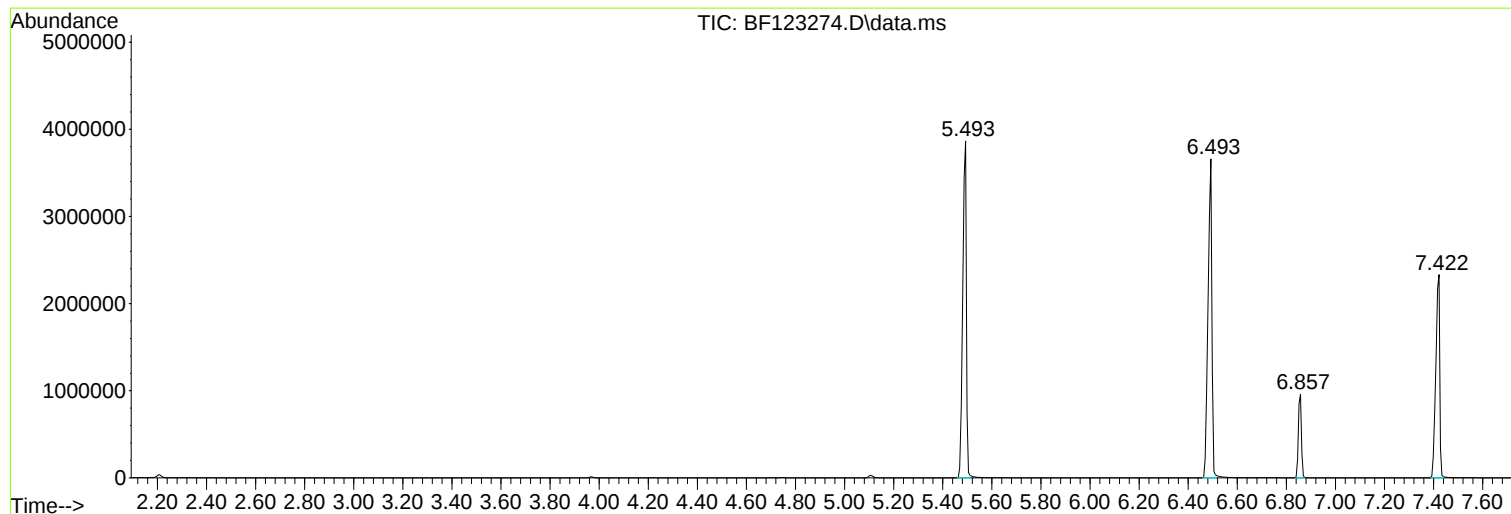

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022321\
Data File : BF123274.D
Acq On : 23 Feb 2021 11:04
Operator : JU/CG
Sample : PB134764BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB134764BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022321\
Data File : BF123274.D
Acq On : 23 Feb 2021 11:04
Operator : JU/CG
Sample : PB134764BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB134764BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------