

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022321\
 Data File : BF123279.D
 Acq On : 23 Feb 2021 14:05
 Operator : JU/CG
 Sample : PB134772BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB134772BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF123279.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.487	573	578	581	rBV	3462897	3588254	81.58%	13.717%
2	6.492	743	749	752	rBV	3398833	3568459	81.13%	13.641%
3	6.857	807	811	814	rBV	810983	727776	16.55%	2.782%
4	7.416	901	906	909	rBV	2173895	2334493	53.07%	8.924%
5	8.139	1024	1029	1037	rBV	1085937	959675	21.82%	3.669%
6	9.216	1206	1212	1216	rBV	3687784	3896754	88.59%	14.896%
7	9.898	1323	1328	1338	rBV	1235987	1071110	24.35%	4.095%
8	10.692	1458	1463	1478	rBV	2413832	2441652	55.51%	9.334%
9	11.386	1576	1581	1585	rBV	1236654	1108748	25.21%	4.238%
10	12.986	1846	1853	1856	rBV	4390364	4398487	100.00%	16.814%
11	14.039	2028	2032	2043	rVB	1196903	1068277	24.29%	4.084%
12	15.509	2277	2282	2295	rBV	748841	995794	22.64%	3.807%




Sum of corrected areas: 26159479

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022321\
Data File : BF123279.D
Acq On : 23 Feb 2021 14:05
Operator : JU/CG
Sample : PB134772BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB134772BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

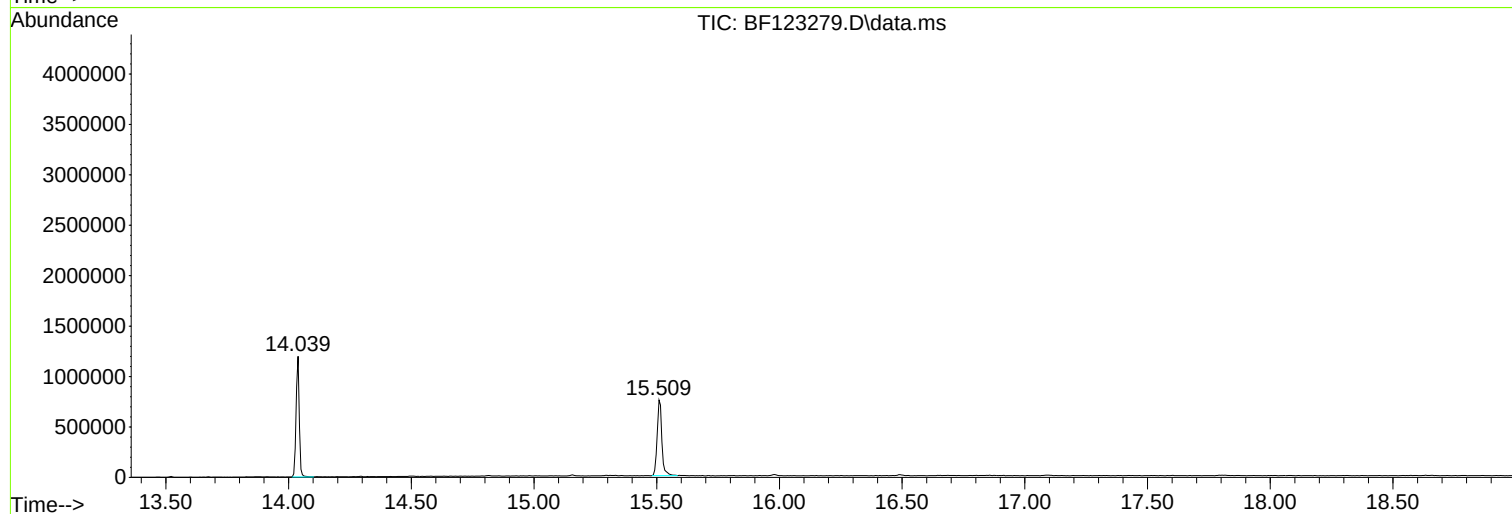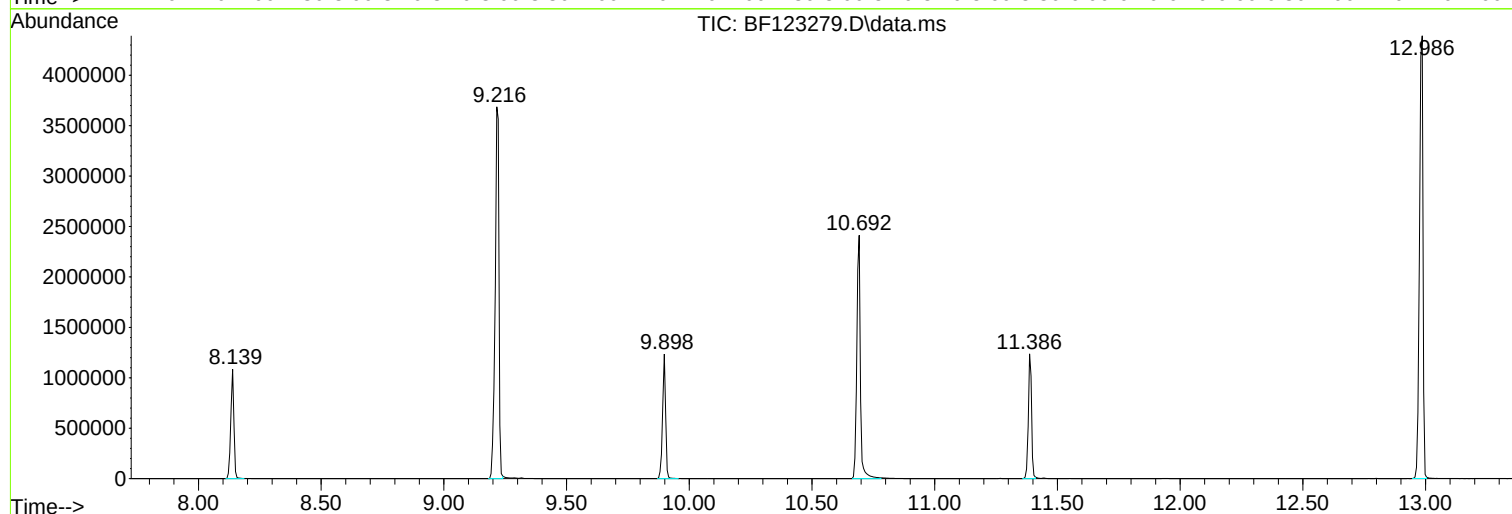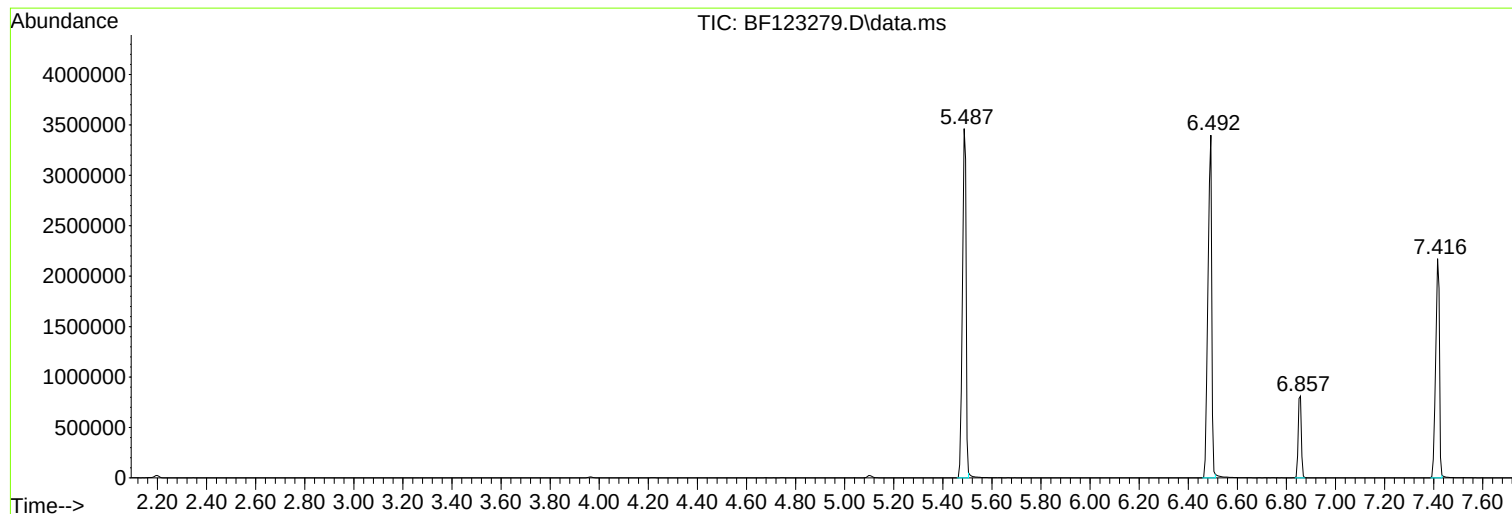

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022321\
Data File : BF123279.D
Acq On : 23 Feb 2021 14:05
Operator : JU/CG
Sample : PB134772BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB134772BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022321\
Data File : BF123279.D
Acq On : 23 Feb 2021 14:05
Operator : JU/CG
Sample : PB134772BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB134772BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------