
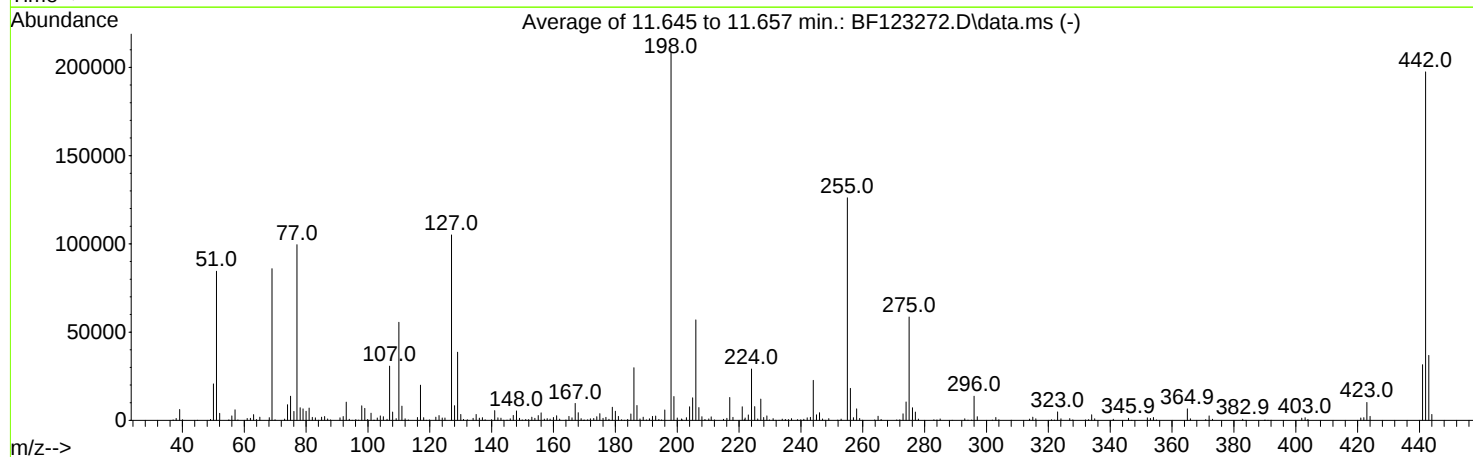


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022321\
 Data File : BF123272.D
 Acq On : 23 Feb 2021 9:47
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 19 16:08:53 2021

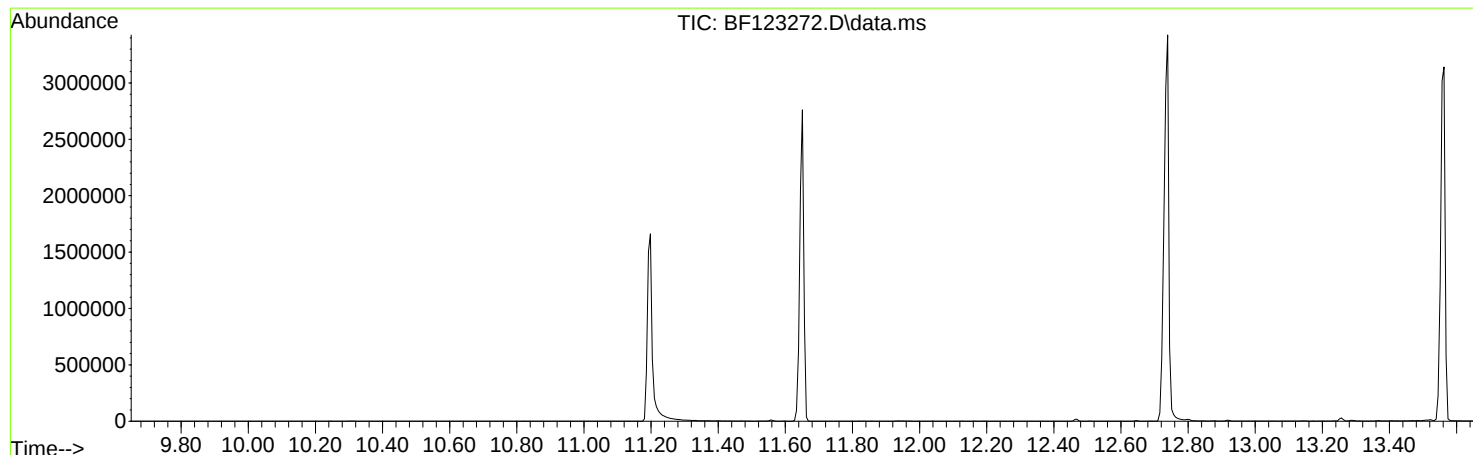

AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.5	84488	PASS
68	69	0.00	2	1.8	1588	PASS
69	198	0.00	100	41.3	85984	PASS
70	69	0.00	2	0.4	364	PASS
127	198	10	80	50.4	105109	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	208437	PASS
199	198	5	9	6.5	13498	PASS
275	198	10	60	28.1	58595	PASS
365	198	1	100	3.1	6522	PASS
441	198	0.01	100	15.1	31520	PASS
442	442	50	100	100.0	197451	PASS
443	442	15	24	18.6	36792	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/23/2021	BNA_F	<u>BF123272.D</u>
Compound Name	Response	Retention Time
DDT	540703	13.56
DDD	5873	13.25
DDE	1673	12.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7546	548249	1.38

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022321\
Data File : BF123272.D
Acq On : 23 Feb 2021 9:47
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 23 10:51:45 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 19 16:08:53 2021
Response via : Initial Calibration

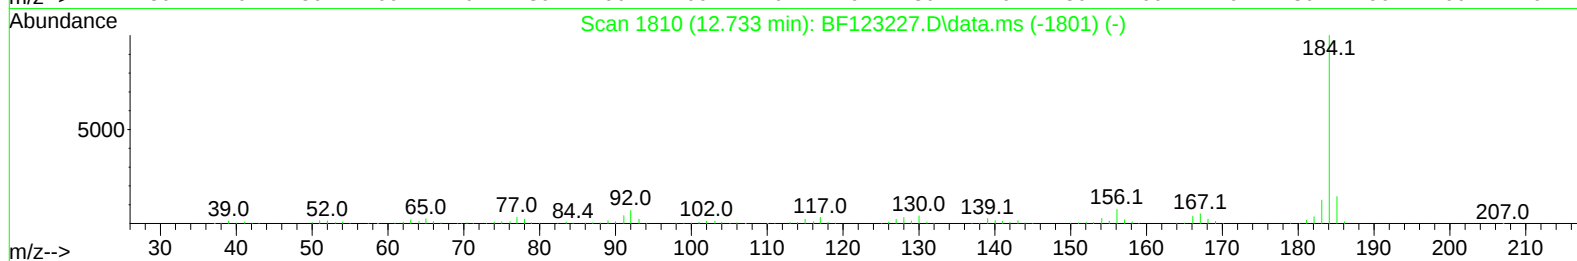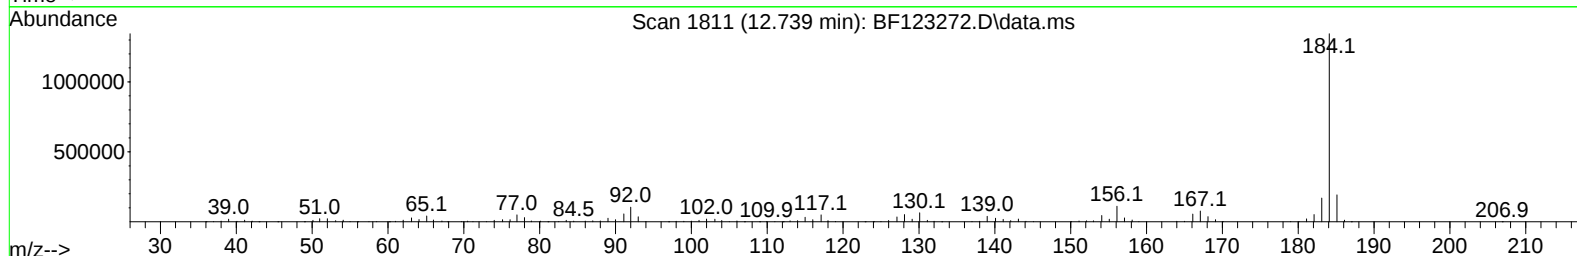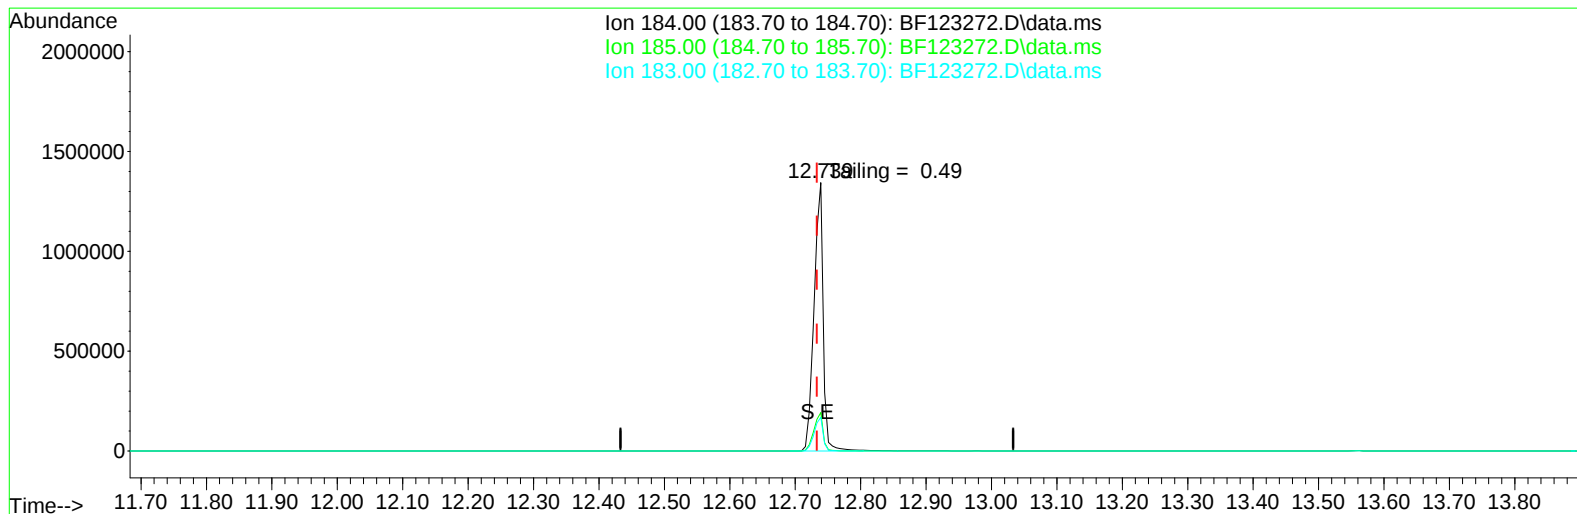

TIC: BF123272.D\data.ms

(77) Benzidine

12.739min (+ 0.006) 0.00 ng

response 1315008

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.33
183.00	12.10	12.62
0.00	0.00	0.00