
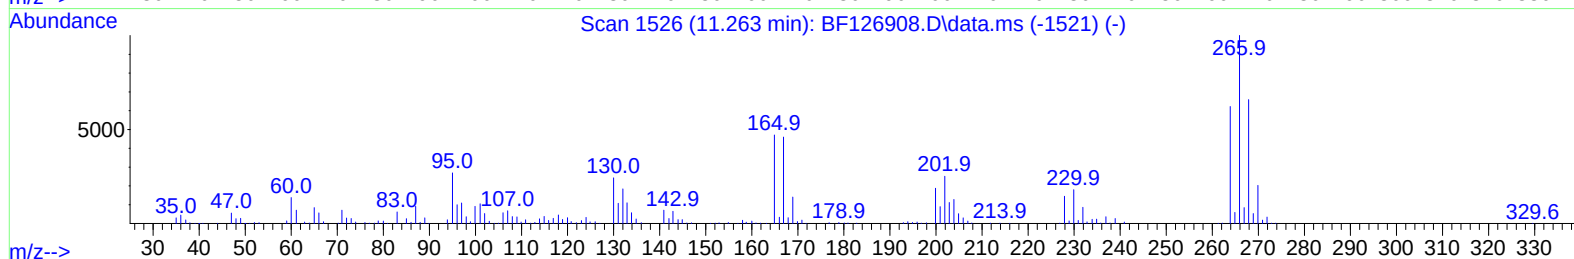
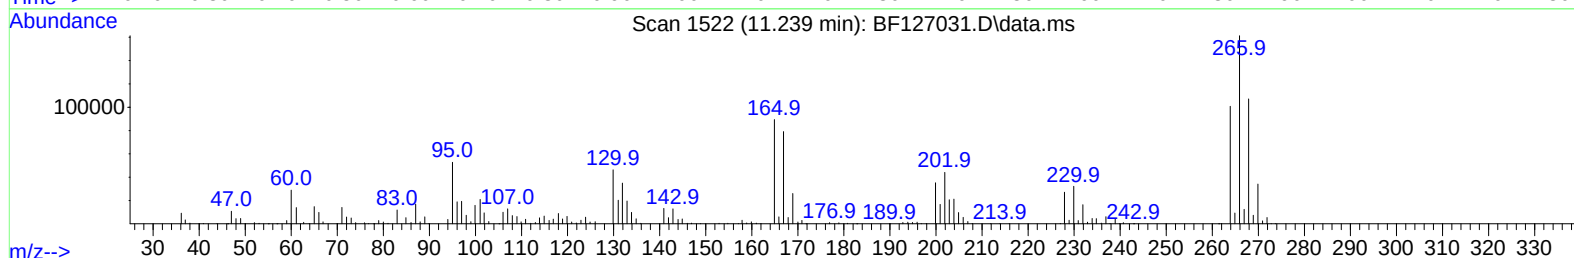


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022322\
Data File : BF127031.D
Acq On : 23 Feb 2022 10:33
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 24 06:09:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 24 02:10:57 2022
Response via : Initial Calibration

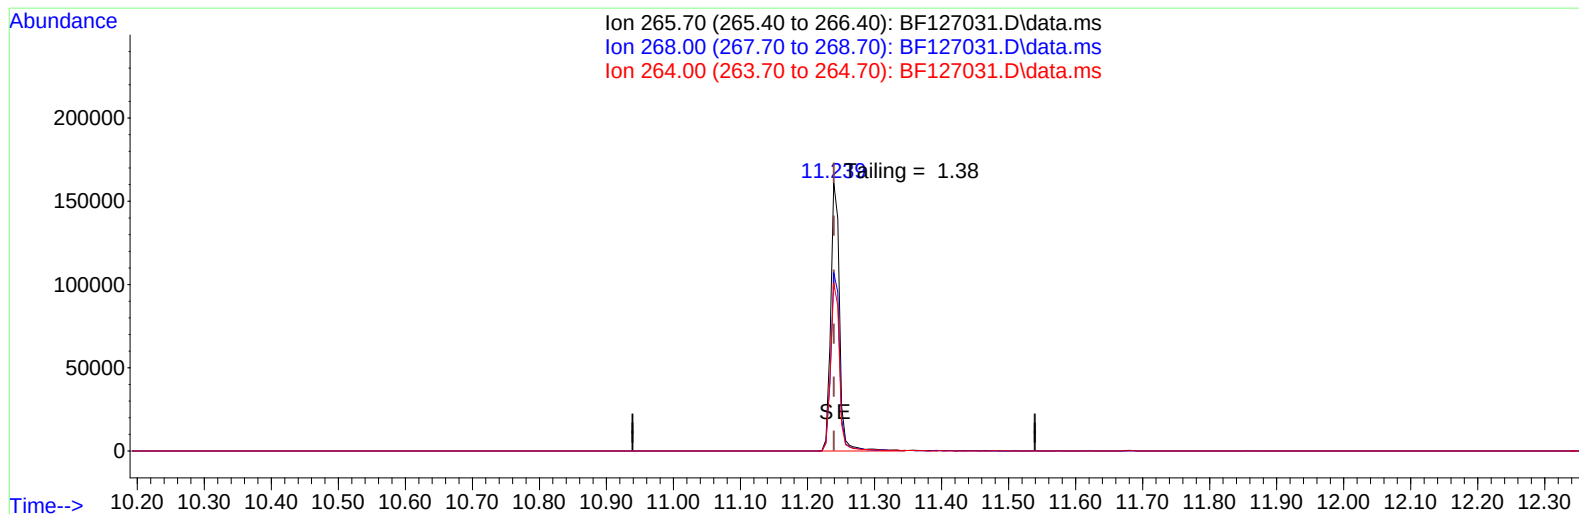

TIC: BF127031.D\data.ms

(70) Pentachlorophenol (C)




11.239min (-0.000) 333620.86 ng

response 148957

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	66.41
264.00	63.00	62.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022322\
Data File : BF127031.D
Acq On : 23 Feb 2022 10:33
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 24 06:09:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 24 02:10:57 2022
Response via : Initial Calibration

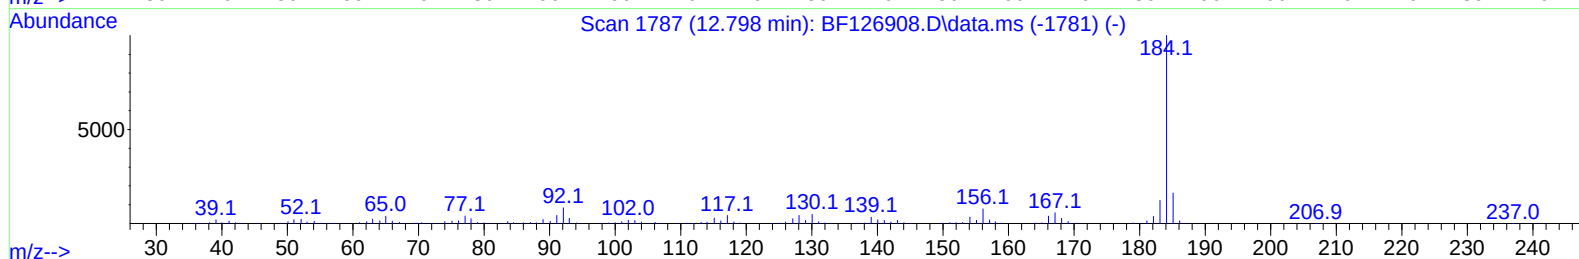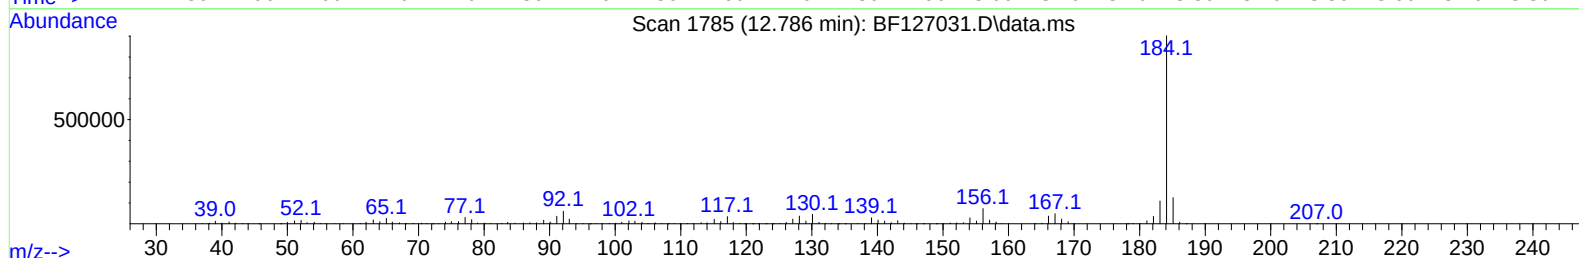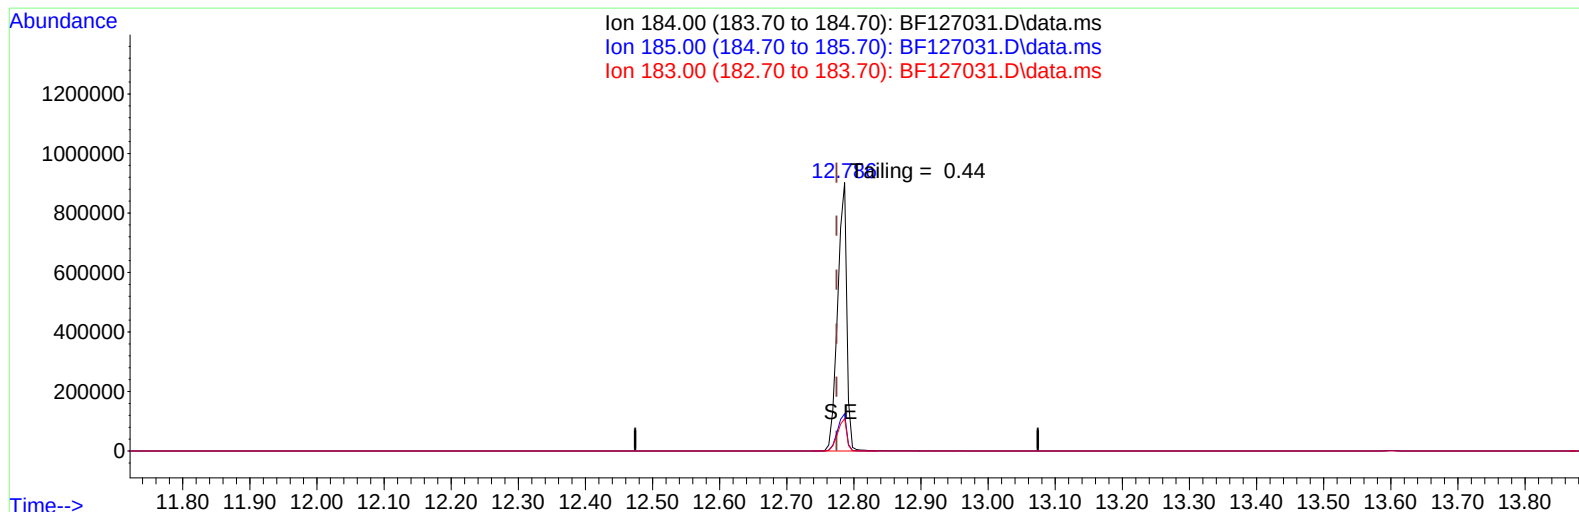

TIC: BF127031.D\data.ms

(77) Benzidine

12.786min (+ 0.012) 76976.28 ng

response 853488

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	13.93
183.00	10.20	12.15
0.00	0.00	0.00