

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022322\
 Data File : BF127033.D
 Acq On : 23 Feb 2022 12:03
 Operator : CG\JU
 Sample : PB142871BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB142871BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127033.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.540	548	553	556	rBV	3218116	3247924	74.02%	13.086%
2	6.539	716	723	725	rBV	2798120	3324357	75.77%	13.394%
3	6.910	782	786	789	rVB	720486	650242	14.82%	2.620%
4	7.469	875	881	884	rBV	2003206	2292453	52.25%	9.237%
5	8.192	998	1004	1007	rBV	902564	881193	20.08%	3.550%
6	9.269	1180	1187	1190	rBV	4259069	4005928	91.30%	16.140%
7	9.945	1297	1302	1306	rBV	1057544	974735	22.22%	3.927%
8	10.739	1430	1437	1440	rBV	2839652	2765992	63.04%	11.145%
9	11.439	1552	1556	1559	rBV	1303232	1015222	23.14%	4.090%
10	13.027	1821	1826	1829	rBV	4293340	4387714	100.00%	17.679%
11	14.080	2002	2005	2009	rBV	764639	734498	16.74%	2.959%
12	15.586	2256	2261	2265	rVB	425603	538976	12.28%	2.172%




Sum of corrected areas: 24819234

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022322\
Data File : BF127033.D
Acq On : 23 Feb 2022 12:03
Operator : CG\JU
Sample : PB142871BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB142871BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

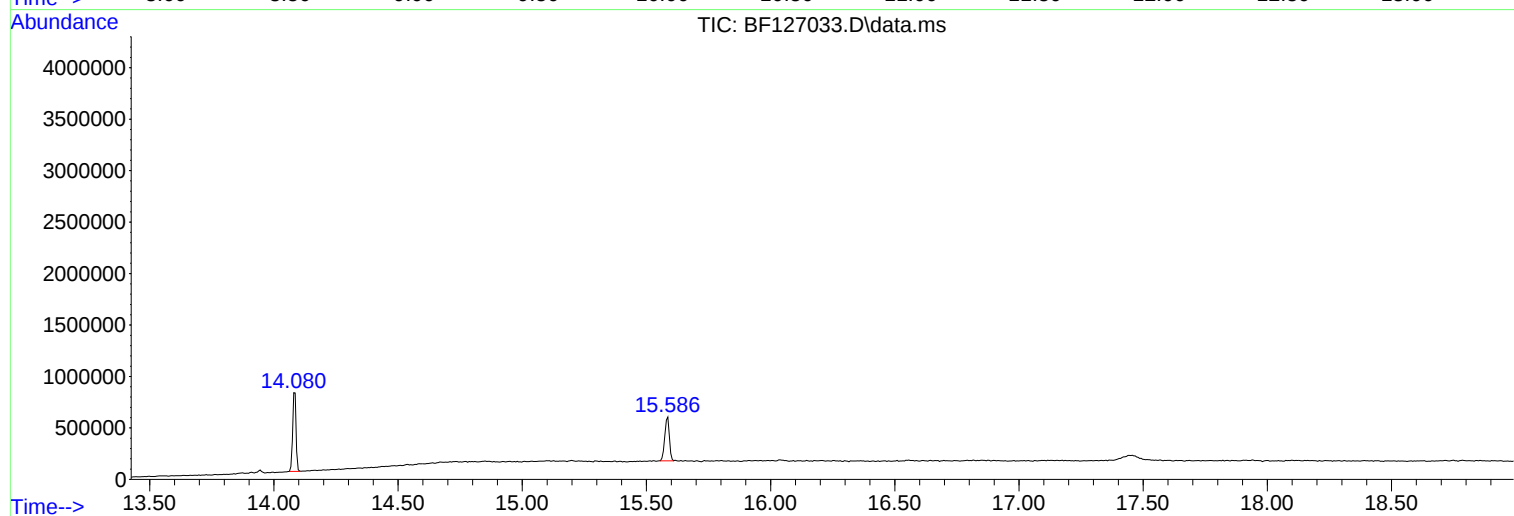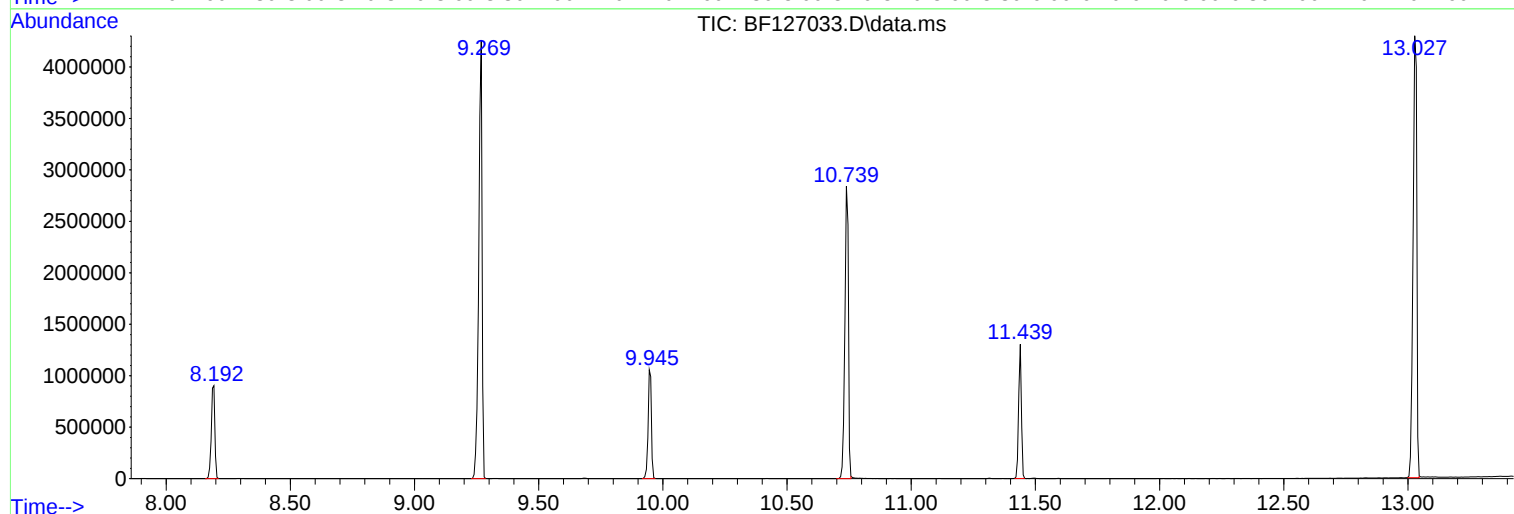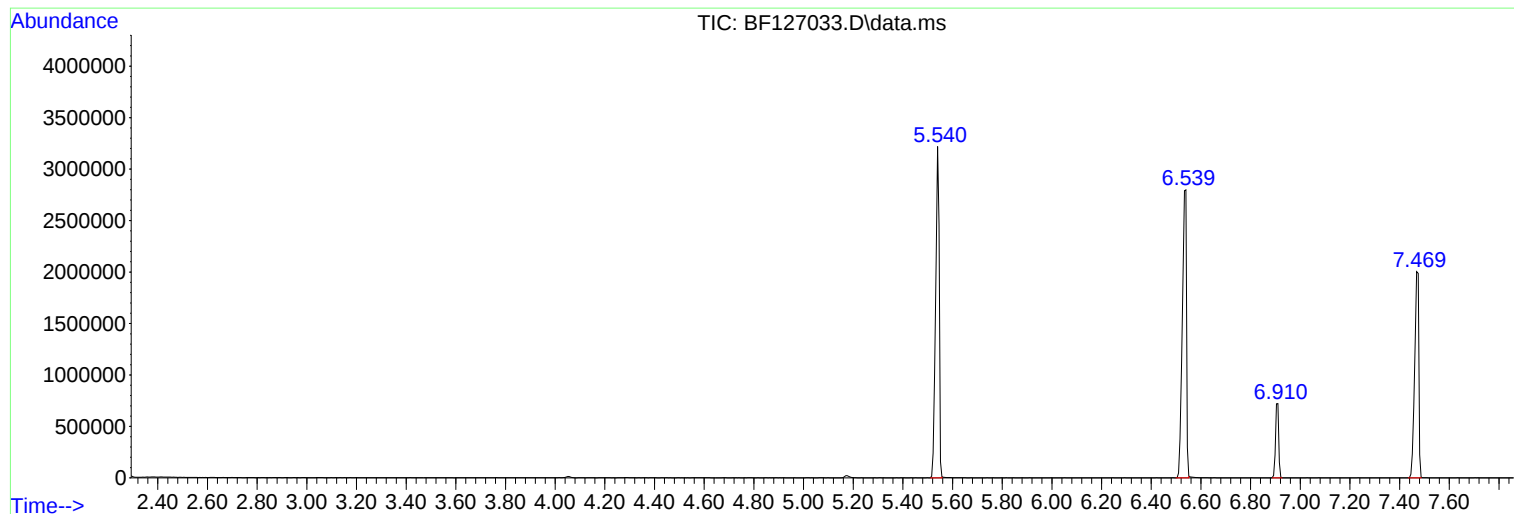

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022322\
Data File : BF127033.D
Acq On : 23 Feb 2022 12:03
Operator : CG\JU
Sample : PB142871BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB142871BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022322\
Data File : BF127033.D
Acq On : 23 Feb 2022 12:03
Operator : CG\JU
Sample : PB142871BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB142871BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------