


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022324\
Data File : BF137365.D
Acq On : 23 Feb 2024 10:01
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Feb 24 04:23:49 2024

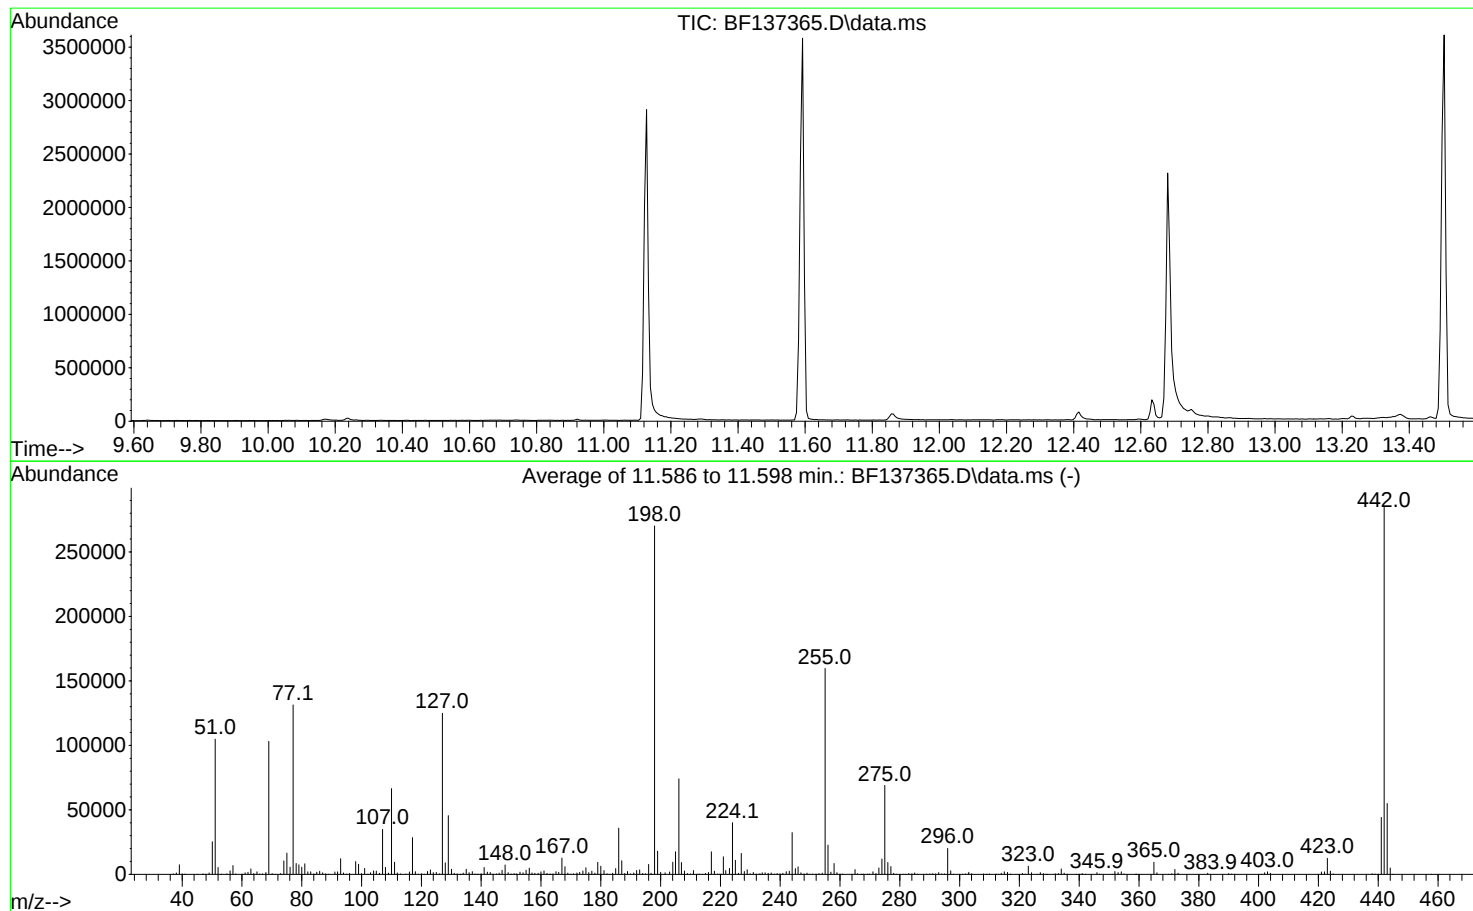




AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.8	104859	PASS
68	69	0.00	2	1.5	1531	PASS
69	198	0.00	100	38.2	103085	PASS
70	69	0.00	2	0.6	629	PASS
127	198	10	80	46.3	124984	PASS
197	198	0.00	2	0.3	896	PASS
198	198	100	100	100.0	270205	PASS
199	198	5	9	6.6	17941	PASS
275	198	10	60	25.5	68981	PASS
365	198	1	100	3.5	9426	PASS
441	198	0.01	100	16.4	44211	PASS
442	442	50	100	100.0	285227	PASS
443	442	15	24	19.3	54992	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022324\
Data File : BF137365.D
Acq On : 23 Feb 2024 10:01
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 24 04:31:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 24 04:23:49 2024
Response via : Initial Calibration

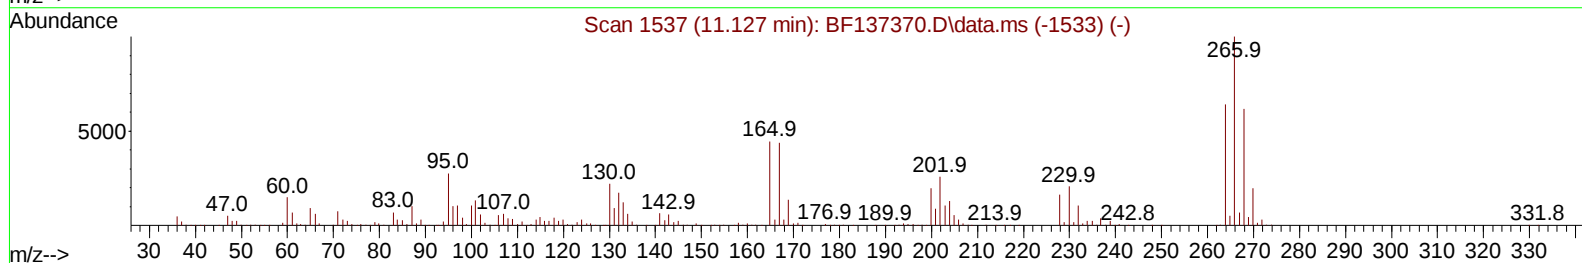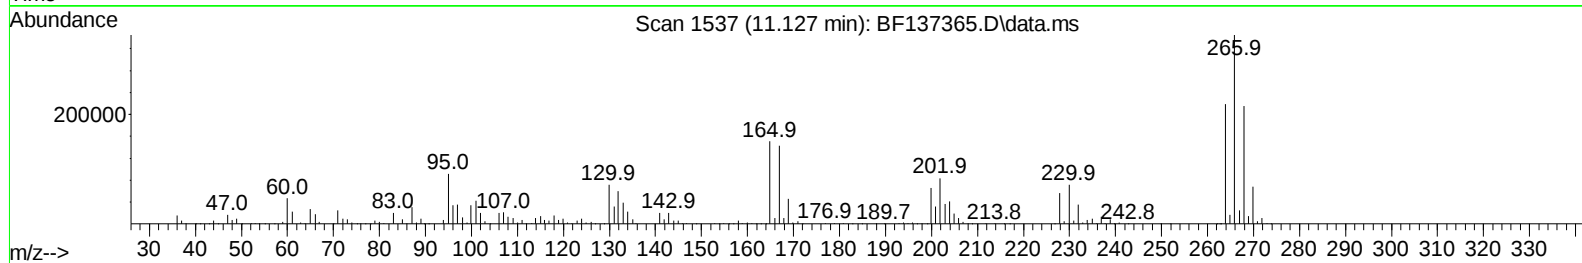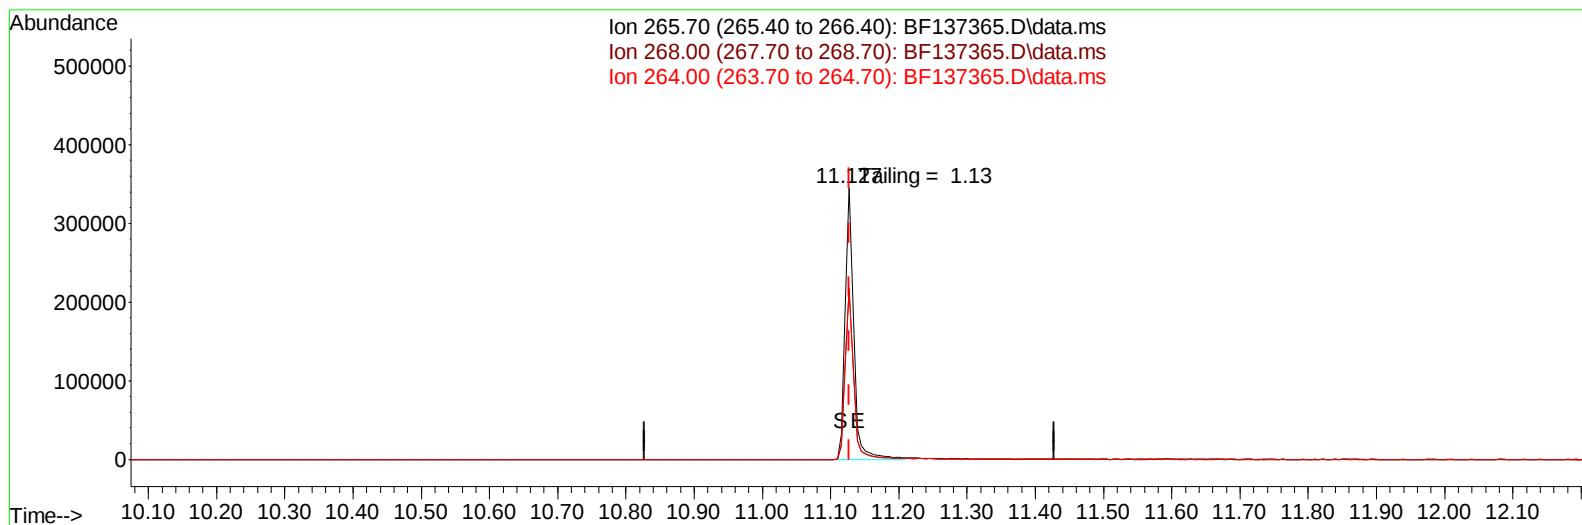

TIC: BF137365.D\data.ms

(70) Pentachlorophenol (C)

11.127min (-0.000) 516873.05 ng




response 302275

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.80	62.47
264.00	64.10	63.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022324\
Data File : BF137365.D
Acq On : 23 Feb 2024 10:01
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 24 04:31:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 24 04:23:49 2024
Response via : Initial Calibration

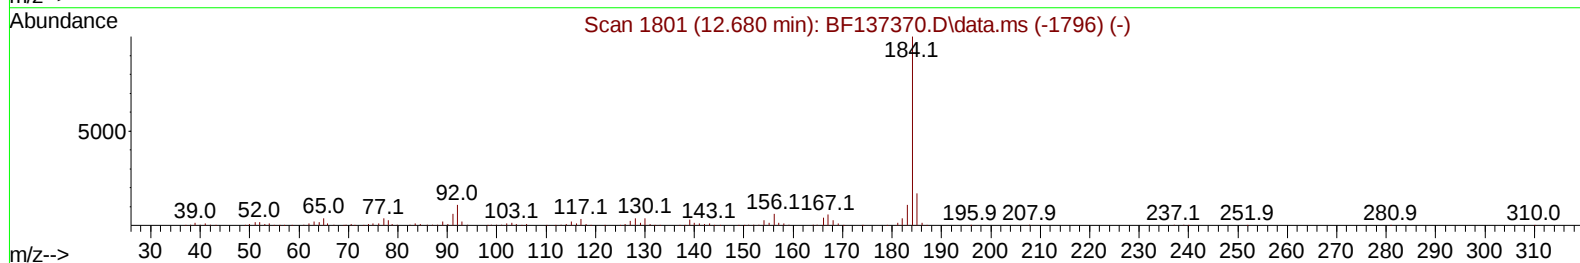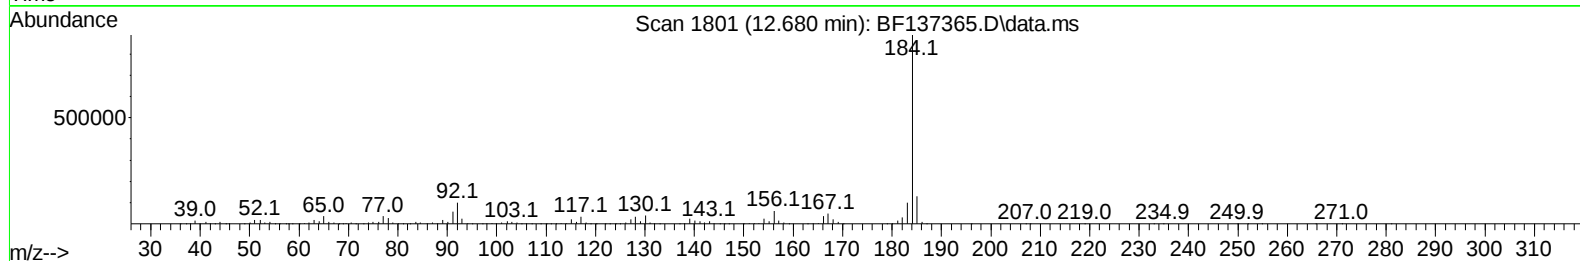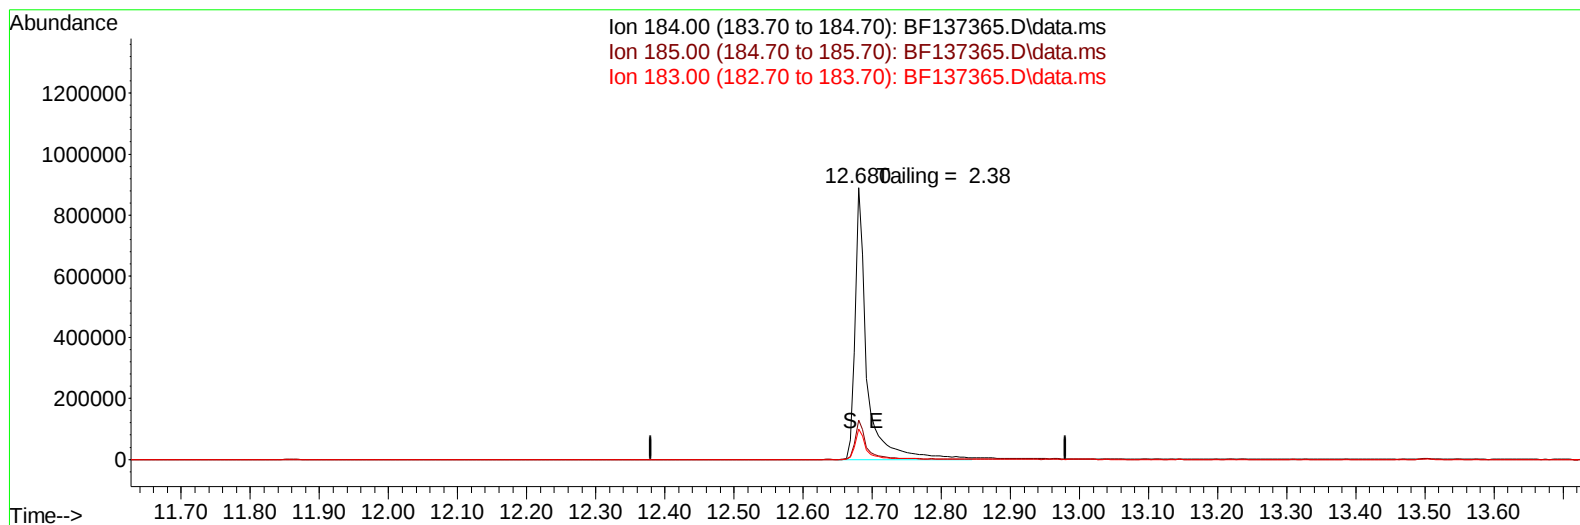

TIC: BF137365.D\data.ms

(77) Benzidine

12.680min (-12.680) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	17.10	0.00#
183.00	11.00	0.00#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/23/2024	BNA_F	<u>BF137365.D</u>
Compound Name	Response	Retention Time
DDT	463833	13.504
DDD	5350	13.227
DDE	486	12.863
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5836	469669	1.24

Instrument :
BNA_F
ClientSampleId :
DFTPP