


Data Path : Z:\HPCHEM1\BNA_F\Data\BF022415\
 Data File : BF077410.D
 Acq On : 24 Feb 2015 10:46
 Operator : IZ / TP
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Feb 19 16:57:32 2015

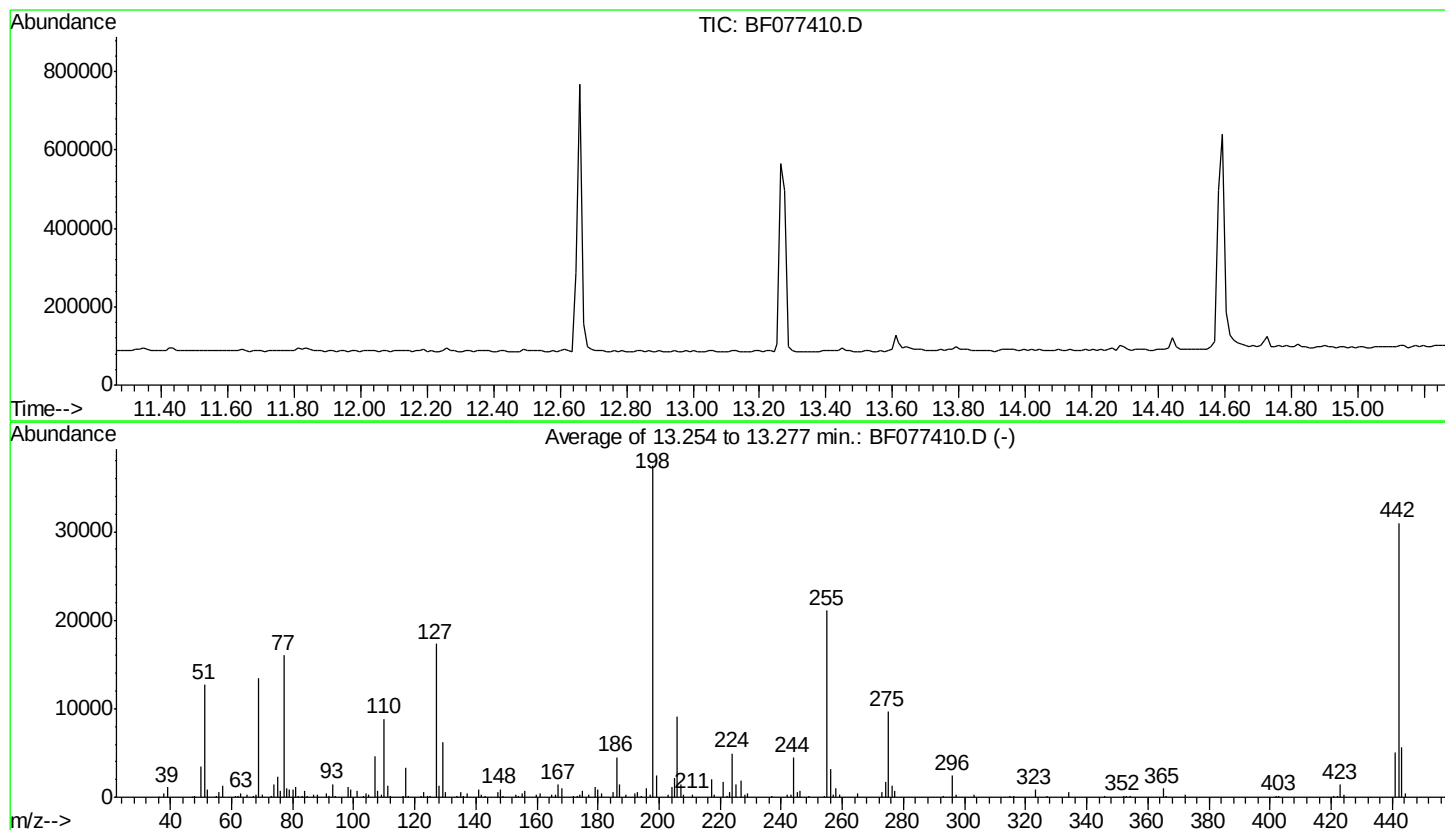

AutoFind: Scans 1082, 1083, 1084; Background Corrected with Scan 1079

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.9	12688	PASS
68	69	0.00	2	1.7	222	PASS
69	198	0.00	100	35.8	13409	PASS
70	69	0.00	2	1.8	241	PASS
127	198	10	80	46.3	17321	PASS
197	198	0.00	2	0.7	264	PASS
198	198	100	100	100.0	37450	PASS
199	198	5	9	6.6	2464	PASS
275	198	10	60	25.8	9667	PASS
365	198	1	100	2.6	985	PASS
441	442	0.01	24	16.6	5133	PASS
442	198	50	100	82.6	30944	PASS
443	442	15	24	18.3	5654	PASS