

Data File : BF093190.D
Acq On : 25 Feb 2017 14:00
Operator : SJ/MA
Sample : I1972-18
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
E2-B1-BASE2-02

Quant Time: Feb 26 23:42:47 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 17:31:55 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.83	152	148385	20.00	ng	-0.02
21) Naphthalene-d8	8.12	136	561298	20.00	ng	-0.02
38) Acenaphthene-d10	9.88	164	225083	20.00	ng	-0.01
63) Phenanthrene-d10	11.37	188	338825	20.00	ng	-0.01
75) Chrysene-d12	14.01	240	312456	20.00	ng	-0.01
86) Perylene-d12	15.45	264	240672	20.00	ng	0.00

System Monitoring Compounds						
5) 2-Fluorophenol	5.44	112	1126294	130.22	ng	-0.01
7) Phenol-d6	6.49	99	1620054	145.58	ng	0.00
23) Nitrobenzene-d5	7.41	82	1038477	103.03	ng	-0.01
41) 2,4,6-Tribromophenol	10.67	330	183649	112.81	ng	-0.01
44) 2-Fluorobiphenyl	9.21	172	1434771	115.48	ng	-0.01
78) Terphenyl-d14	12.96	244	903629	67.95	ng	-0.01

Target Compounds						Qvalue
10) Phenol	6.50	94	65185	5.01	ng	# 65
19) n-Nitroso-di-n-propylamine	7.40	70	141227	19.94	ng	# 82
25) Isophorone	7.41	82	959747	51.10	ng	# 65
31) Naphthalene	8.14	128	138938	4.88	ng	99
32) Benzoic acid	7.93	122	1523	7.43	ng	# 54
37) 2-Methylnaphthalene	8.83	142	78898	4.32	ng	98
48) Acenaphthylene	9.73	152	48659	2.21	ng	97
49) Dimethylphthalate	9.60	163	134443	8.87	ng	99
53) 2,4-Dinitrophenol	10.17	184	846	5.21	ng	# 69
54) Dibenzofuran	10.08	168	41006	2.33	ng	# 95
64) 4,6-Dinitro-2-methylphenol	10.69	198	1877	3.53	ng	# 4
66) 4-Bromophenyl-phenylether	10.67	248	13922	3.93	ng	# 1
69) Pentachlorophenol	11.16	266	881	7.65	ng	# 1
70) Phenanthrene	11.39	178	409882	21.11	ng	97
71) Anthracene	11.44	178	106171	5.45	ng	99
72) Carbazole	11.60	167	39010	2.09	ng	99
74) Fluoranthene	12.58	202	587186	29.33	ng	97
77) Pyrene	12.81	202	564640	24.15	ng	99
80) Benzo(a)anthracene	14.00	228	362409	18.96	ng	97
82) Chrysene	14.03	228	245352	13.71	ng	97
85) Indeno(1,2,3-cd)pyrene	16.85	276	101312	7.31	ng	96
87) Benzo(b)fluoranthene	15.04	252	436735	27.57	ng	97
88) Benzo(k)fluoranthene	15.04	252	436735	31.93	ng	# 96
89) Benzo(a)pyrene	15.38	252	203427	14.85	ng	# 95
90) Dibenzo(a,h)anthracene	16.85	278	29831	2.69	ng	# 81
91) Benzo(g,h,i)perylene	17.28	276	95481	8.53	ng	# 90

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BF093190.D

Acq On : 25 Feb 2017 14:00

Operator : SJ/MA

Sample : I1972-18

Misc :

ALS Vial : 43 Sample Multiplier: 1

Instrument :

BNA_F

ClientSampleId :

E2-B1-BASE2-02


Quant Time: Feb 26 23:42:47 2017


Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Feb 17 17:31:55 2017

Response via : Initial Calibration



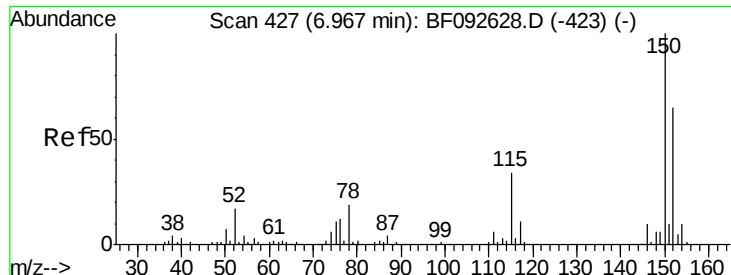

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.83 min Scan# 415

Delta R.T. -0.02 min

Lab File: BF093190.D

Acq: 25 Feb 2017 14:00

Instrument :

BNA_F

ClientSampleId :

E2-B1-BASE2-02


Tgt Ion:152 Resp: 148385

Ion Ratio Lower Upper

152 100

150 158.3 124.9 187.3




115 66.0 46.0 69.0



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E



#5

2-Fluorophenol

Concen: 130.22 ng

RT: 5.44 min Scan# 293

Delta R.T. -0.01 min

Lab File: BF093190.D

Acq: 25 Feb 2017 14:00


Tgt Ion:112 Resp: 1126294

Ion Ratio Lower Upper

112 100

64 65.3 46.1 69.1



63 32.2 23.8 35.6




Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0





#7

Phenol-d6

Concen: 145.58 ng

RT: 6.49 min Scan# 385

Delta R.T. -0.00 min

Lab File: BF093190.D

Acq: 25 Feb 2017 14:00

Instrument :

BNA_F

ClientSampleId :

E2-B1-BASE2-02


Tgt Ion: 99 Resp: 1620054

Ion Ratio Lower Upper

99 100

42 16.5 15.6 23.4




71 29.5 27.5 41.3



Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0



#10

Phenol

Concen: 5.01 ng

RT: 6.50 min Scan# 386

Delta R.T. -0.01 min

Lab File: BF093190.D

Acq: 25 Feb 2017 14:00


Tgt Ion: 94 Resp: 65185

Ion Ratio Lower Upper

94 100

65 25.0 21.4 61.4



66 32.5 44.0 84.0#



Abundance Ion 94.00 (93.70 to 94.70): BF0

Ion 65.00 (64.70 to 65.70): BF0

Ion 66.00 (65.70 to 66.70): BF0









#19
n-Nitroso-di-n-propylamine
Concen: 19.94 ng
RT: 7.40 min Scan# 465
Delta R.T. 0.13 min
Lab File: BF093190.D
Acq: 25 Feb 2017 14:00




Instrument :
BNA_F
ClientSampleId :
E2-B1-BASE2-02


Tgt Ion: 70 Resp: 141227
Ion Ratio Lower Upper
70 100
42 52.3 49.4 74.0
101 0.0 7.4 11.2#
130 1.8 14.2 21.4#



#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.12 min Scan# 528
Delta R.T. -0.02 min
Lab File: BF093190.D
Acq: 25 Feb 2017 14:00

Tgt Ion: 136 Resp: 561298
Ion Ratio Lower Upper
136 100
137 10.9 8.4 12.6
54 9.7 4.5 6.7#
68 7.1 3.6 5.4#





#23

Nitrobenzene-d5

Concen: 103.03 ng

RT: 7.41 min Scan# 466

Delta R.T. -0.01 min

Lab File: BF093190.D

Acq: 25 Feb 2017 14:00

Instrument :

BNA_F

ClientSampleId :

E2-B1-BASE2-02


Tgt Ion: 82 Resp: 1038477

Ion Ratio Lower Upper

82 100

128 53.0 34.6 52.0#




54 48.4 39.5 59.3



Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): BF0

Ion 54.00 (53.70 to 54.70): BF0



#25

Isophorone

Concen: 51.10 ng

RT: 7.41 min Scan# 466

Delta R.T. -0.27 min

Lab File: BF093190.D

Acq: 25 Feb 2017 14:00


Tgt Ion: 82 Resp: 959747

Ion Ratio Lower Upper

82 100

95 0.1 5.6 8.4#



138 0.0 14.6 22.0#




Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 95.00 (94.70 to 95.70): BF0

Ion 138.00 (137.70 to 138.70): BF0









#31
Naphthalene
Concen: 4.88 ng
RT: 8.14 min Scan# 530
Delta R.T. -0.02 min
Lab File: BF093190.D
Acq: 25 Feb 2017 14:00




Instrument :
BNA_F
ClientSampleId :
E2-B1-BASE2-02


Tgt Ion:128 Resp: 138938
Ion Ratio Lower Upper
128 100
129 11.0 9.5 14.3
127 13.6 10.8 16.2



#32
Benzoic acid
Concen: 7.43 ng
RT: 7.93 min Scan# 511
Delta R.T. -0.00 min
Lab File: BF093190.D
Acq: 25 Feb 2017 14:00

Tgt Ion:122 Resp: 1523
Ion Ratio Lower Upper
122 100
105 45.9 107.2 147.2#
77 107.8 74.5 114.5









#37
 2-Methylnaphthalene
 Concen: 4.32 ng
 RT: 8.83 min Scan# 590
 Delta R.T. -0.02 min
 Lab File: BF093190.D
 Acq: 25 Feb 2017 14:00

Instrument :
 BNA_F
 ClientSampleId :
 E2-B1-BASE2-02

Tgt Ion:142 Resp: 78898
 Ion Ratio Lower Upper
 142 100
 141 90.6 71.0 106.6
 115 34.4 28.3 42.5




Abundance Ion 142.00 (141.70 to 142.70): E
 Ion 141.00 (140.70 to 141.70): E
 Ion 115.00 (114.70 to 115.70): E






#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.88 min Scan# 682
 Delta R.T. -0.01 min
 Lab File: BF093190.D
 Acq: 25 Feb 2017 14:00

Tgt Ion:164 Resp: 225083
 Ion Ratio Lower Upper
 164 100
 162 108.0 80.2 120.2
 160 47.2 36.9 55.3



Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E









#41
 2,4,6-Tribromophenol
 Concen: 112.81 ng
 RT: 10.67 min Scan# 751
 Delta R.T. -0.01 min
 Lab File: BF093190.D
 Acq: 25 Feb 2017 14:00

Instrument :
 BNA_F
 ClientSampleId :
 E2-B1-BASE2-02

Tgt Ion:330 Resp: 183649
 Ion Ratio Lower Upper
 330 100
 332 96.8 77.4 116.2
 141 45.2 34.1 51.1




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E






#44
 2-Fluorobiphenyl
 Concen: 115.48 ng
 RT: 9.21 min Scan# 623
 Delta R.T. -0.01 min
 Lab File: BF093190.D
 Acq: 25 Feb 2017 14:00

Tgt Ion:172 Resp: 1434771
 Ion Ratio Lower Upper
 172 100
 171 36.1 29.4 44.0
 170 24.0 20.2 30.4



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E





#48

Acenaphthylene

Concen: 2.21 ng

RT: 9.73 min Scan# 669

Delta R.T. -0.02 min

Lab File: BF093190.D

Acq: 25 Feb 2017 14:00

Instrument :

BNA_F

ClientSampleId :

E2-B1-BASE2-02


Tgt Ion:152 Resp: 48659

Ion Ratio Lower Upper

152 100

151 20.4 16.9 25.3




153 16.6 11.4 17.2



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E



#49

Dimethylphthalate

Concen: 8.87 ng

RT: 9.60 min Scan# 657

Delta R.T. -0.02 min

Lab File: BF093190.D

Acq: 25 Feb 2017 14:00


Tgt Ion:163 Resp: 134443

Ion Ratio Lower Upper

163 100

194 3.5 3.0 4.4



164 9.5 8.0 12.0




Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E









#53
 2,4-Dinitrophenol
 Concen: 5.21 ng
 RT: 10.17 min Scan# 707
 Delta R.T. 0.21 min
 Lab File: BF093190.D
 Acq: 25 Feb 2017 14:00




Instrument :
 BNA_F
 ClientSampleId :
 E2-B1-BASE2-02


Tgt Ion:184 Resp: 846
 Ion Ratio Lower Upper
 184 100
 63 0.0 28.4 42.6#
 154 64.3 44.3 66.5



#54
 Dibenzofuran
 Concen: 2.33 ng
 RT: 10.08 min Scan# 699
 Delta R.T. -0.02 min
 Lab File: BF093190.D
 Acq: 25 Feb 2017 14:00

Tgt Ion:168 Resp: 41006
 Ion Ratio Lower Upper
 168 100
 139 40.9 32.6 49.0
 169 21.6 11.3 16.9#









#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.37 min Scan# 812
Delta R.T. -0.01 min
Lab File: BF093190.D
Acq: 25 Feb 2017 14:00




Instrument :
BNA_F
ClientSampleId :
E2-B1-BASE2-02


Tgt Ion:188 Resp: 338825
Ion Ratio Lower Upper
188 100
94 8.0 10.0 15.0#
80 8.1 11.2 16.8#



#64
4,6-Dinitro-2-methylphenol
Concen: 3.53 ng
RT: 10.69 min Scan# 753
Delta R.T. 0.19 min
Lab File: BF093190.D
Acq: 25 Feb 2017 14:00

Tgt Ion:198 Resp: 1877
Ion Ratio Lower Upper
198 100
51 71.5 6.7 46.7#
105 97.9 16.6 56.6#





#66

4-Bromophenyl-phenylether

Concen: 3.93 ng

RT: 10.67 min Scan# 751

Delta R.T. -0.25 min

Lab File: BF093190.D

Acq: 25 Feb 2017 14:00

Instrument :

BNA_F

ClientSampleId :

E2-B1-BASE2-02


Tgt Ion:248 Resp: 13922

Ion Ratio Lower Upper

248 100

250 207.1 76.9 115.3#




141 479.1 68.2 102.4#



Abundance Ion 248.00 (247.70 to 248.70): E

Ion 250.00 (249.70 to 250.70): E

Ion 141.00 (140.70 to 141.70): E



#69

Pentachlorophenol

Concen: 7.65 ng

RT: 11.16 min Scan# 794

Delta R.T. -0.02 min

Lab File: BF093190.D

Acq: 25 Feb 2017 14:00


Tgt Ion:266 Resp: 881

Ion Ratio Lower Upper

266 100

268 161.4 53.3 79.9#



264 0.0 50.3 75.5#




Abundance Ion 265.70 (265.40 to 266.40): E

Ion 268.00 (267.70 to 268.70): E

Ion 264.00 (263.70 to 264.70): E





#70

Phenanthrene

Concen: 21.11 ng

RT: 11.39 min Scan# 814

Delta R.T. -0.01 min

Lab File: BF093190.D

Acq: 25 Feb 2017 14:00

Instrument :

BNA_F

ClientSampleId :

E2-B1-BASE2-02


Tgt Ion:178 Resp: 409882

Ion Ratio Lower Upper

178 100

176 19.0 16.6 25.0




179 15.0 12.8 19.2



Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E



#71

Anthracene

Concen: 5.45 ng

RT: 11.44 min Scan# 818

Delta R.T. -0.02 min

Lab File: BF093190.D

Acq: 25 Feb 2017 14:00


Tgt Ion:178 Resp: 106171

Ion Ratio Lower Upper

178 100

176 20.5 15.9 23.9



179 16.2 13.2 19.8




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E





#72

Carbazole

Concen: 2.09 ng

RT: 11.60 min Scan# 832

Delta R.T. -0.01 min

Lab File: BF093190.D

Acq: 25 Feb 2017 14:00

Instrument :

BNA_F

ClientSampleId :

E2-B1-BASE2-02


Tgt Ion:167 Resp: 39010

Ion Ratio Lower Upper

167 100

166 23.2 18.2 27.2




139 13.8 11.4 17.2



Abundance Ion 167.00 (166.70 to 167.70): E

Ion 166.00 (165.70 to 166.70): E

Ion 139.00 (138.70 to 139.70): E



#74

Fluoranthene

Concen: 29.33 ng

RT: 12.58 min Scan# 918

Delta R.T. -0.01 min

Lab File: BF093190.D

Acq: 25 Feb 2017 14:00


Tgt Ion:202 Resp: 587186

Ion Ratio Lower Upper

202 100

101 13.6 0.0 34.6



203 17.4 0.0 38.7




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E





#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.01 min Scan# 1043

Delta R.T. -0.01 min

Lab File: BF093190.D

Acq: 25 Feb 2017 14:00

Instrument :

BNA_F

ClientSampleId :

E2-B1-BASE2-02


Tgt Ion:240 Resp: 312456

Ion Ratio Lower Upper

240 100

120 13.7 12.9 19.3




236 25.9 20.9 31.3



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E



#77

Pyrene

Concen: 24.15 ng

RT: 12.81 min Scan# 938

Delta R.T. -0.01 min

Lab File: BF093190.D

Acq: 25 Feb 2017 14:00


Tgt Ion:202 Resp: 564640

Ion Ratio Lower Upper

202 100

200 21.8 17.7 26.5



203 18.1 14.7 22.1




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E





#78

Terphenyl-d14

Concen: 67.95 ng

RT: 12.96 min Scan# 951

Delta R.T. -0.01 min

Lab File: BF093190.D

Acq: 25 Feb 2017 14:00

Instrument :

BNA_F

ClientSampleId :

E2-B1-BASE2-02


Tgt Ion:244 Resp: 903629

Ion Ratio Lower Upper

244 100

212 6.9 6.2 9.2




122 9.6 11.4 17.2#



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E



#80

Benzo(a)anthracene

Concen: 18.96 ng

RT: 14.00 min Scan# 1042

Delta R.T. -0.01 min

Lab File: BF093190.D

Acq: 25 Feb 2017 14:00


Tgt Ion:228 Resp: 362409

Ion Ratio Lower Upper

228 100

226 30.0 22.4 33.6



229 21.2 16.2 24.4




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E





#82

Chrysene

Concen: 13.71 ng

RT: 14.03 min Scan# 1045

Delta R.T. -0.01 min

Lab File: BF093190.D

Acq: 25 Feb 2017 14:00

Instrument :

BNA_F

ClientSampleId :

E2-B1-BASE2-02


Tgt Ion:228 Resp: 245352

Ion Ratio Lower Upper

228 100

226 31.0 25.4 38.0




229 22.5 16.2 24.2



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E



#85

Indeno(1,2,3-cd)pyrene

Concen: 7.31 ng

RT: 16.85 min Scan# 1292

Delta R.T. -0.00 min

Lab File: BF093190.D

Acq: 25 Feb 2017 14:00


Tgt Ion:276 Resp: 101312

Ion Ratio Lower Upper

276 100

138 28.7 21.8 32.6



277 22.5 20.2 30.4




Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E









#86
Perylene-d12
Concen: 20.00 ng
RT: 15.45 min Scan# 1169
Delta R.T. -0.00 min
Lab File: BF093190.D
Acq: 25 Feb 2017 14:00




Instrument :
BNA_F
ClientSampleId :
E2-B1-BASE2-02


Tgt Ion: 264 Resp: 240672
Ion Ratio Lower Upper
264 100
260 24.2 19.2 28.8
265 21.9 17.4 26.0



#87
Benzo(b)fluoranthene
Concen: 27.57 ng
RT: 15.04 min Scan# 1133
Delta R.T. -0.00 min
Lab File: BF093190.D
Acq: 25 Feb 2017 14:00

Tgt Ion: 252 Resp: 436735
Ion Ratio Lower Upper
252 100
253 22.2 18.2 27.4
125 14.3 9.8 14.6









#88
Benzo(k)fluoranthene
Concen: 31.93 ng
RT: 15.04 min Scan# 1133
Delta R.T. -0.03 min
Lab File: BF093190.D
Acq: 25 Feb 2017 14:00




Instrument :
BNA_F
ClientSampleId :
E2-B1-BASE2-02


Tgt Ion:252 Resp: 436735
Ion Ratio Lower Upper
252 100
253 22.2 18.5 27.7
125 14.3 8.9 13.3#



#89
Benzo(a)pyrene
Concen: 14.85 ng
RT: 15.38 min Scan# 1163
Delta R.T. -0.01 min
Lab File: BF093190.D
Acq: 25 Feb 2017 14:00

Tgt Ion:252 Resp: 203427
Ion Ratio Lower Upper
252 100
253 23.4 18.2 27.2
125 17.4 10.0 15.0#









#90
Dibenzo(a,h)anthracene
Concen: 2.69 ng
RT: 16.85 min Scan# 1292
Delta R.T. -0.01 min
Lab File: BF093190.D
Acq: 25 Feb 2017 14:00

Instrument :
BNA_F
ClientSampleId :
E2-B1-BASE2-02

Tgt Ion	Ratio	Lower	Upper
278	100		
139	30.6	14.8	22.2#
279	31.3	19.8	29.6#



#91
Benzo(g,h,i)perylene
Concen: 8.53 ng
RT: 17.28 min Scan# 1329
Delta R.T. -0.01 min
Lab File: BF093190.D
Acq: 25 Feb 2017 14:00

Tgt Ion	Ratio	Lower	Upper
276	100		
277	23.6	19.2	28.8
138	29.2	16.0	24.0#

