

Data Path : Z:\HPCHEM1\BNA F\DATA\BF022417\
 Data File : BF093158.D
 Acq On : 24 Feb 2017 21:35
 Operator : SJ/MA
 Sample : I1957-10
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SRI-SB-5(13-15)20170222

Quant Time: Feb 24 22:33:57 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF013017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 17 17:31:55 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.83	152	152223	20.00	ng	-0.02
21) Naphthalene-d8	8.12	136	598974	20.00	ng	-0.02
38) Acenaphthene-d10	9.87	164	285160	20.00	ng	-0.02
63) Phenanthrene-d10	11.36	188	517058	20.00	ng	-0.02
75) Chrysene-d12	14.00	240	457070	20.00	ng	-0.02
86) Perylene-d12	15.43	264	339315	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.44	112	1389741	156.63	ng	-0.01
7) Phenol-d6	6.48	99	1574688	137.93	ng	-0.01
23) Nitrobenzene-d5	7.40	82	972306	90.40	ng	-0.02
41) 2,4,6-Tribromophenol	10.67	330	347616	168.54	ng	-0.01
44) 2-Fluorobiphenyl	9.20	172	1562072	99.24	ng	-0.02
78) Terphenyl-d14	12.96	244	1577663	81.10	ng	-0.01
Target Compounds						
10) Phenol	6.49	94	57518	4.31	ng	Qvalue # 70
49) Dimethylphthalate	9.60	163	418685	21.80	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF022417\
Data File : BF093158.D
Acq On : 24 Feb 2017 21:35
Operator : SJ/MA
Sample : I1957-10
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SRI-SB-5(13-15)20170222

Quant Time: Feb 24 22:33:57 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 17:31:55 2017
Response via : Initial Calibration

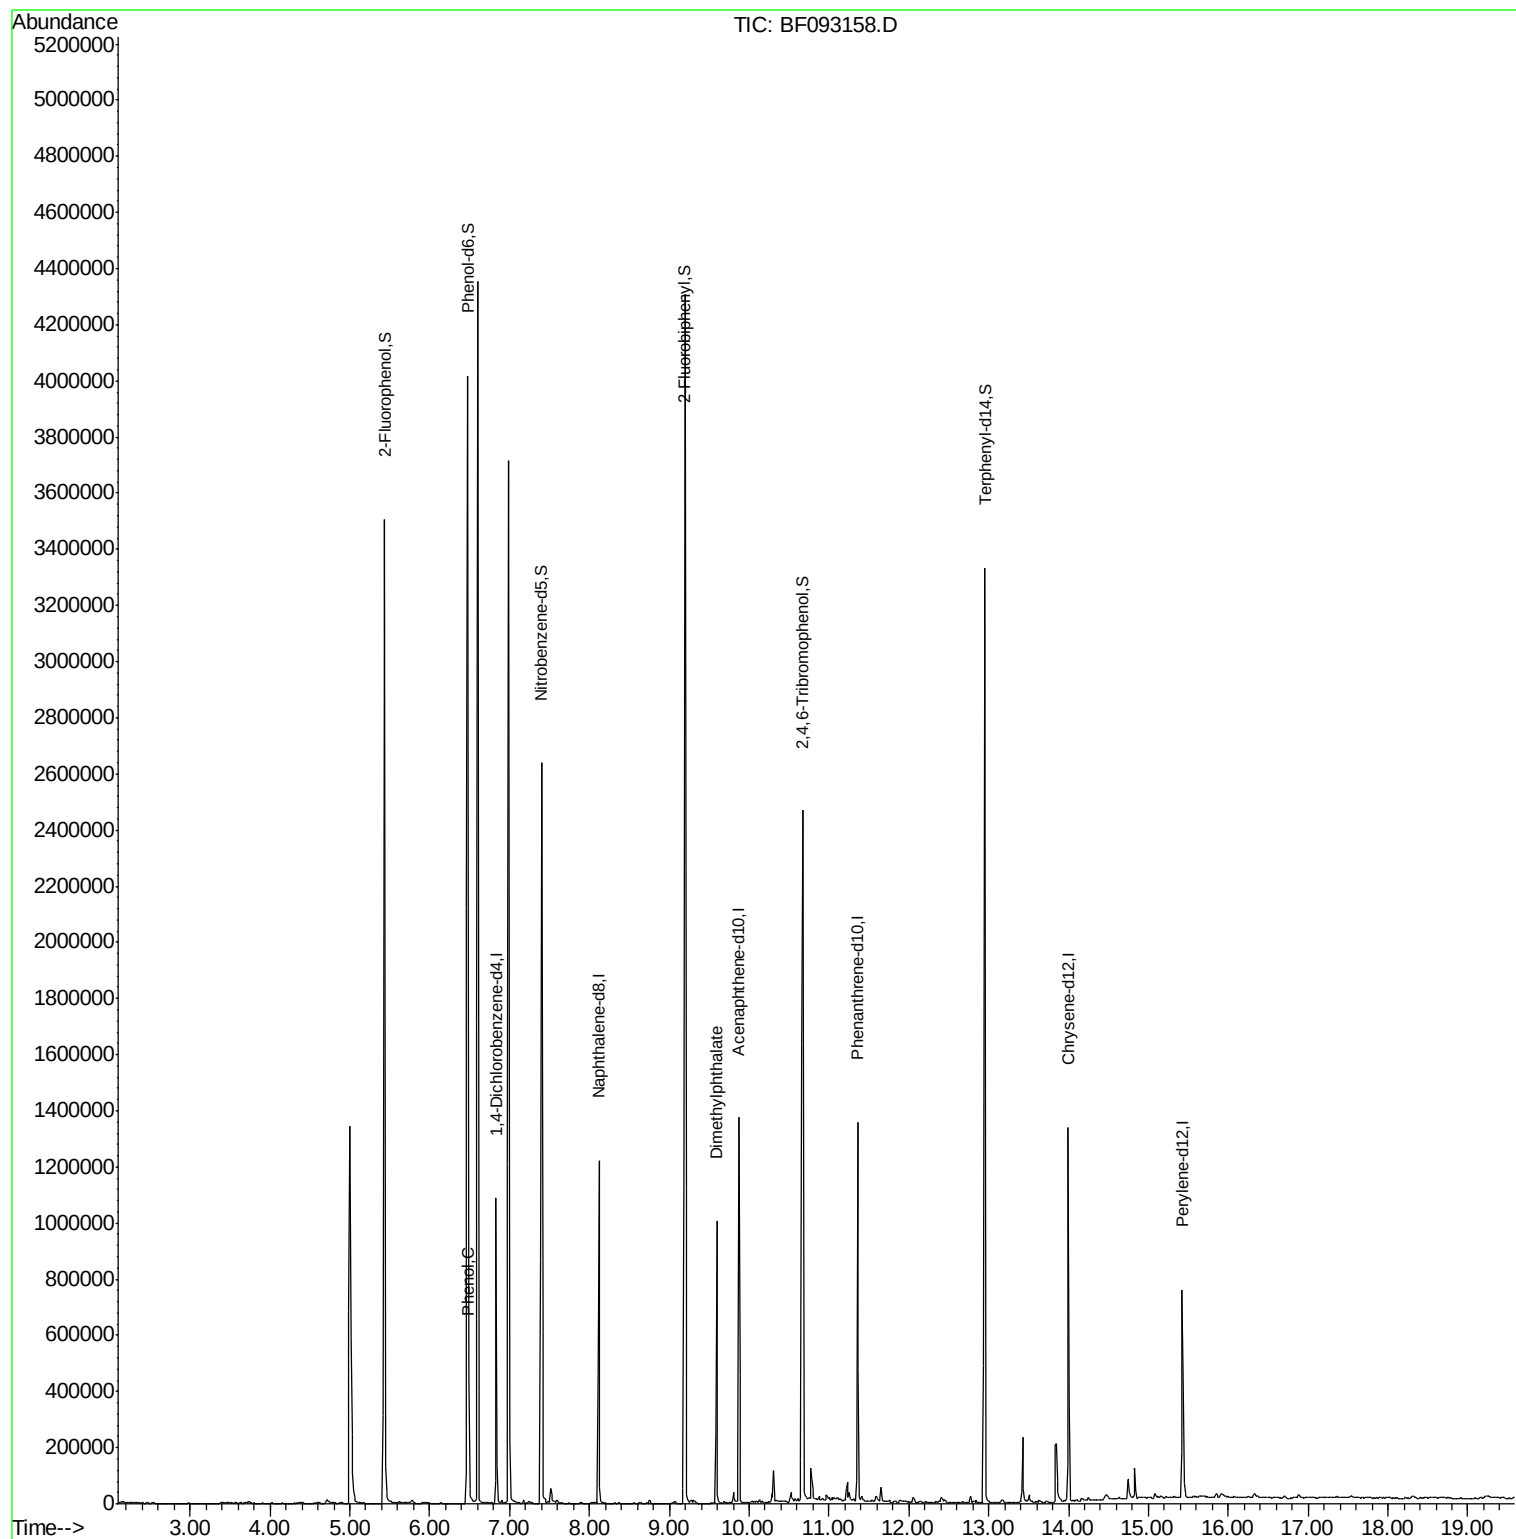

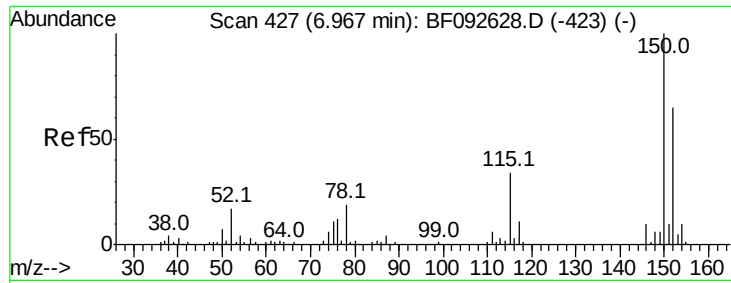


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.83 min Scan# 415
Delta R.T. -0.02 min
Lab File: BF093158.D
Acq: 24 Feb 2017 21:35

Instrument :
BNA_F
ClientSampleId :
SRI-SB-5(13-15)20170222

Tot Ion:152 Resp: 152223
Ion Ratio Lower Upper
152 100
150 155.0 124.9 187.3
115 61.0 46.0 69.0

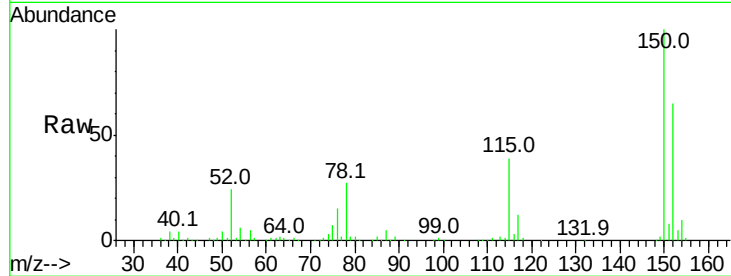


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

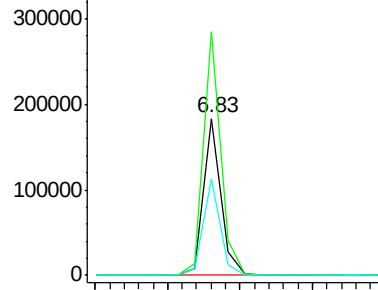



#5


2-Fluorophenol
Concen: 156.63 ng
RT: 5.44 min Scan# 293
Delta R.T. -0.01 min
Lab File: BF093158.D
Acq: 24 Feb 2017 21:35

Tgt Ion:112 Resp: 1389741
Ion Ratio Lower Upper
112 100
64 56.1 46.1 69.1
63 27.5 23.8 35.6



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

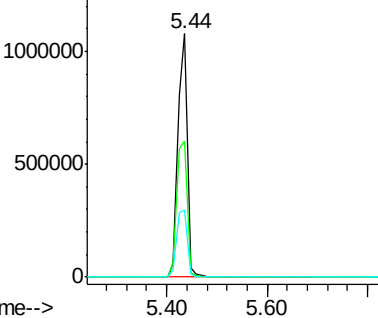

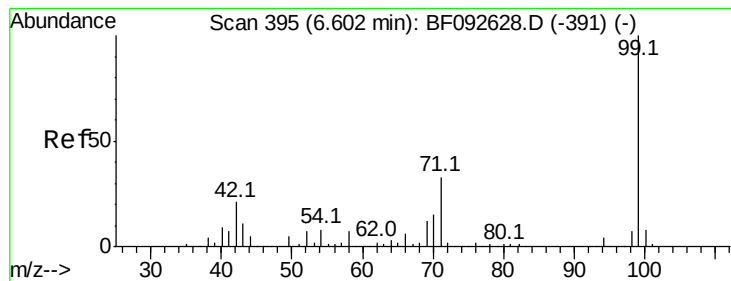

#7

Phenol-d6

Concen: 137.93 ng

RT: 6.48 min Scan# 384

Delta R.T. -0.01 min

Lab File: BF093158.D

Acq: 24 Feb 2017 21:35

Instrument :

BNA_F

ClientSampleId :

SRI-SB-5(13-15)20170222


Tot Ion: 99 Resp: 1574688

Ion Ratio Lower Upper

99 100

42 19.6 15.6 23.4




71 32.9 27.5 41.3



Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

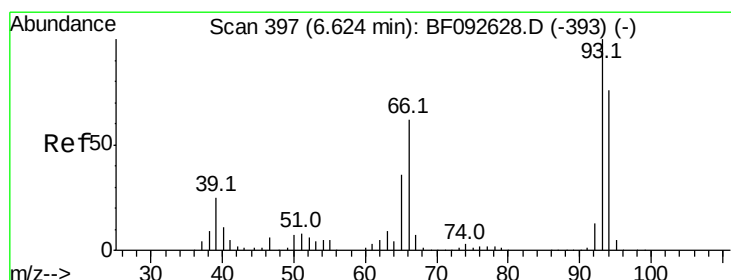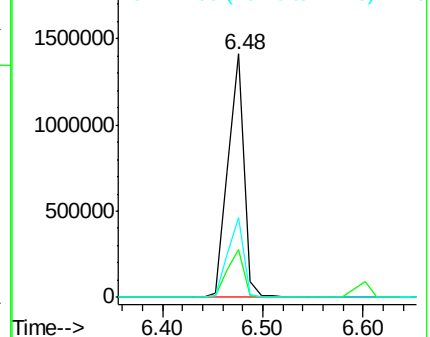

#10

Phenol

Concen: 4.31 ng

RT: 6.49 min Scan# 385

Delta R.T. -0.02 min

Lab File: BF093158.D

Acq: 24 Feb 2017 21:35


Tgt Ion: 94 Resp: 57518

Ion Ratio Lower Upper

94 100

65 26.3 21.4 61.4



66 37.2 44.0 84.0#




Abundance Ion 94.00 (93.70 to 94.70): BF0

Ion 65.00 (64.70 to 65.70): BF0

Ion 66.00 (65.70 to 66.70): BF0

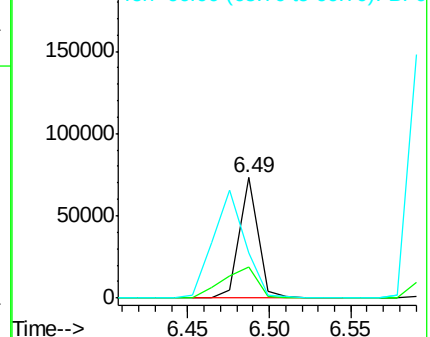


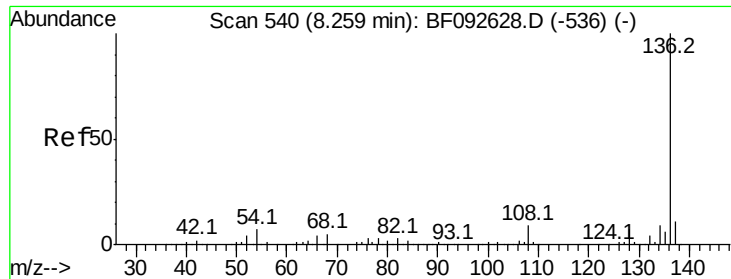




#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.12 min Scan# 528
Delta R.T. -0.02 min
Lab File: BF093158.D
Acq: 24 Feb 2017 21:35

Instrument :
BNA_F
ClientSampleId :
SRI-SB-5(13-15)20170222

Tot Ion:136	Resp:	598974
Ion Ratio	Lower	Upper
136	100	
137	10.9	8.4 12.6
54	8.2	4.5 6.7#
68	6.1	3.6 5.4#




Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0

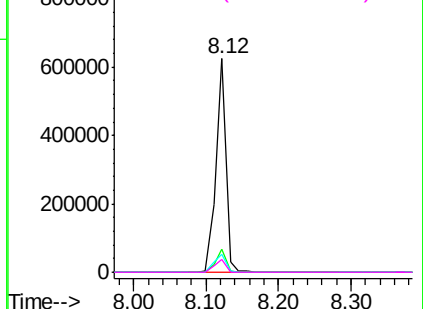




#23
Nitrobenzene-d5
Concen: 90.40 ng
RT: 7.40 min Scan# 465
Delta R.T. -0.02 min
Lab File: BF093158.D
Acq: 24 Feb 2017 21:35

Tgt Ion: 82	Resp:	972306
Ion Ratio	Lower	Upper
82	100	
128	41.7	34.6 52.0
54	57.8	39.5 59.3



Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0

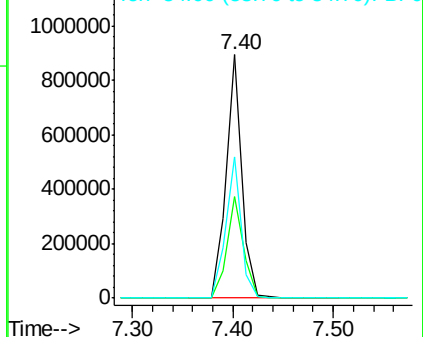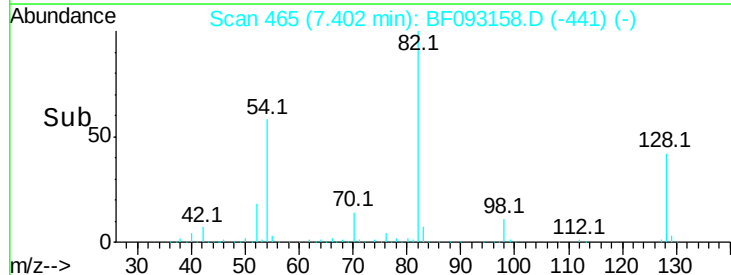







#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.87 min Scan# 681
 Delta R.T. -0.02 min
 Lab File: BF093158.D
 Acq: 24 Feb 2017 21:35

Instrument :
 BNA_F
 ClientSampleId :
 SRI-SB-5(13-15)20170222

Tot Ion:164 Resp: 285160
 Ion Ratio Lower Upper
 164 100
 162 100.5 80.2 120.2
 160 43.0 36.9 55.3

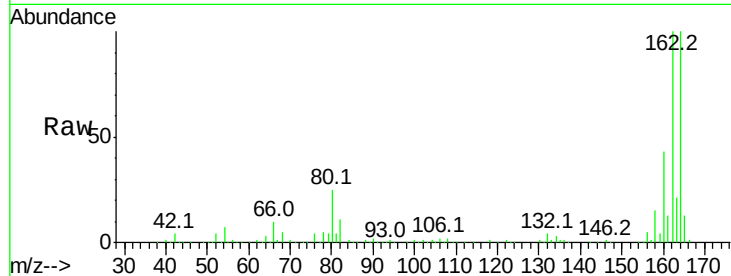


Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

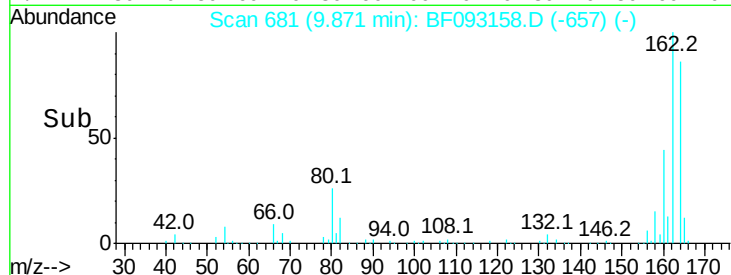
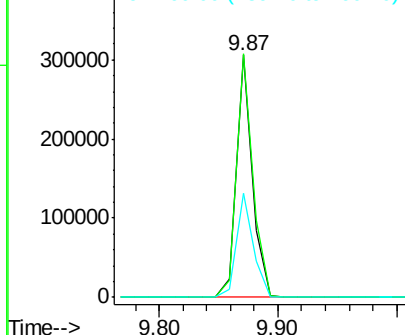



#41
 2,4,6-Tribromophenol
 Concen: 168.54 ng
 RT: 10.67 min Scan# 751
 Delta R.T. -0.01 min
 Lab File: BF093158.D
 Acq: 24 Feb 2017 21:35

Tgt Ion:330 Resp: 347616
 Ion Ratio Lower Upper
 330 100
 332 97.3 77.4 116.2
 141 39.0 34.1 51.1

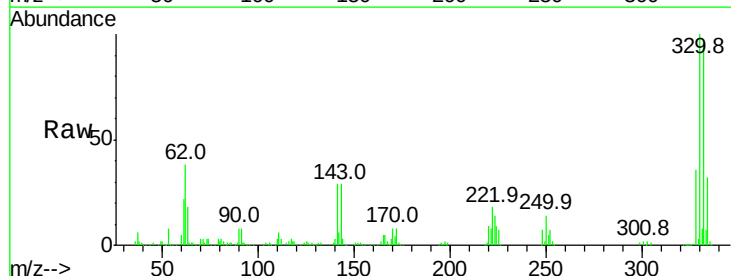

Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

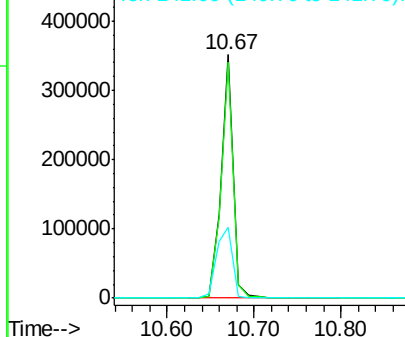




#44
 2-Fluorobiphenyl
 Concen: 99.24 ng
 RT: 9.20 min Scan# 622
 Delta R.T. -0.02 min
 Lab File: BF093158.D
 Acq: 24 Feb 2017 21:35




Instrument :
 BNA_F
 ClientSampleId :
 SRI-SB-5(13-15)20170222

Tot Ion:172 Resp: 1562072

Ion	Ratio	Lower	Upper
172	100		
171	36.7	29.4	44.0
170	24.8	20.2	30.4




Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

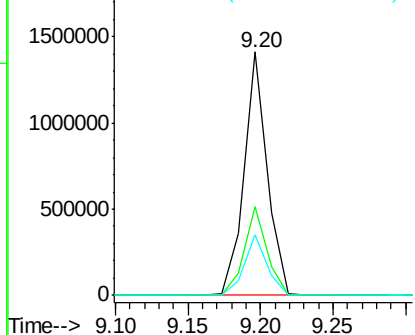



#49
 Dimethylphthalate
 Concen: 21.80 ng
 RT: 9.60 min Scan# 657
 Delta R.T. -0.02 min
 Lab File: BF093158.D
 Acq: 24 Feb 2017 21:35


Tgt Ion:163 Resp: 418685

Ion	Ratio	Lower	Upper
163	100		
194	3.6	3.0	4.4
164	9.6	8.0	12.0



Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

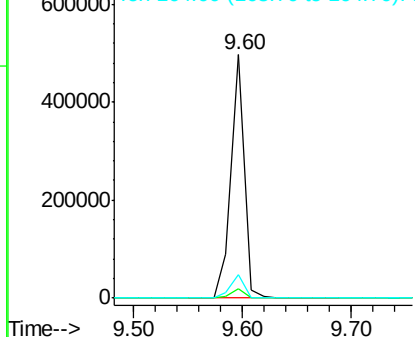


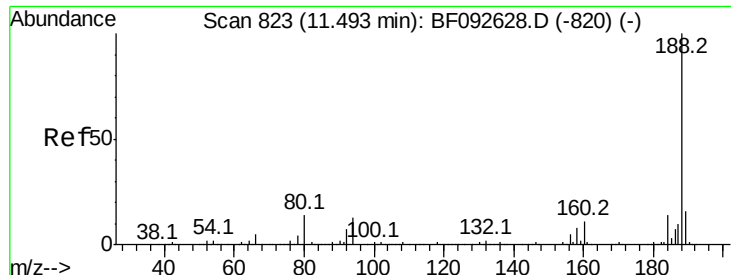




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.36 min Scan# 811
Delta R.T. -0.02 min
Lab File: BF093158.D
Acq: 24 Feb 2017 21:35

Instrument :
BNA_F
ClientSampleId :
SRI-SB-5(13-15)20170222

Tot Ion:188 Resp: 517058
Ion Ratio Lower Upper
188 100
94 13.1 10.0 15.0
80 14.8 11.2 16.8

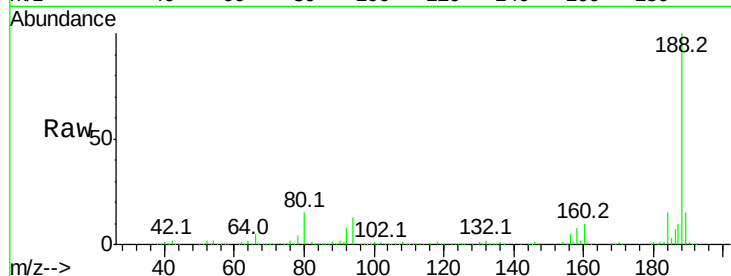


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

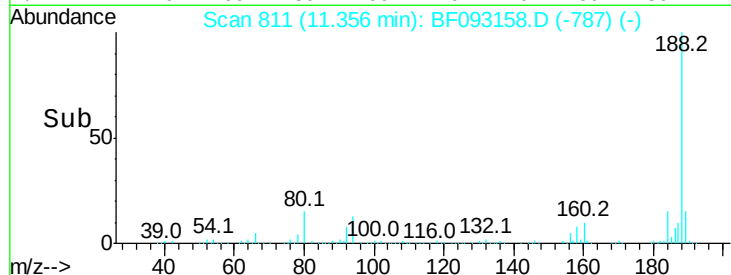
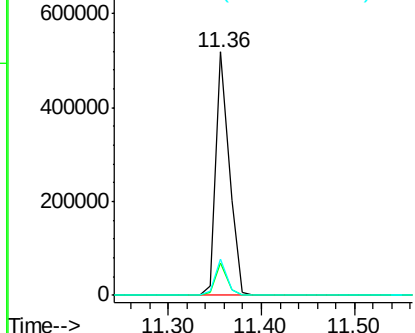



#75
Chrysene-d12
Concen: 20.00 ng
RT: 14.00 min Scan# 1042
Delta R.T. -0.02 min
Lab File: BF093158.D
Acq: 24 Feb 2017 21:35

Tgt Ion:240 Resp: 457070
Ion Ratio Lower Upper
240 100
120 16.0 12.9 19.3
236 26.0 20.9 31.3

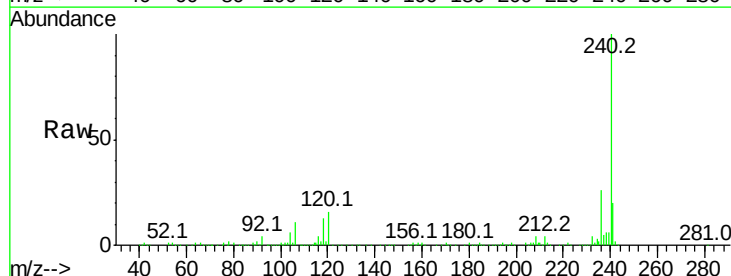

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

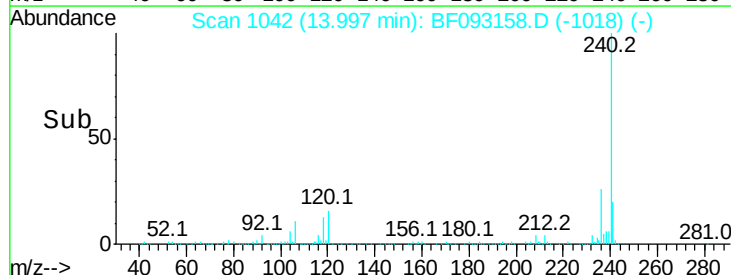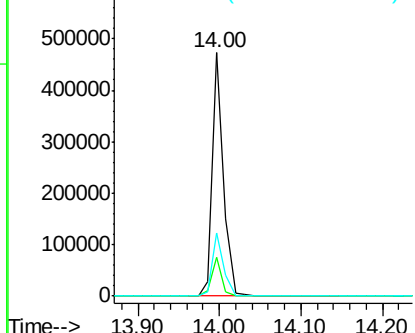



#78

Terphenyl-d14

Concen: 81.10 ng

RT: 12.96 min Scan# 951

Delta R.T. -0.01 min

Lab File: BF093158.D

Acq: 24 Feb 2017 21:35

Instrument :

BNA_F

ClientSampleId :

SRI-SB-5(13-15)20170222

Tot Ion:244 Resp: 1577663

Ion Ratio Lower Upper

244 100

212 7.1


6.2

9.2

122 7.7

11.4




17.2#



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

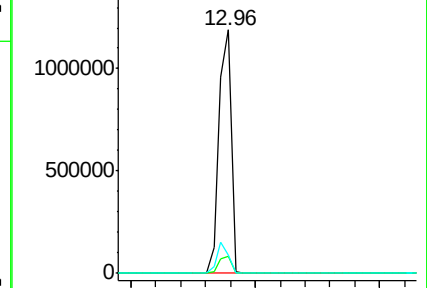

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.43 min Scan# 1167

Delta R.T. -0.02 min

Lab File: BF093158.D

Acq: 24 Feb 2017 21:35

Tgt Ion:264 Resp: 339315

Ion Ratio Lower Upper

264 100

260 23.6


19.2

28.8

265 21.0

17.4

26.0



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

