


Data Path : Z:\HPCHEM1\BNA_F\Data\BF022417\
Data File : BF093171.D
Acq On : 25 Feb 2017 5:07
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Feb 17 17:31:55 2017

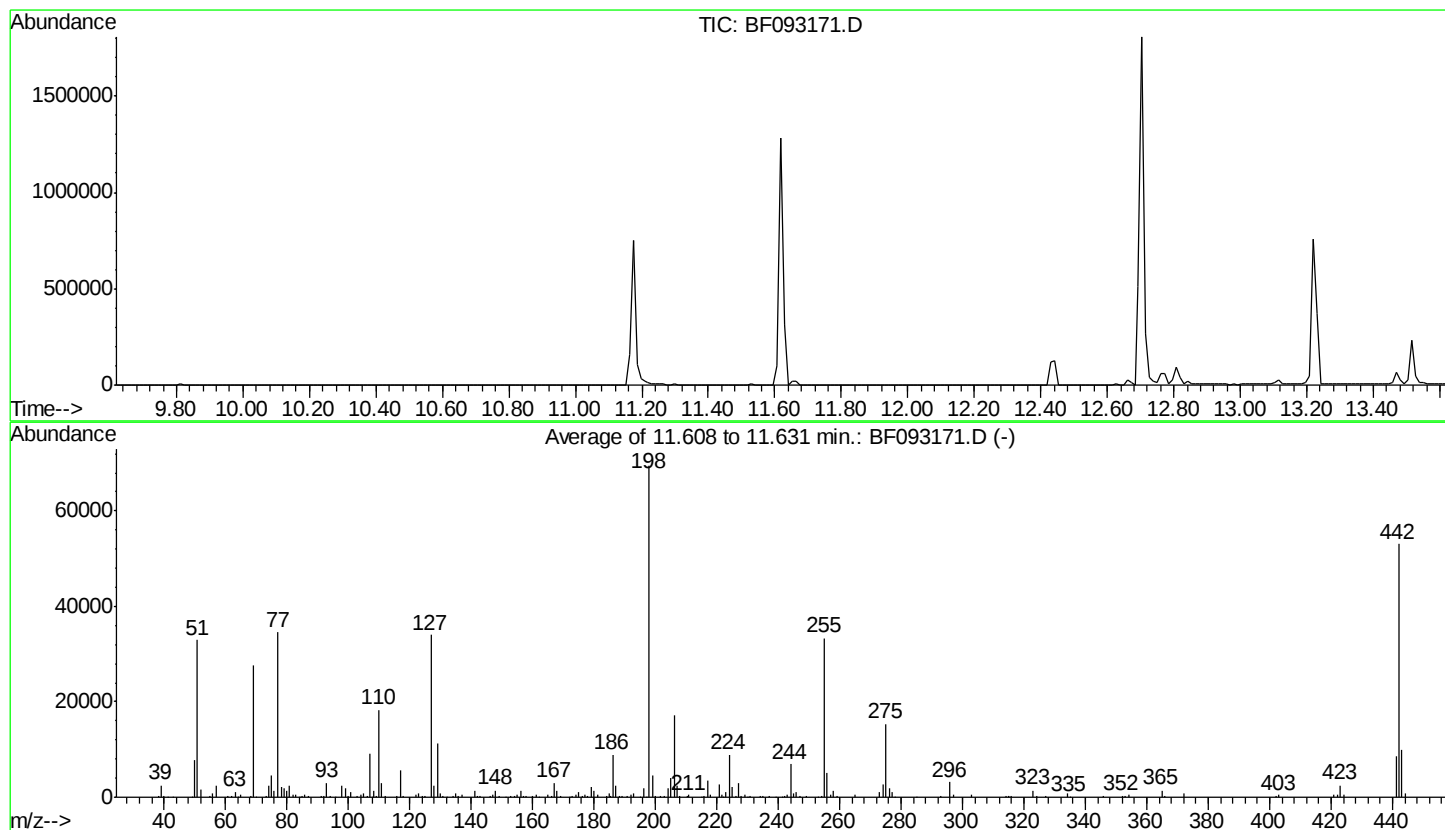

AutoFind: Scans 833, 834, 835; Background Corrected with Scan 830

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.4	32958	PASS
68	69	0.00	2	1.3	348	PASS
69	198	0.00	100	39.8	27631	PASS
70	69	0.00	2	0.5	140	PASS
127	198	10	80	48.9	33967	PASS
197	198	0.00	2	0.2	118	PASS
198	198	100	100	100.0	69502	PASS
199	198	5	9	6.6	4621	PASS
275	198	10	60	22.2	15410	PASS
365	198	1	100	2.1	1476	PASS
441	442	0.01	24	16.0	8467	PASS
442	198	50	100	76.3	53021	PASS
443	442	15	24	18.8	9994	PASS