
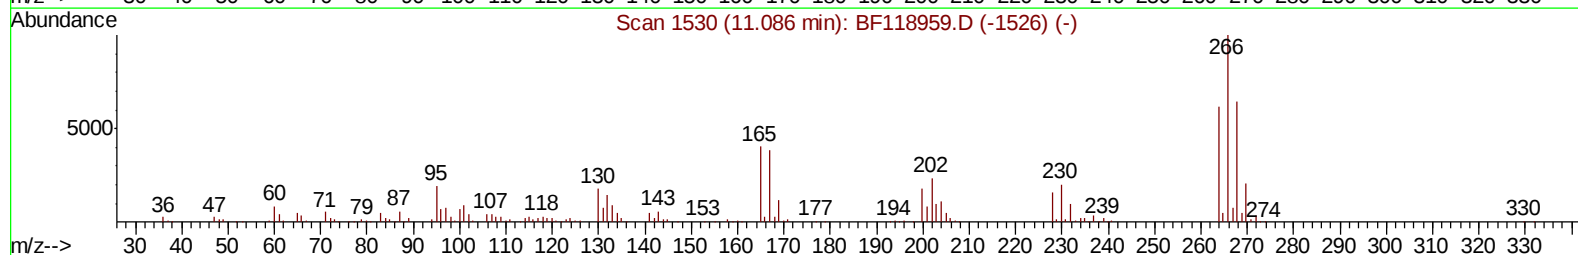
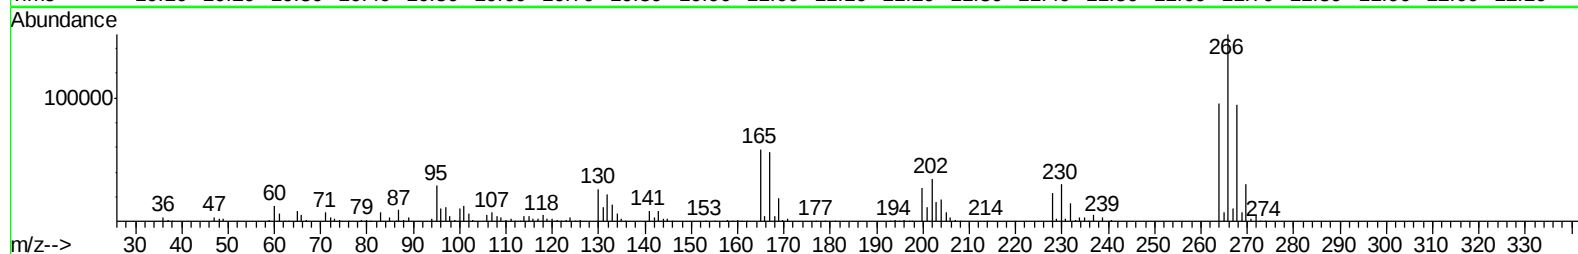


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF022420\  
Data File : BF119013.D  
Acq On : 24 Feb 2020 9:42  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 25 06:57:37 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022020.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Feb 20 17:40:17 2020  
Response via : Initial Calibration

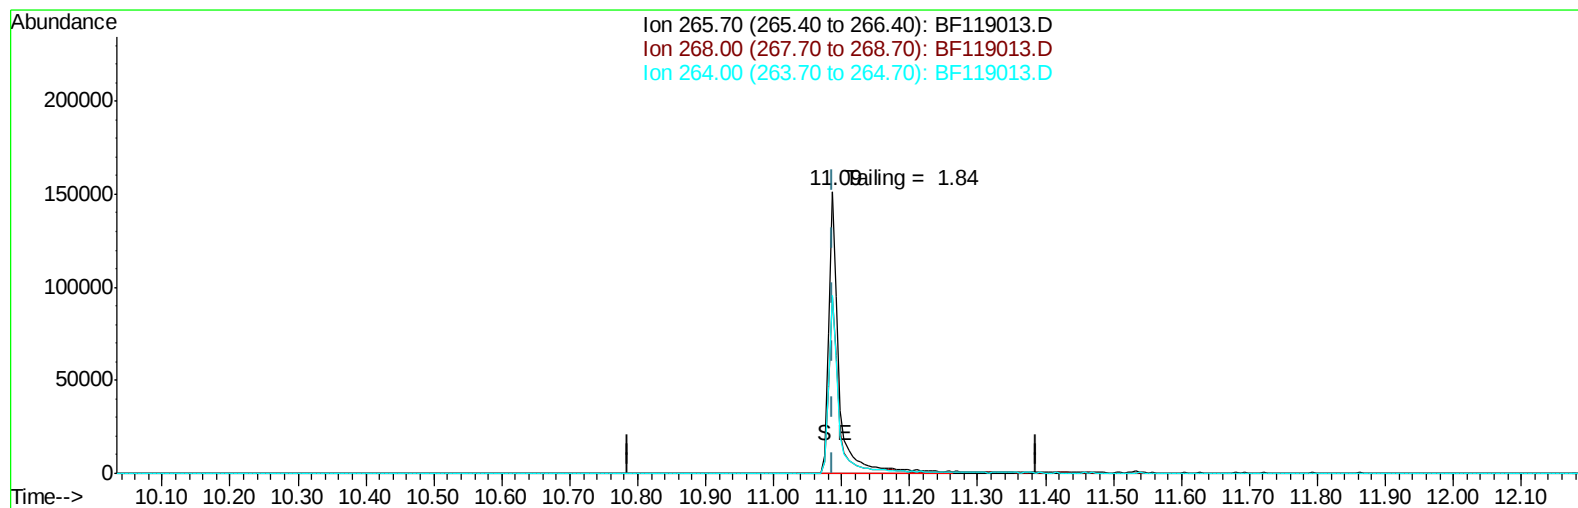

TIC: BF119013.D

(70) Pentachlorophenol (C)




11.086min (-0.000) 29283.80ng

response 158042

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 64.20 | 62.75 |
| 264.00 | 61.90 | 63.02 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF022420\  
 Data File : BF119013.D  
 Acq On : 24 Feb 2020 9:42  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 25 06:57:37 2020  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022020.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Feb 20 17:40:17 2020  
 Response via : Initial Calibration

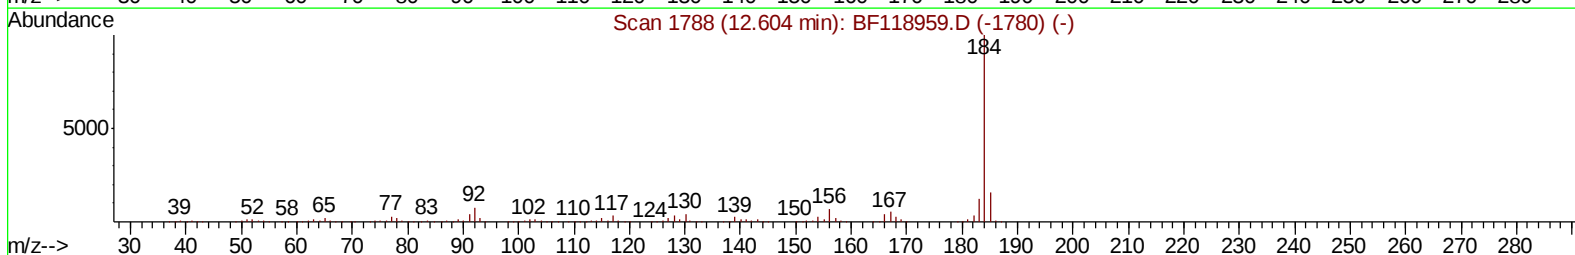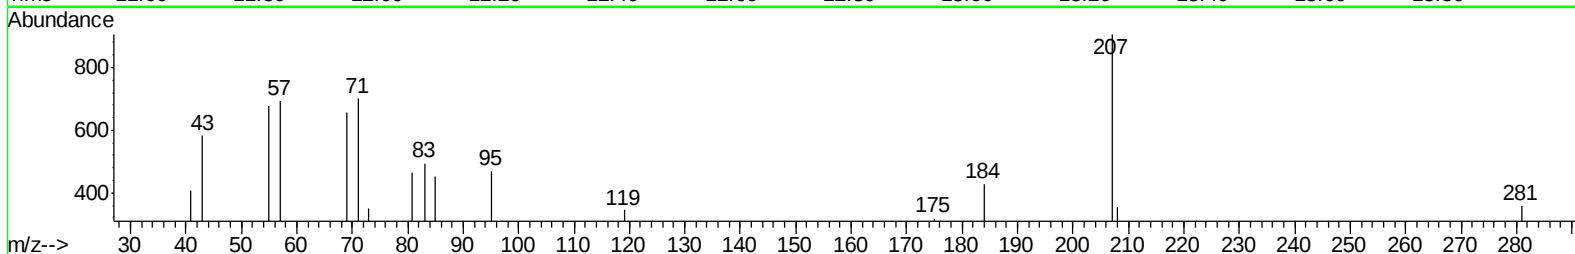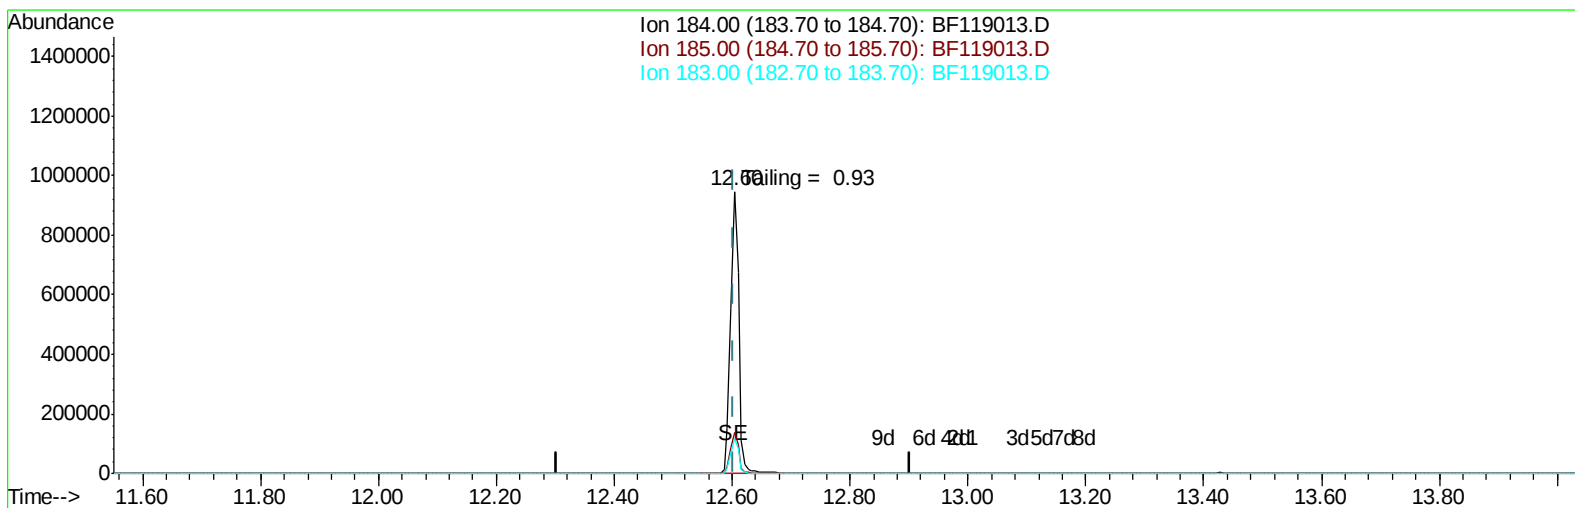

TIC: BF119013.D

(77) Benzidine

13.010min (+0.406) 111.85ng

response 514

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.80 | 0.00# |
| 183.00 | 12.40 | 0.00# |
| 0.00   | 0.00  | 0.00  |