
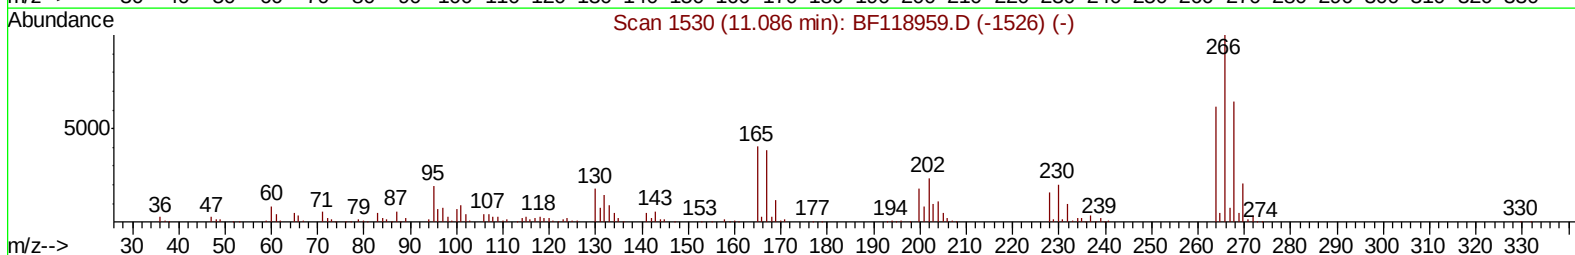
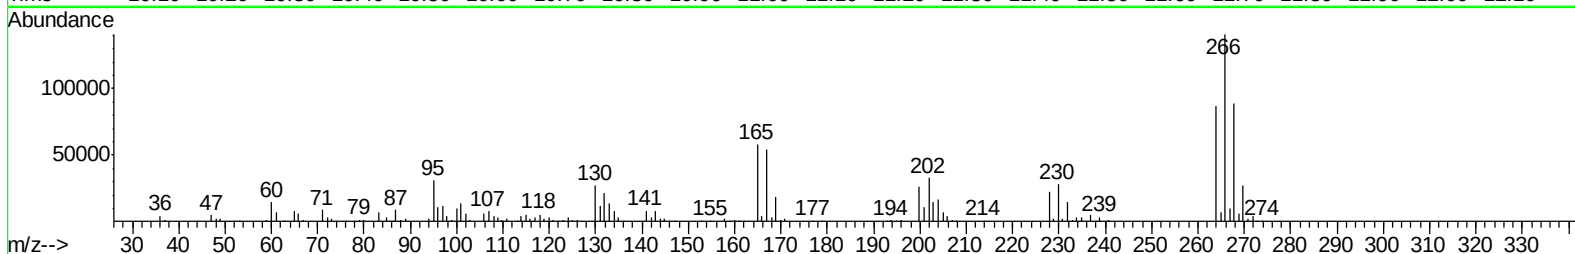


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF022420\
Data File : BF119026.D
Acq On : 24 Feb 2020 17:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 25 06:58:48 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 20 17:40:17 2020
Response via : Initial Calibration

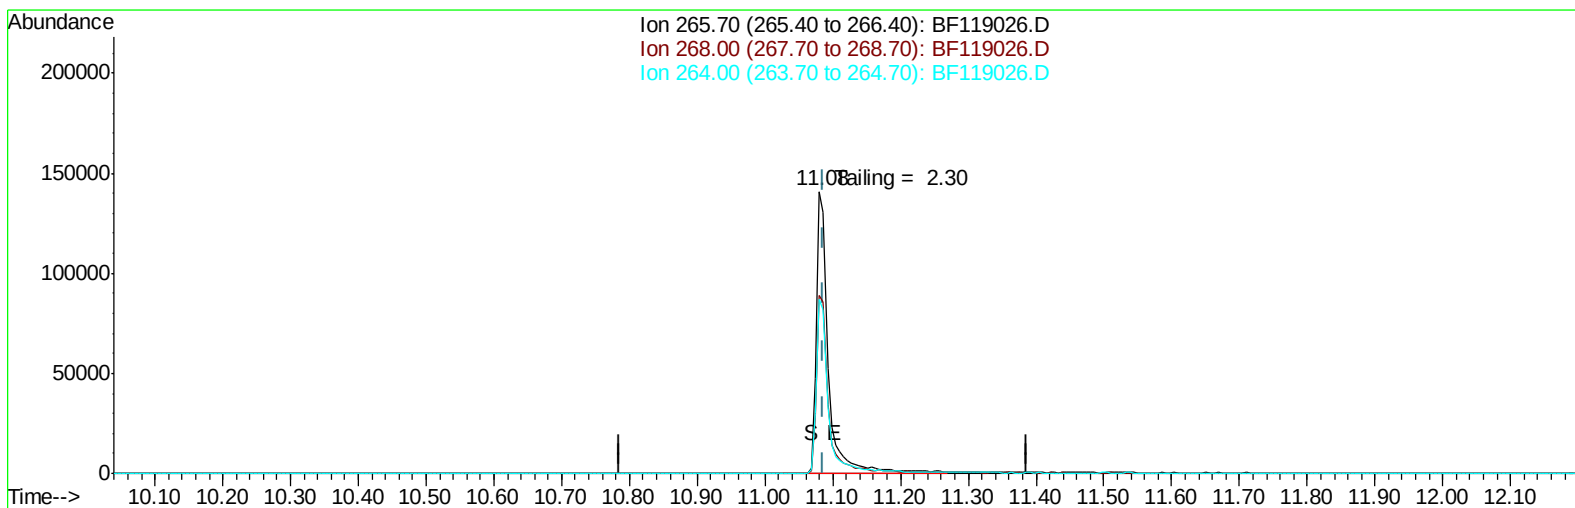

TIC: BF119026.D

(70) Pentachlorophenol (C)




11.080min (-0.006) 36464.58ng

response 166690

Ion	Exp%	Act%
265.70	100	100
268.00	64.20	63.07
264.00	61.90	61.66
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF022420\
 Data File : BF119026.D
 Acq On : 24 Feb 2020 17:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 25 06:58:48 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 20 17:40:17 2020
 Response via : Initial Calibration

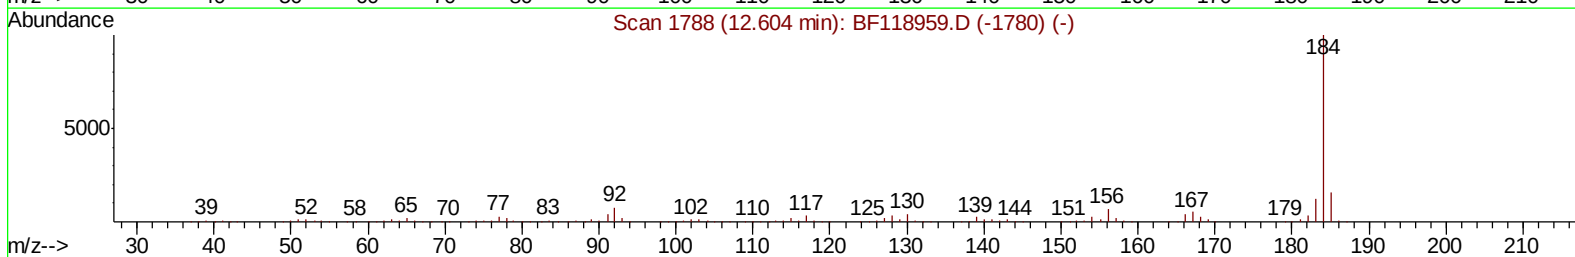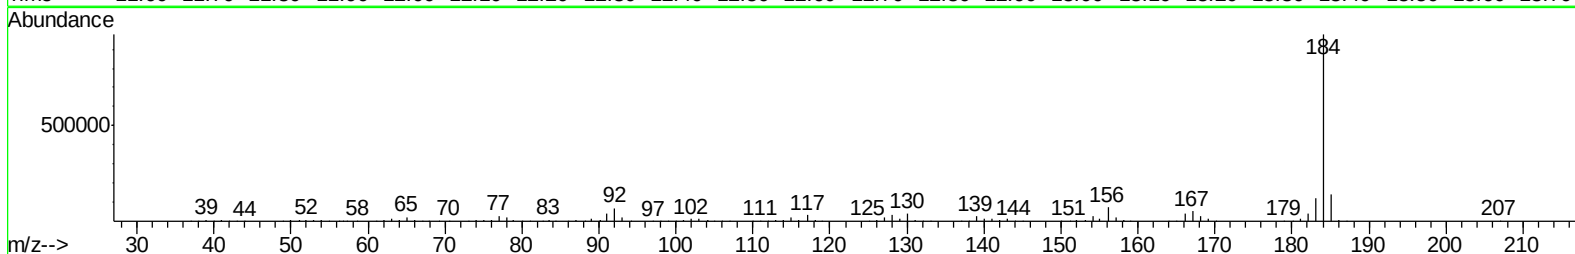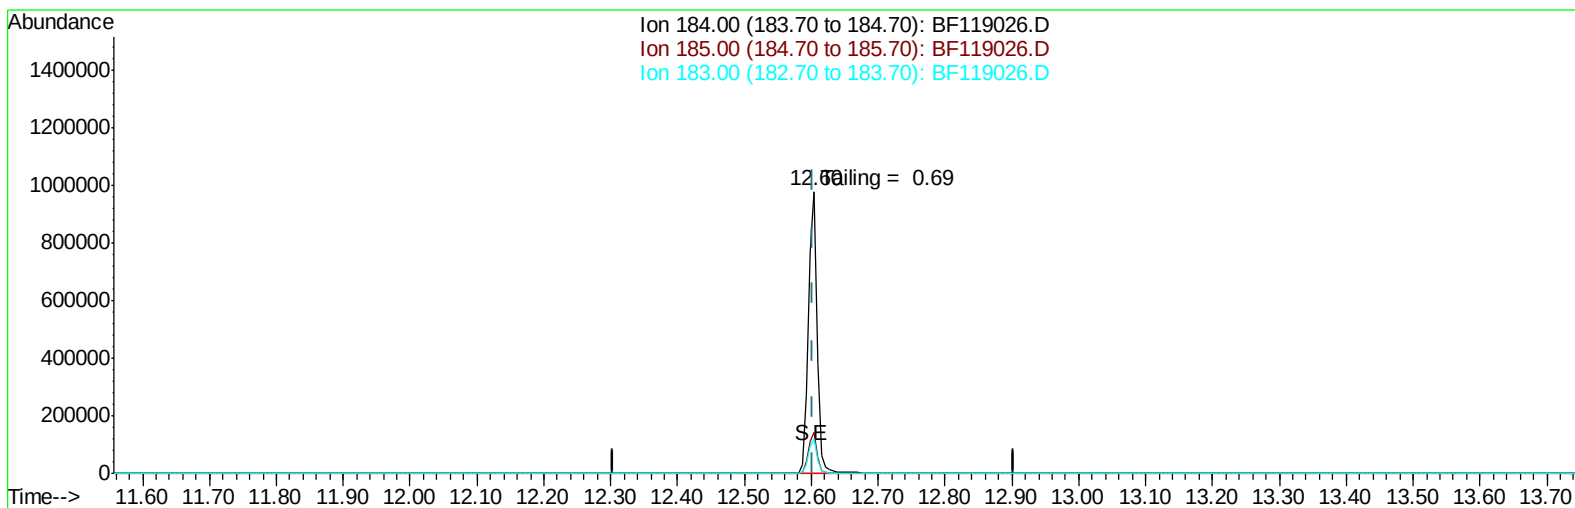

TIC: BF119026.D

(77) Benzidine

12.604min (-0.000) 0.00ng

response 909906

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	14.46
183.00	12.40	12.45
0.00	0.00	0.00