
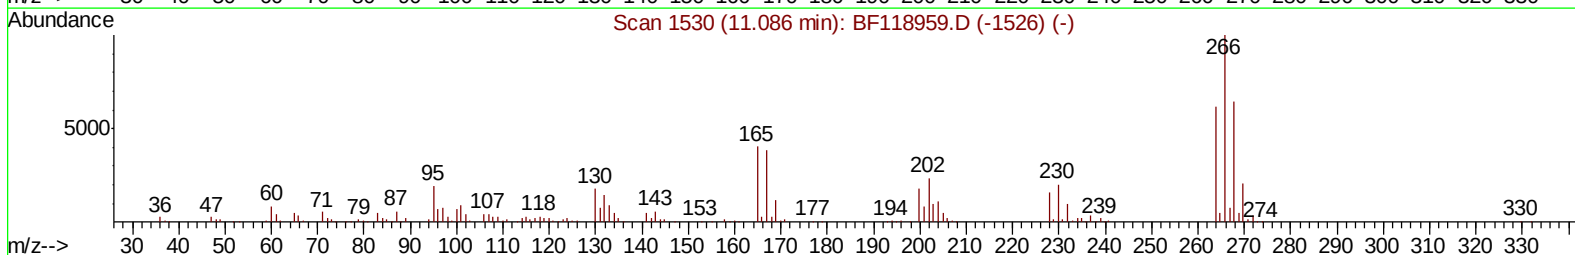
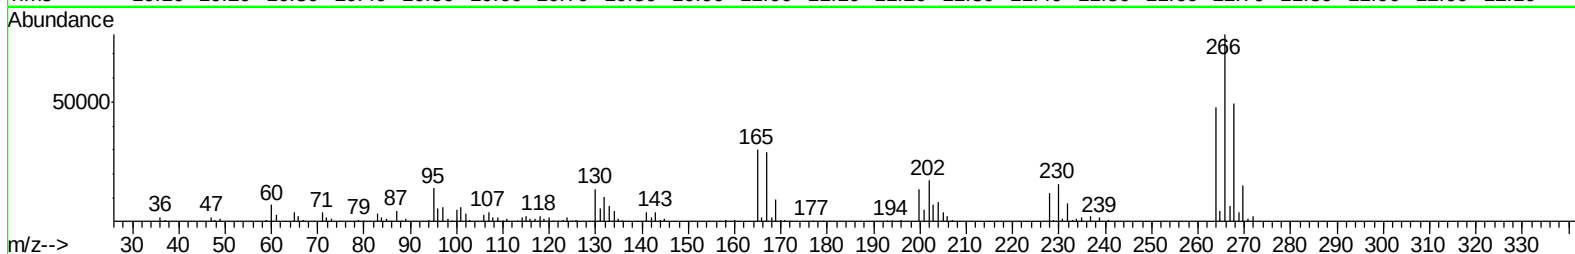


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF022420\
 Data File : BF119051.D
 Acq On : 25 Feb 2020 6:16
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 25 06:59:39 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 20 17:40:17 2020
 Response via : Initial Calibration

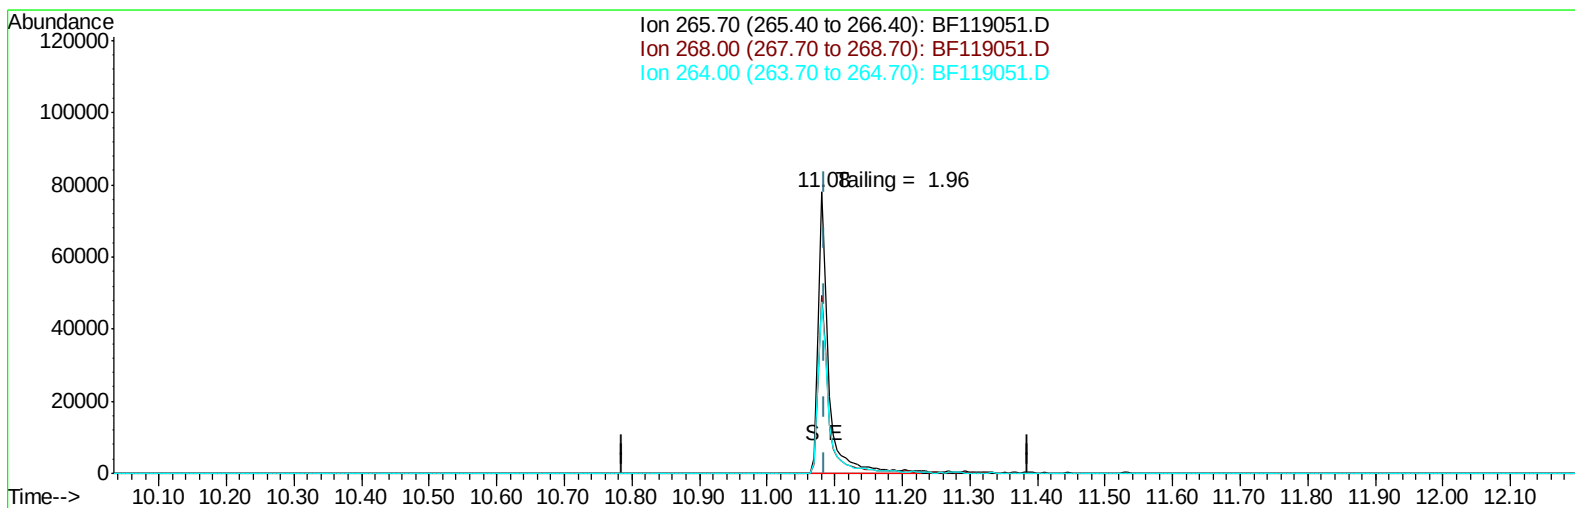

TIC: BF119051.D

(70) Pentachlorophenol (C)

11.080min (-0.006) 102440.23ng

response 85199

Ion	Exp%	Act%
265.70	100	100
268.00	64.20	63.08
264.00	61.90	60.81
0.00	0.00	0.00

