

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF022420\
 Data File : BF119015.D
 Acq On : 24 Feb 2020 11:00
 Operator : CG/JU
 Sample : PB126945TB
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB126945TB

Quant Time: Feb 25 00:35:18 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 20 17:40:17 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.76	152	221932	20.00	ng	0.00
21) Naphthalene-d8	8.03	136	835222	20.00	ng	-0.01
39) Acenaphthene-d10	9.79	164	459457	20.00	ng	0.00
64) Phenanthrene-d10	11.27	188	849181	20.00	ng	0.00
76) Chrysene-d12	13.91	240	684732	20.00	ng	0.00
87) Perylene-d12	15.34	264	694428	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.40	112	1522533	114.65	ng	0.02
7) Phenol-d6	6.40	99	1762421	109.12	ng	0.00
23) Nitrobenzene-d5	7.32	82	1403544	88.73	ng	0.00
42) 2,4,6-Tribromophenol	10.59	330	813541	135.35	ng	0.00
45) 2-Fluorobiphenyl	9.12	172	2593260	83.15	ng	0.00
79) Terphenyl-d14	12.86	244	3294485	82.84	ng	0.00
Target Compounds						
50) Dimethylphthalate	9.50	163	71514	2.035	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF022420\
Data File : BF119015.D
Acq On : 24 Feb 2020 11:00
Operator : CG/JU
Sample : PB126945TB
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB126945TB

Quant Time: Feb 25 00:35:18 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 20 17:40:17 2020
Response via : Initial Calibration

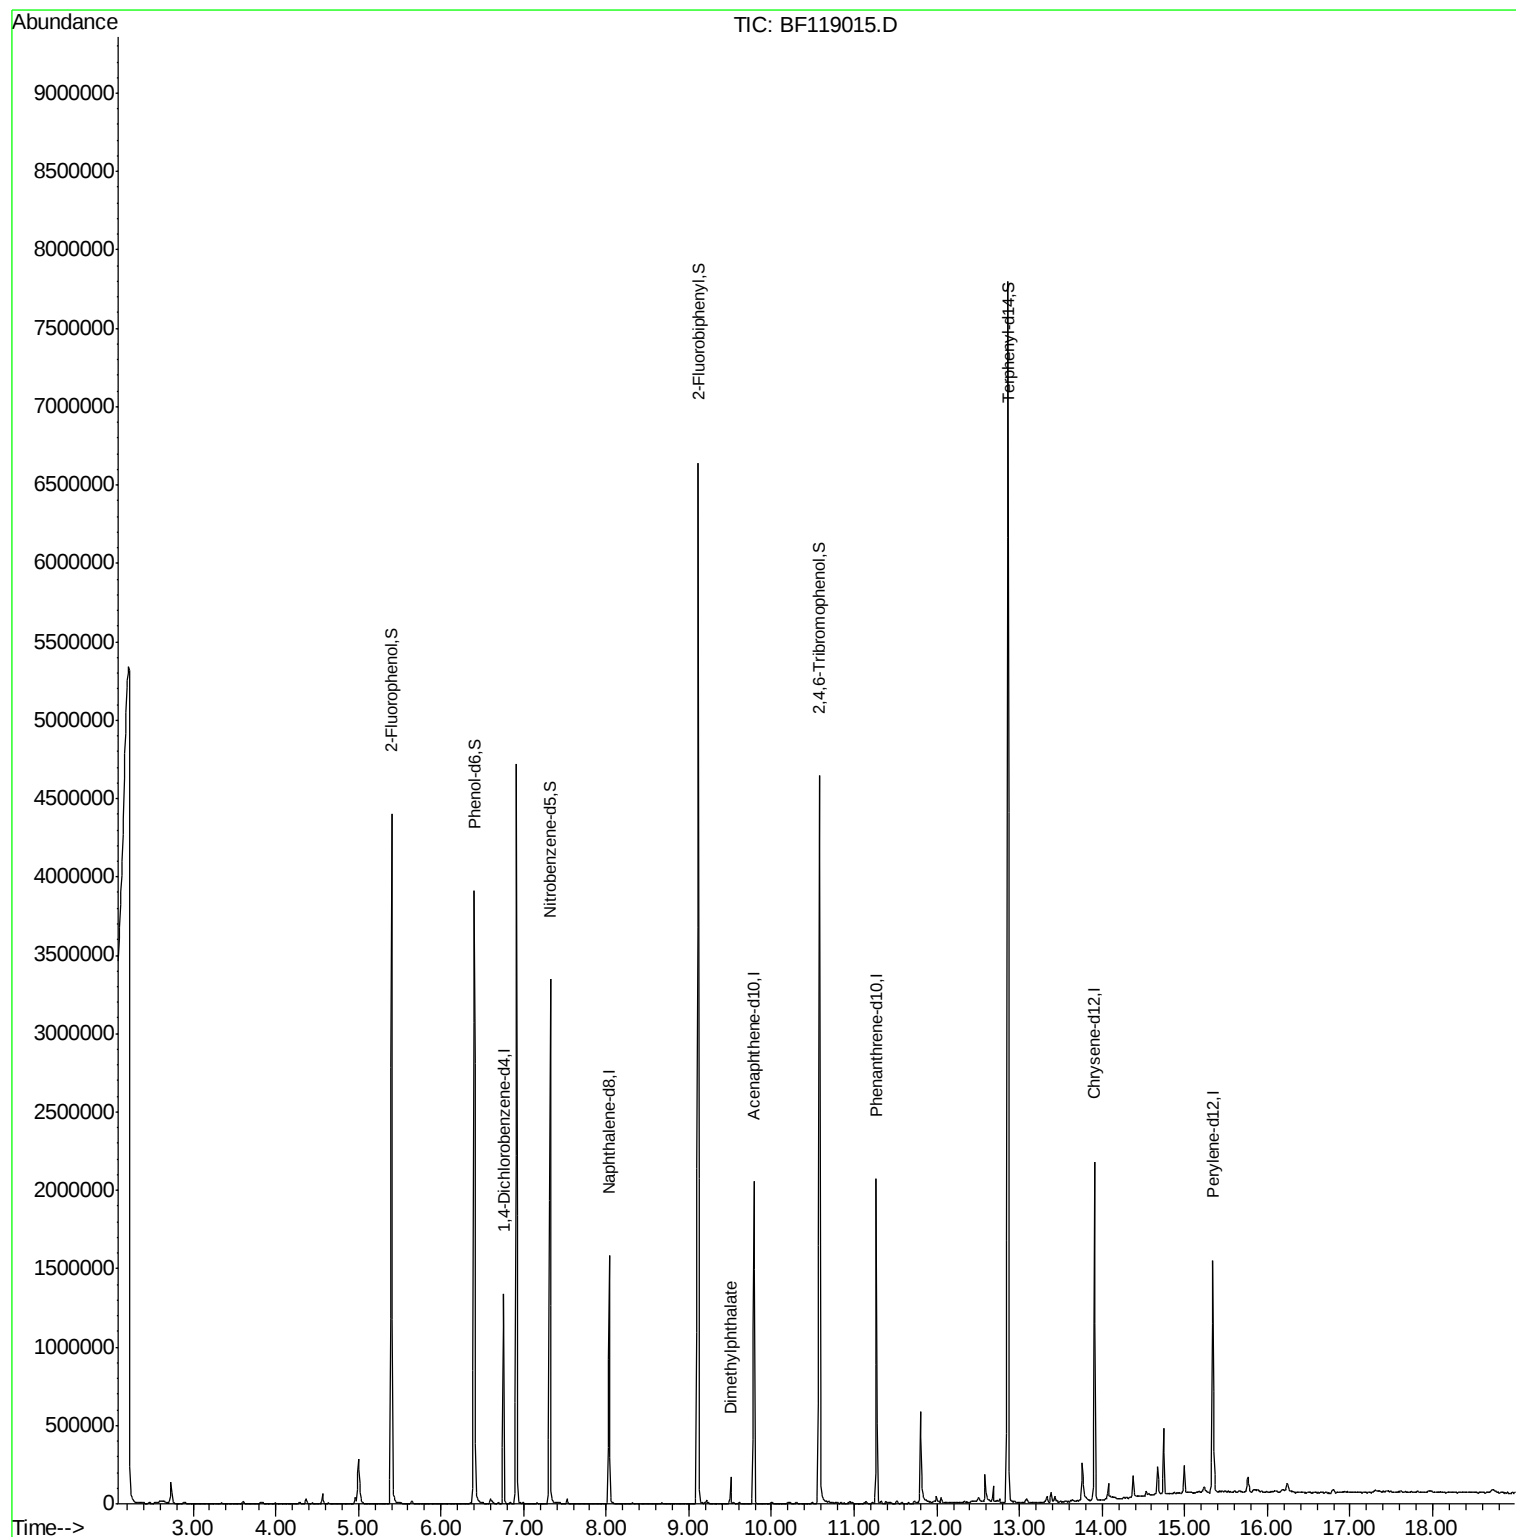

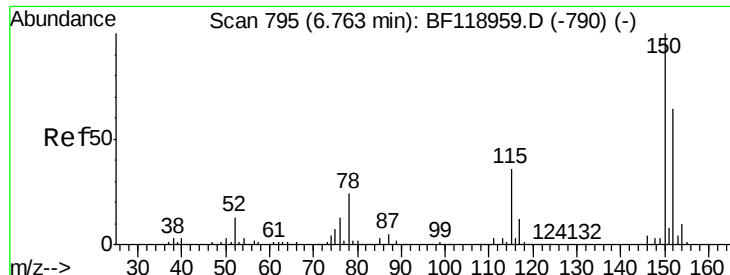


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.76 min Scan# 794
Delta R.T. -0.01 min
Lab File: BF119015.D
Acq: 24 Feb 2020 11:00

Instrument :
BNA_F
ClientSampleId :
PB126945TB

Tot Ion:152 Resp: 221932
Ion Ratio Lower Upper
152 100
150 151.6 124.3 186.5
115 57.2 44.6 67.0

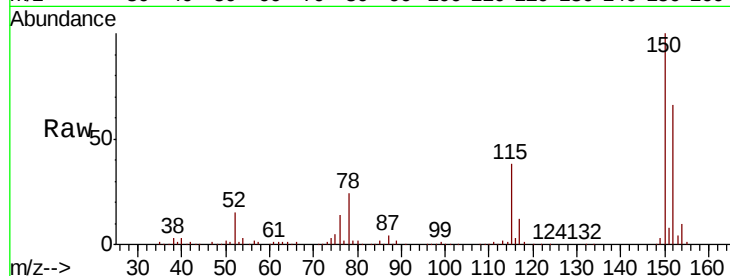


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

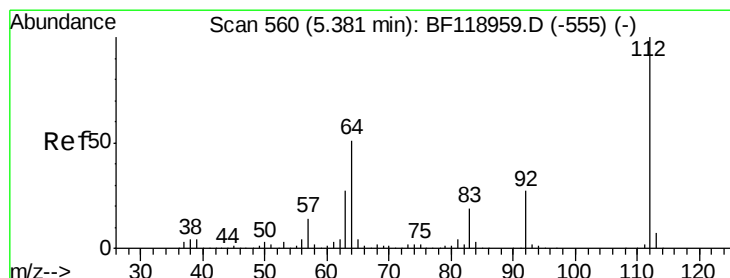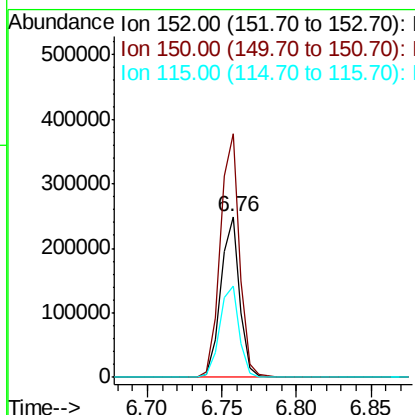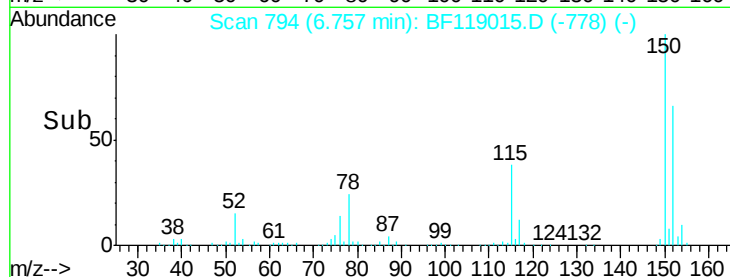



#5

2-Fluorophenol
Concen: 114.649 ng
RT: 5.40 min Scan# 564
Delta R.T. 0.02 min
Lab File: BF119015.D
Acq: 24 Feb 2020 11:00

Tgt Ion:112 Resp: 1522533
Ion Ratio Lower Upper
112 100
64 54.1 40.4 60.6
63 29.2 21.3 31.9

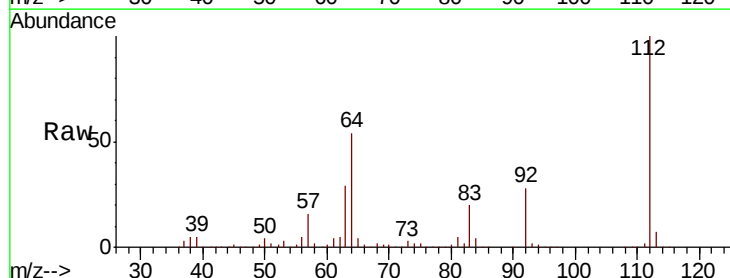

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

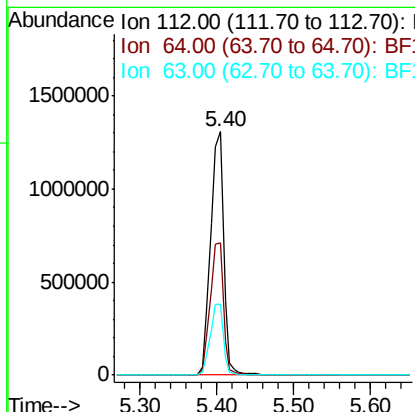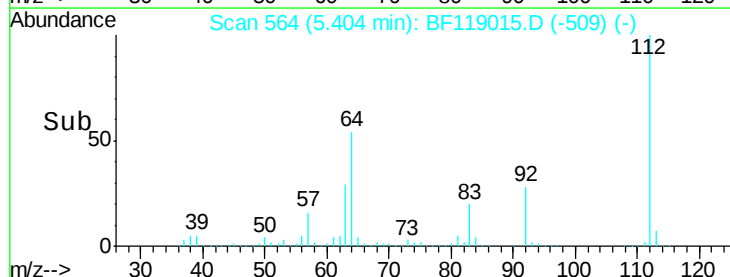



#7

Phenol-d6

Concen: 109.122 ng

RT: 6.40 min Scan# 734

Delta R.T. 0.00 min

Lab File: BF119015.D

Acq: 24 Feb 2020 11:00

Instrument :

BNA_F

ClientSampleId :

PB126945TB


Tot Ion: 99 Resp: 1762421

Ion Ratio Lower Upper



99 100

42 15.3 11.4 17.0

71 39.2 29.8 44.6

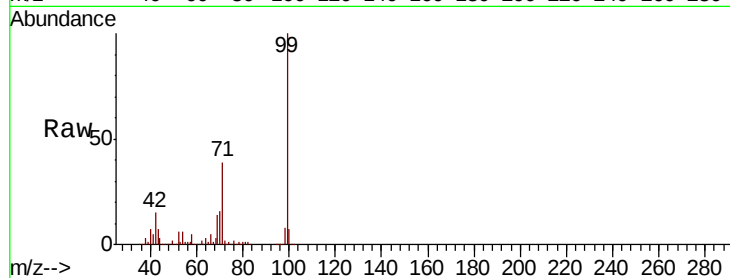

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

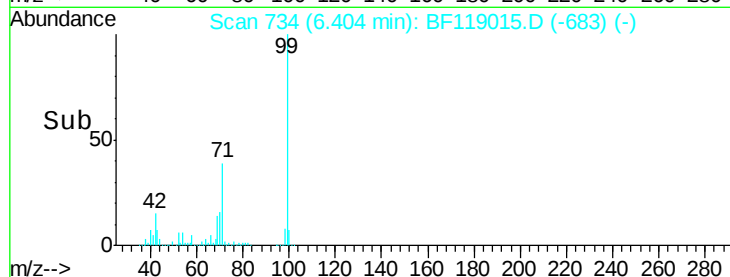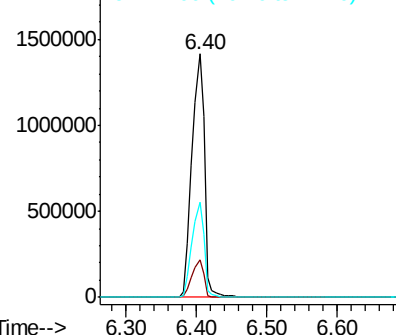

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.03 min Scan# 1011

Delta R.T. -0.01 min

Lab File: BF119015.D

Acq: 24 Feb 2020 11:00

Tgt Ion: 136 Resp: 835222


Ion Ratio Lower Upper

136 100



137 11.3 8.9 13.3

54 5.2 3.8 5.6

68 5.6 4.2 6.2

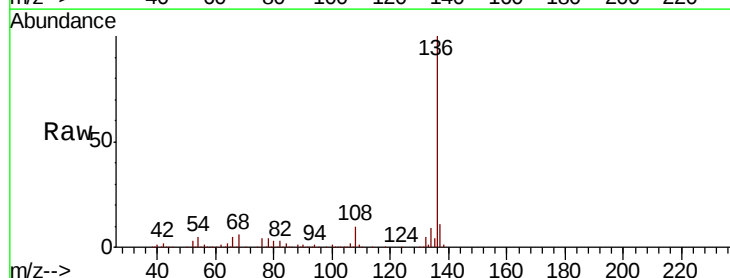

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

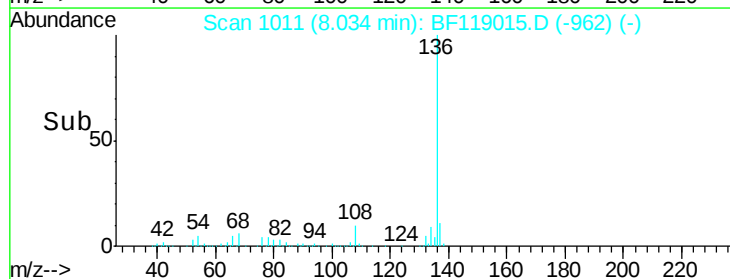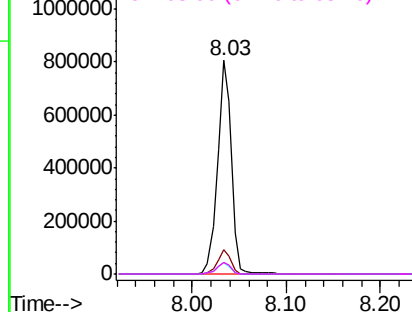







#23
Nitrobenzene-d5
Concen: 88.727 ng
RT: 7.32 min Scan# 890
Delta R.T. -0.01 min
Lab File: BF119015.D
Acq: 24 Feb 2020 11:00

Instrument :
BNA_F
ClientSampleId :
PB126945TB

Tot Ion: 82 Resp: 1403544
Ion Ratio Lower Upper
82 100
128 47.3 38.2 57.2
54 40.7 31.3 46.9

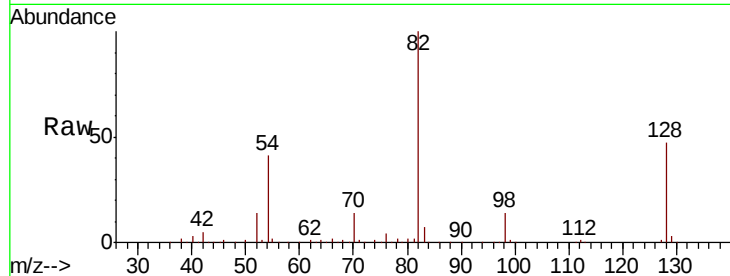


Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): BF1
Ion 54.00 (53.70 to 54.70): BF1

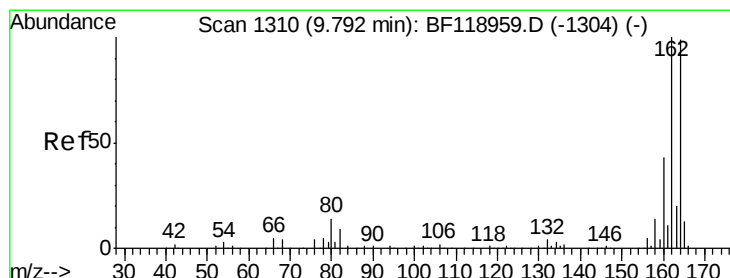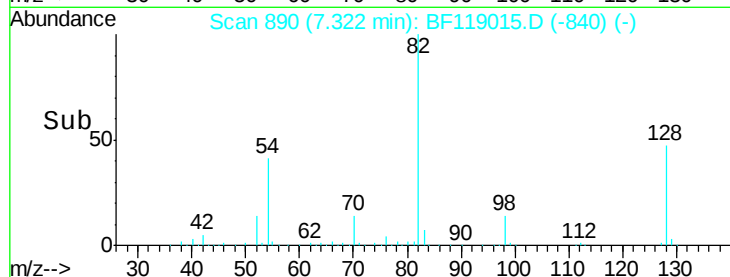
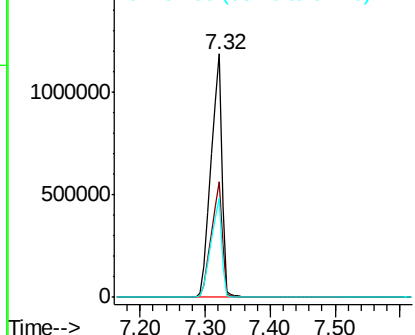


#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.79 min Scan# 1309
Delta R.T. -0.01 min
Lab File: BF119015.D
Acq: 24 Feb 2020 11:00

Tgt Ion:164 Resp: 459457
Ion Ratio Lower Upper
164 100
162 103.4 81.2 121.8
160 45.6 35.2 52.8

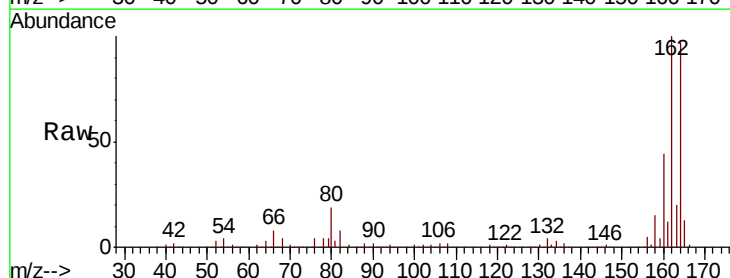

Abundance Ion 164.00 (163.70 to 164.70): BF1
Ion 162.00 (161.70 to 162.70): BF1
Ion 160.00 (159.70 to 160.70): BF1

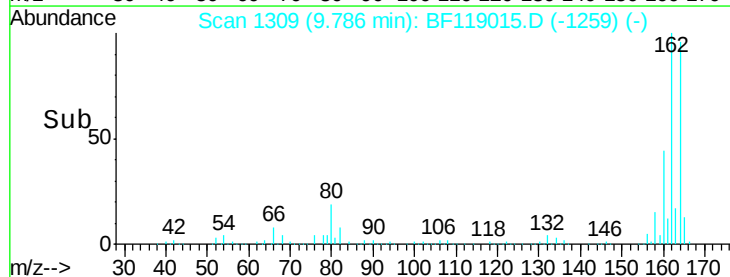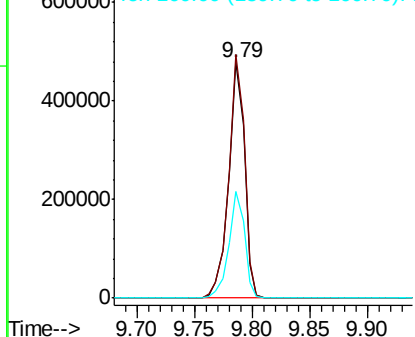







#42
 2,4,6-Tribromophenol
 Concen: 135.354 ng
 RT: 10.59 min Scan# 1445
 Delta R.T. 0.01 min
 Lab File: BF119015.D
 Acq: 24 Feb 2020 11:00

Instrument :
 BNA_F
 ClientSampleId :
 PB126945TB

Tot Ion:330 Resp: 813541
 Ion Ratio Lower Upper
 330 100
 332 97.7 77.1 115.7
 141 28.5 23.0 34.6

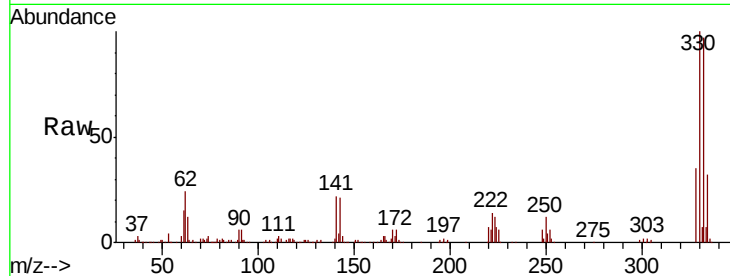


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

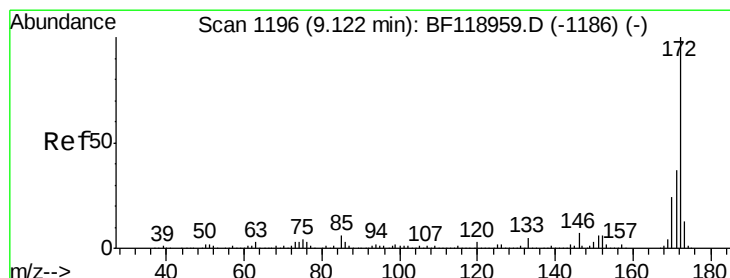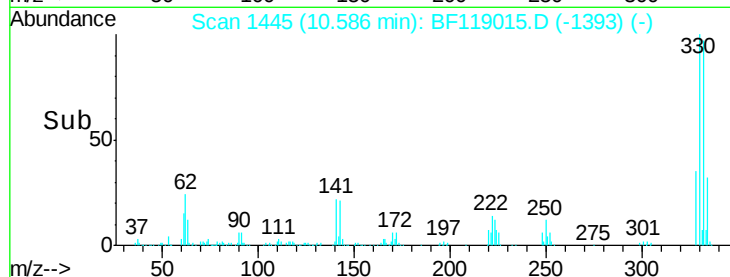
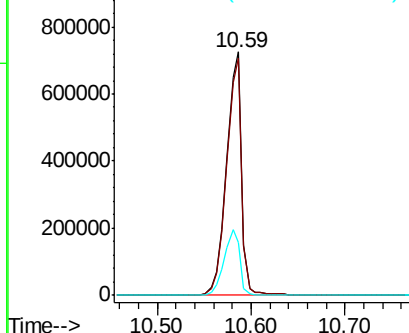



#45
 2-Fluorobiphenyl
 Concen: 83.149 ng
 RT: 9.12 min Scan# 1195
 Delta R.T. -0.01 min
 Lab File: BF119015.D
 Acq: 24 Feb 2020 11:00

Tgt Ion:172 Resp: 2593260
 Ion Ratio Lower Upper
 172 100
 171 38.1 29.4 44.2
 170 25.6 19.6 29.4

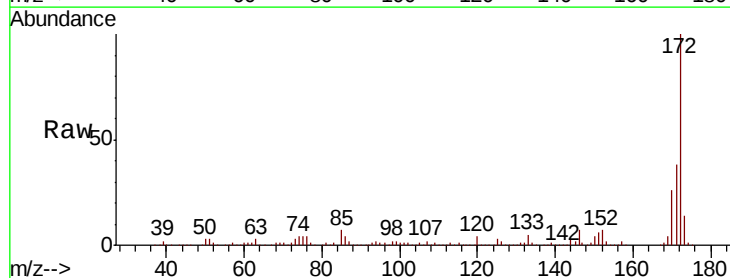

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

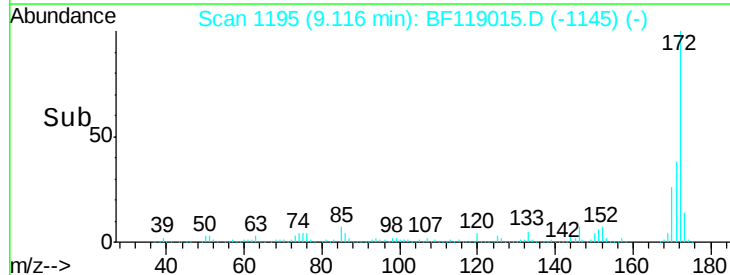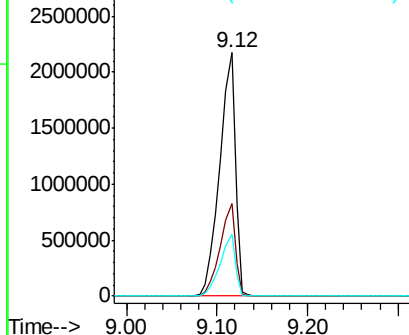

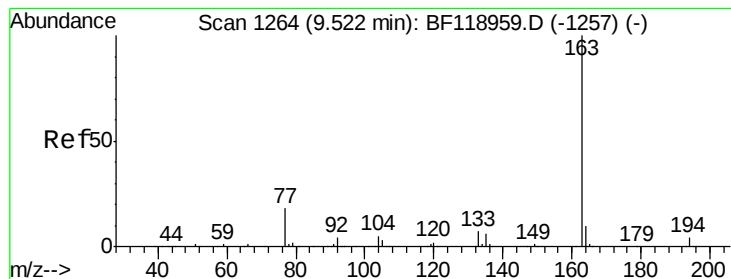

#50

Dimethylphthalate

Concen: 2.035 ng

RT: 9.50 min Scan# 1261

Delta R.T. -0.02 min

Lab File: BF119015.D

Acq: 24 Feb 2020 11:00

Instrument :

BNA_F

ClientSampleId :

PB126945TB


Tot Ion:163 Resp: 71514

Ion Ratio Lower Upper




163 100

194 4.6 3.4 5.2

164 9.7 8.2 12.2

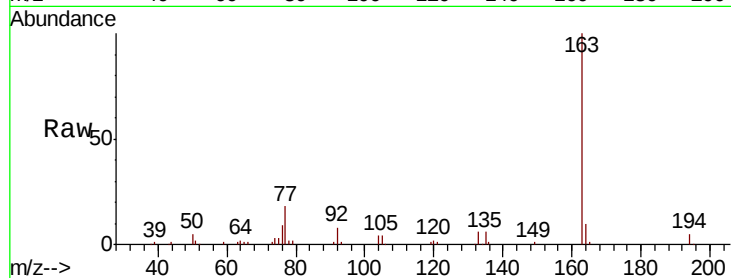

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

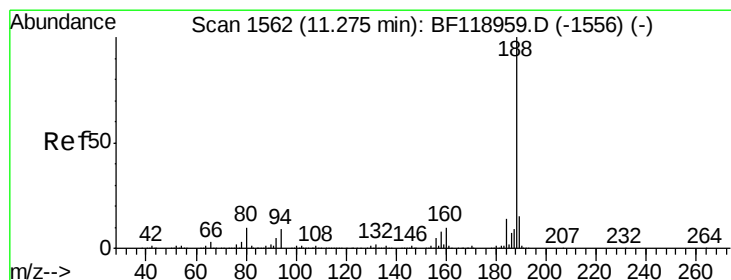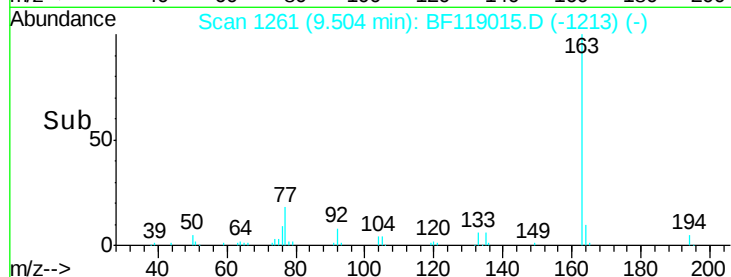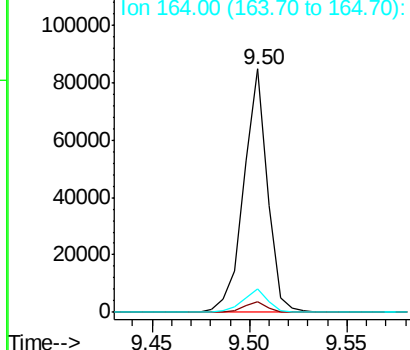

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.27 min Scan# 1561

Delta R.T. -0.01 min

Lab File: BF119015.D

Acq: 24 Feb 2020 11:00


Tgt Ion:188 Resp: 849181

Ion Ratio Lower Upper



188 100


94 9.4 7.0 10.6

80 10.6 7.9 11.9

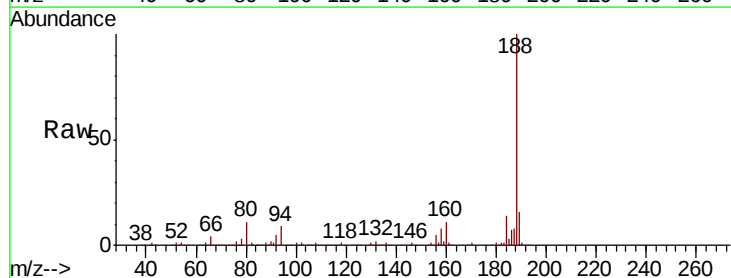

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1



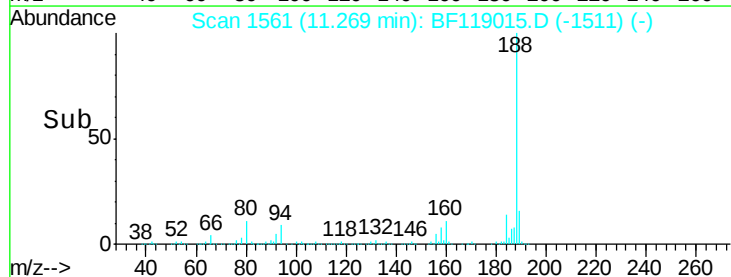
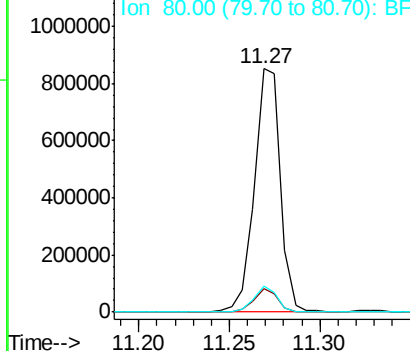


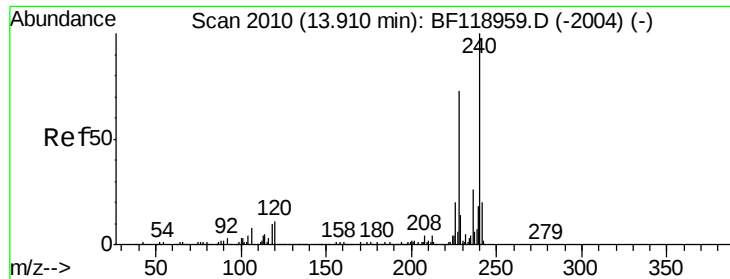

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.91 min Scan# 2010
Delta R.T. 0.00 min
Lab File: BF119015.D
Acq: 24 Feb 2020 11:00




Instrument :
BNA_F
ClientSampleId :
PB126945TB




Tot Ion:240 Resp: 684732
Ion Ratio Lower Upper
240 100
120 10.2 8.9 13.3
236 26.4 20.6 30.8

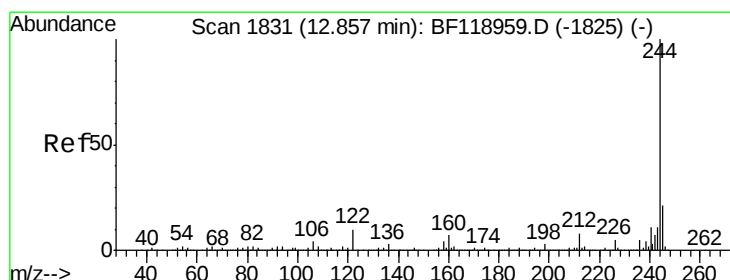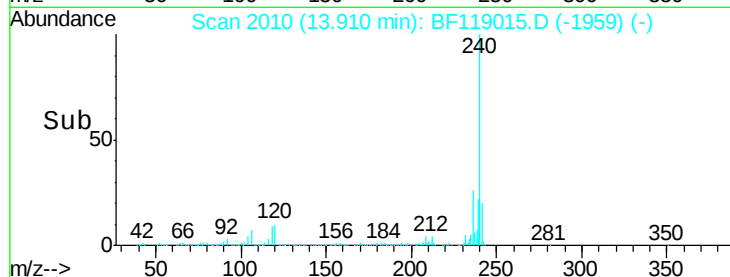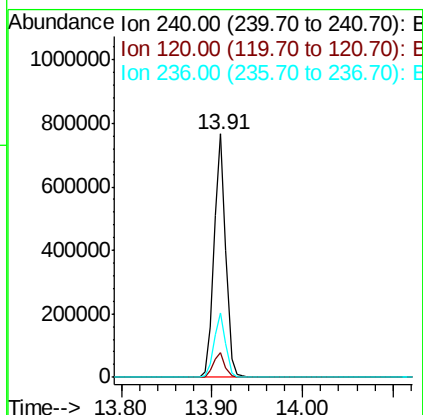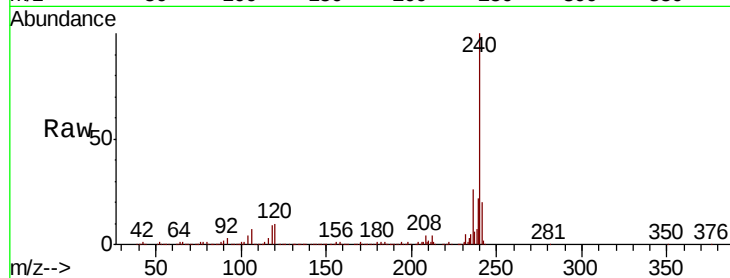

#79
Terphenyl-d14
Concen: 82.836 ng
RT: 12.86 min Scan# 1832
Delta R.T. 0.01 min
Lab File: BF119015.D
Acq: 24 Feb 2020 11:00

Tgt Ion:244 Resp: 3294485
Ion Ratio Lower Upper
244 100
212 8.1 6.3 9.5
122 10.1 8.4 12.6

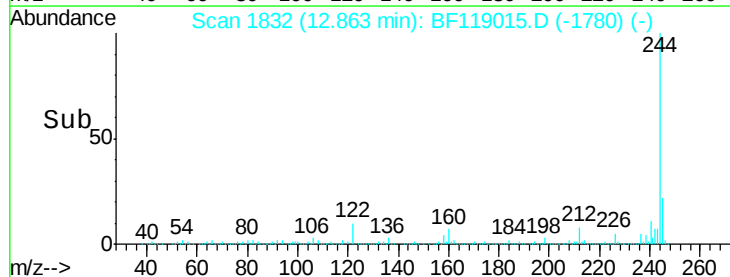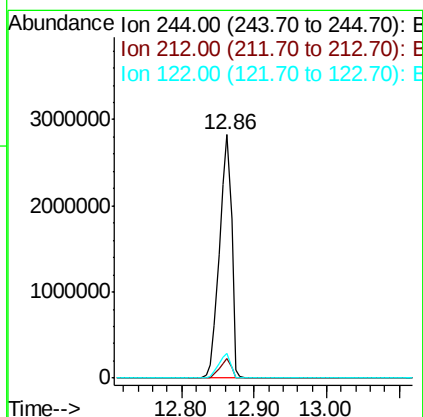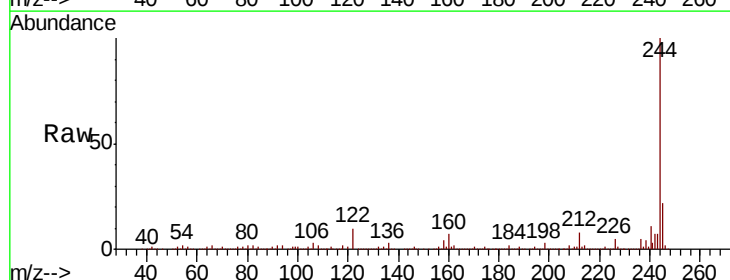

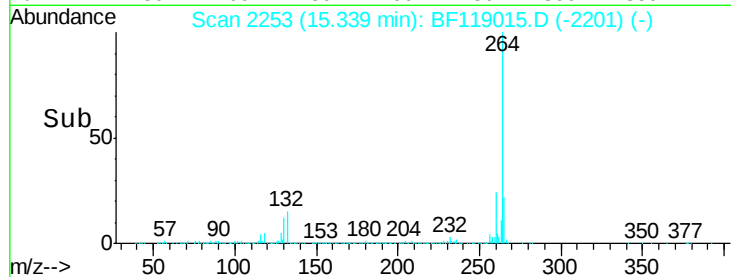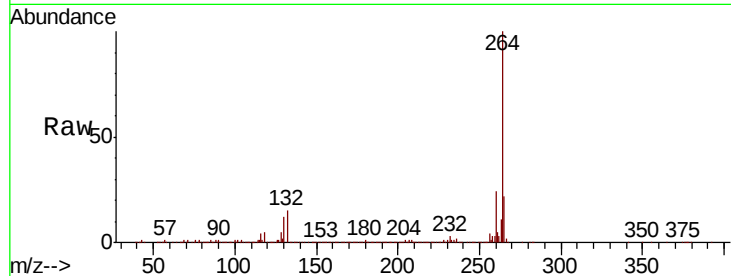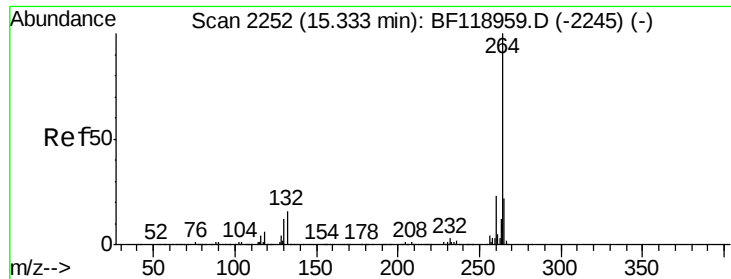

#87
Pervlene-d12
Concen: 20.000 ng
RT: 15.34 min Scan# 2253
Delta R.T. 0.01 min
Lab File: BF119015.D
Acq: 24 Feb 2020 11:00

Instrument :
BNA_F
ClientSampleId :
PB126945TB

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.9	18.6	28.0
265	21.7	17.3	25.9

