

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF022420\
 Data File : BF119042.D
 Acq On : 25 Feb 2020 1:25
 Operator : CG/JU
 Sample : L1635-10
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DUNR-TS007-01

Quant Time: Feb 25 03:37:09 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 20 17:40:17 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.75	152	182820	20.00	ng	-0.01
21) Naphthalene-d8	8.03	136	711539	20.00	ng	-0.01
39) Acenaphthene-d10	9.79	164	388893	20.00	ng	0.00
64) Phenanthrene-d10	11.27	188	684773	20.00	ng	0.00
76) Chrysene-d12	13.90	240	407745	20.00	ng	0.00
87) Perylene-d12	15.33	264	389184	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.39	112	1004418	91.81	ng	0.00
7) Phenol-d6	6.40	99	1220999	91.77	ng	0.00
23) Nitrobenzene-d5	7.32	82	811550	60.22	ng	-0.01
42) 2,4,6-Tribromophenol	10.57	330	446769	87.82	ng	0.00
45) 2-Fluorobiphenyl	9.11	172	1608876	60.95	ng	-0.01
79) Terphenyl-d14	12.85	244	1636121	69.08	ng	0.00
Target Compounds						
50) Dimethylphthalate	9.50	163	124705	4.193	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF022420\
Data File : BF119042.D
Acq On : 25 Feb 2020 1:25
Operator : CG/JU
Sample : L1635-10
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DUNR-TS007-01

Quant Time: Feb 25 03:37:09 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 20 17:40:17 2020
Response via : Initial Calibration

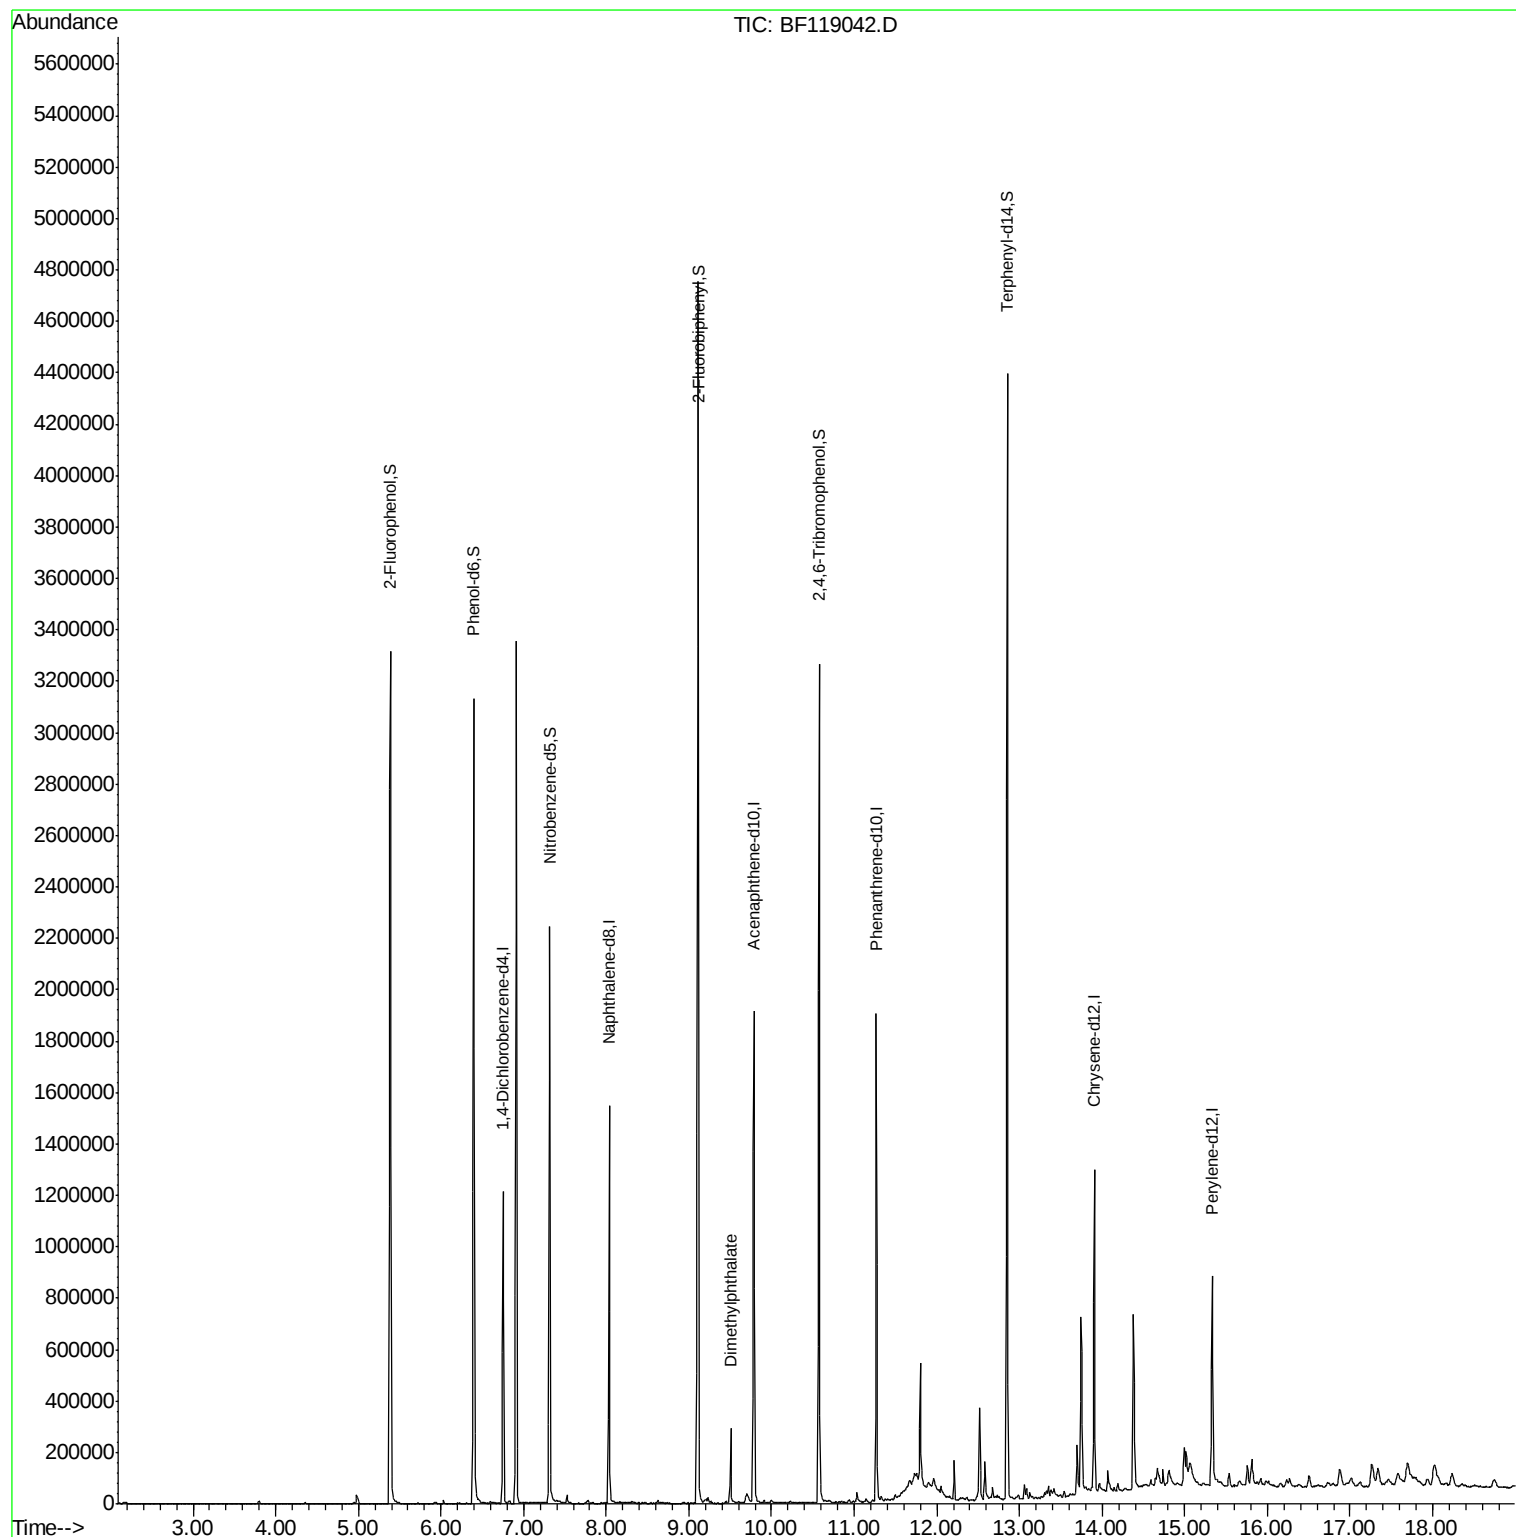

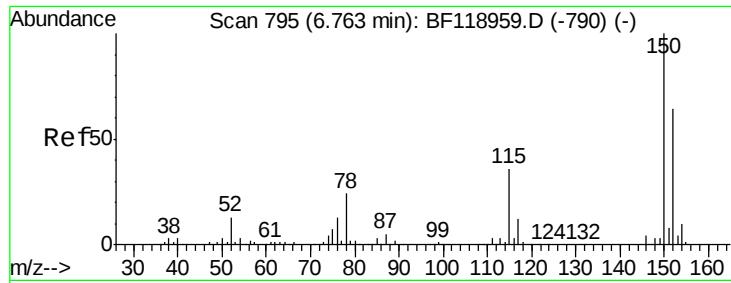


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.75 min Scan# 793
Delta R.T. -0.01 min
Lab File: BF119042.D
Acq: 25 Feb 2020 1:25

Instrument :
BNA_F
ClientSampleId :
DUNR-TS007-01

Tot Ion:152 Resp: 182820
Ion Ratio Lower Upper
152 100
150 156.3 124.3 186.5
115 60.5 44.6 67.0

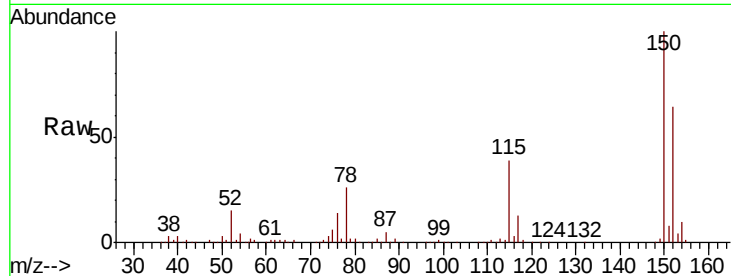


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

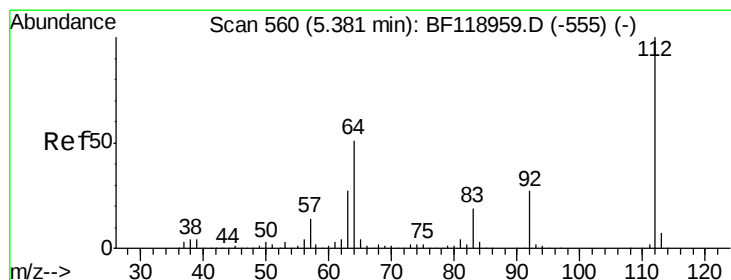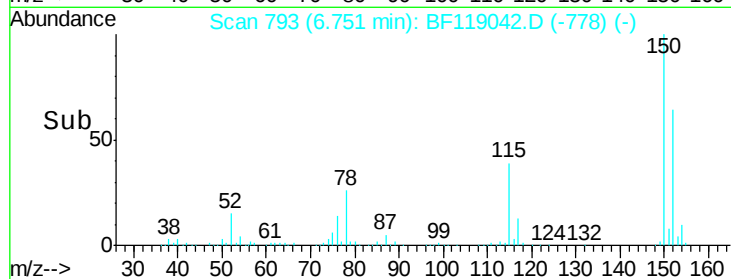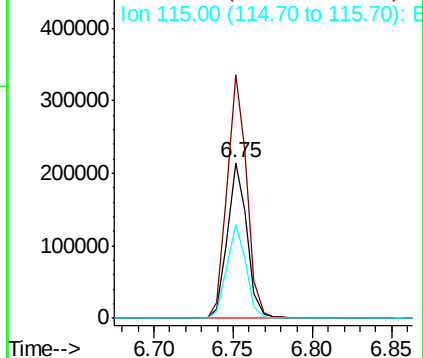



#5

2-Fluorophenol
Concen: 91.815 ng
RT: 5.39 min Scan# 561
Delta R.T. 0.01 min
Lab File: BF119042.D
Acq: 25 Feb 2020 1:25

Tgt Ion:112 Resp: 1004418
Ion Ratio Lower Upper
112 100
64 53.0 40.4 60.6
63 28.8 21.3 31.9

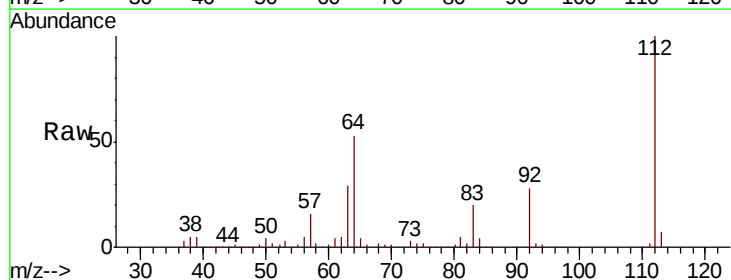

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

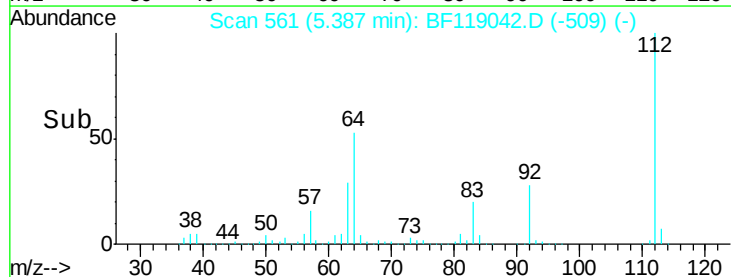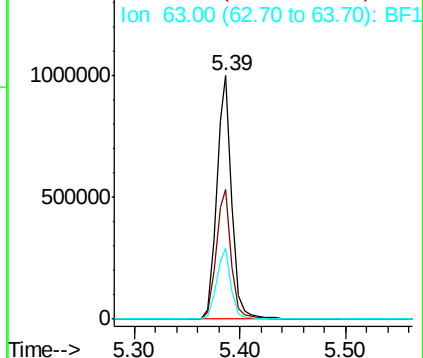



#7

Phenol-d6

Concen: 91.773 ng

RT: 6.40 min Scan# 733

Delta R.T. -0.01 min

Lab File: BF119042.D

Acq: 25 Feb 2020 1:25

Instrument :

BNA_F

ClientSampleId :

DUNR-TS007-01


Tot Ion: 99 Resp: 1220999

Ion Ratio Lower Upper



99 100

42 15.3 11.4 17.0

71 38.4 29.8 44.6

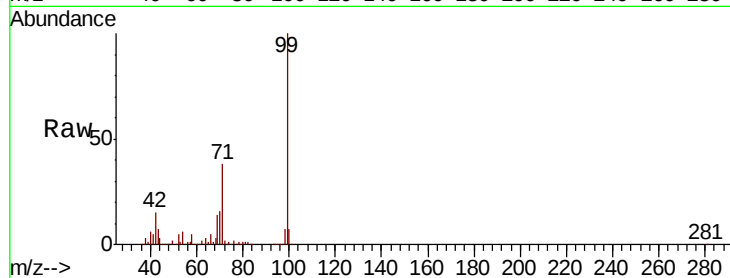

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

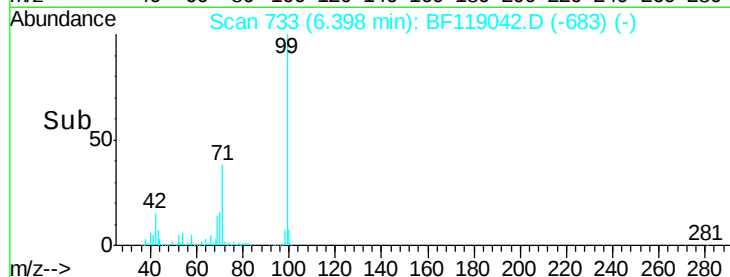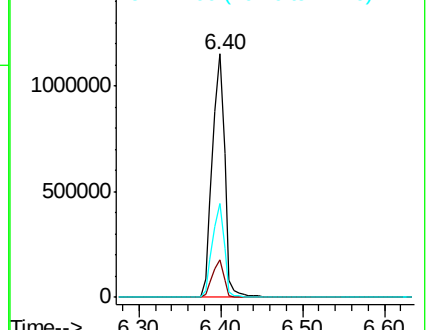

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.03 min Scan# 1011

Delta R.T. -0.01 min

Lab File: BF119042.D

Acq: 25 Feb 2020 1:25

Tgt Ion: 136 Resp: 711539


Ion Ratio Lower Upper

136 100



137 11.1 8.9 13.3

54 4.9 3.8 5.6

68 5.2 4.2 6.2

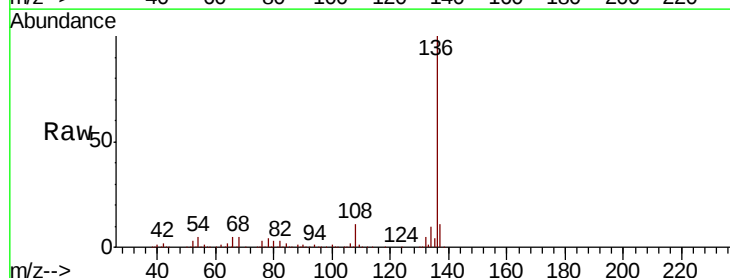

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1



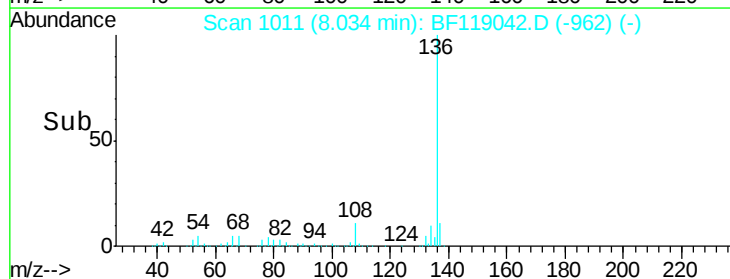
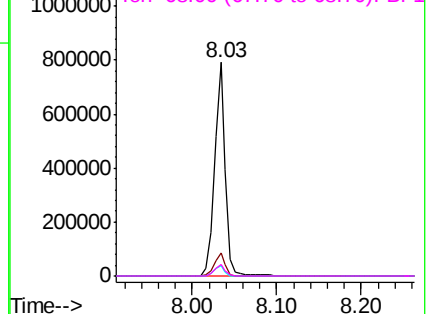




#23
 Nitrobenzene-d5
 Concen: 60.221 ng
 RT: 7.32 min Scan# 889
 Delta R.T. -0.01 min
 Lab File: BF119042.D
 Acq: 25 Feb 2020 1:25




Instrument :
 BNA_F
 ClientSampleId :
 DUNR-TS007-01

Tot Ion	82	Resp	811550
Ion Ratio	Lower	Upper	
82	100		
128	47.4	38.2	57.2
54	39.6	31.3	46.9

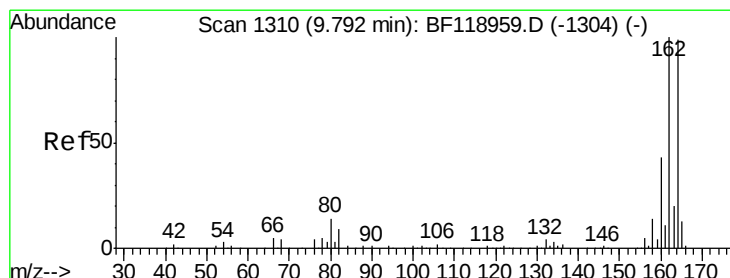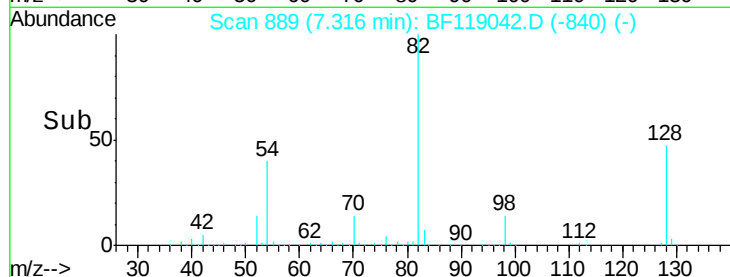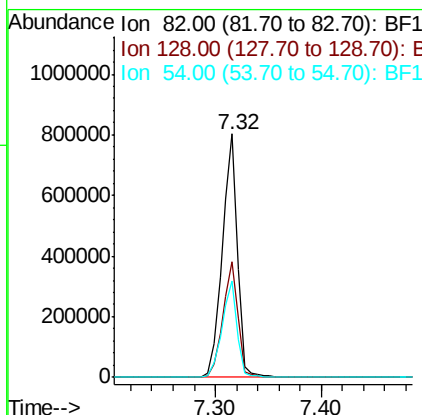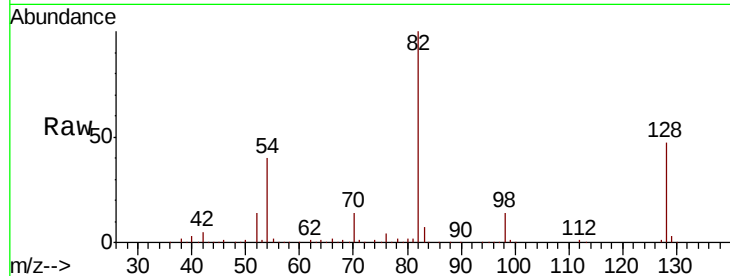

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.79 min Scan# 1309
 Delta R.T. -0.01 min
 Lab File: BF119042.D
 Acq: 25 Feb 2020 1:25

Tgt Ion	164	Resp	388893
Ion Ratio	Lower	Upper	
164	100		
162	102.4	81.2	121.8
160	43.7	35.2	52.8

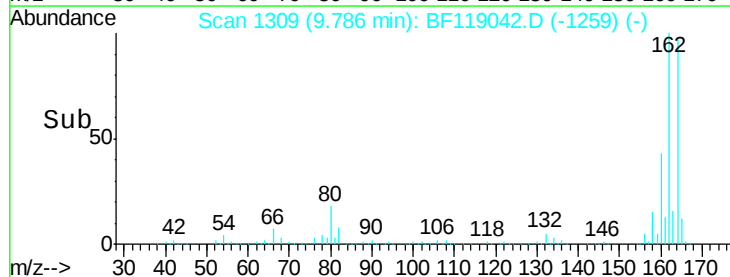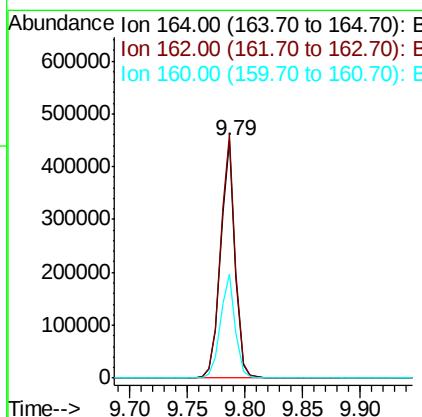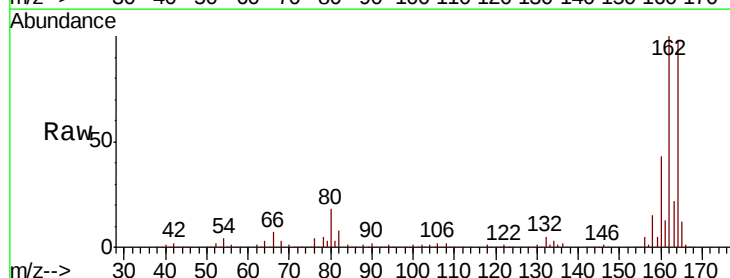







#42
 2,4,6-Tribromophenol
 Concen: 87.819 ng
 RT: 10.57 min Scan# 1443
 Delta R.T. -0.01 min
 Lab File: BF119042.D
 Acq: 25 Feb 2020 1:25

Instrument :
 BNA_F
 ClientSampleId :
 DUNR-TS007-01

Tot Ion:330 Resp: 446769
 Ion Ratio Lower Upper
 330 100
 332 96.1 77.1 115.7
 141 28.2 23.0 34.6

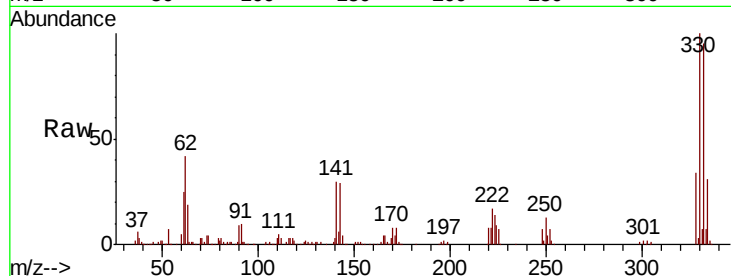


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

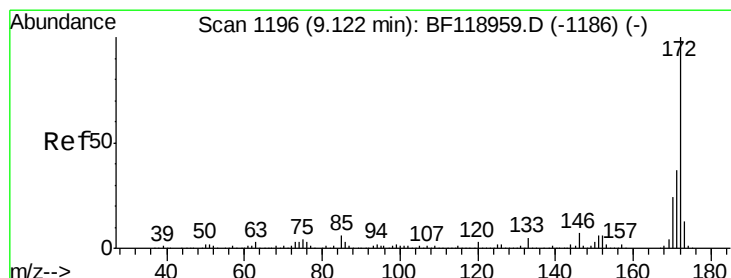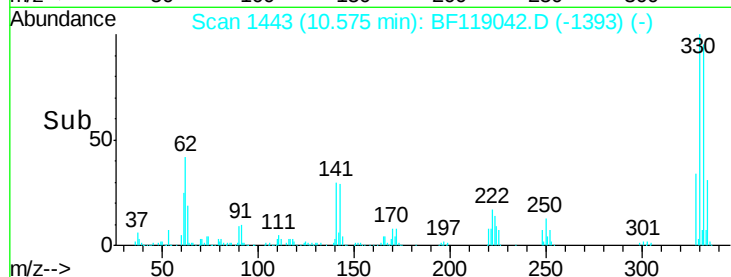
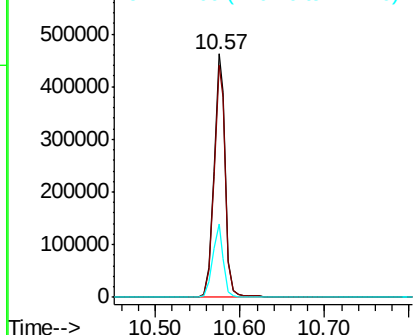



#45
 2-Fluorobiphenyl
 Concen: 60.946 ng
 RT: 9.11 min Scan# 1194
 Delta R.T. -0.01 min
 Lab File: BF119042.D
 Acq: 25 Feb 2020 1:25

Tgt Ion:172 Resp: 1608876
 Ion Ratio Lower Upper
 172 100
 171 36.7 29.4 44.2
 170 23.8 19.6 29.4

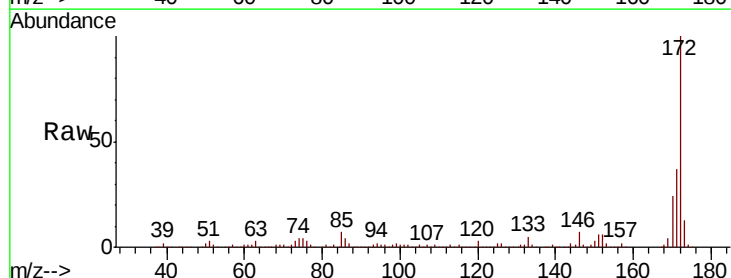

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

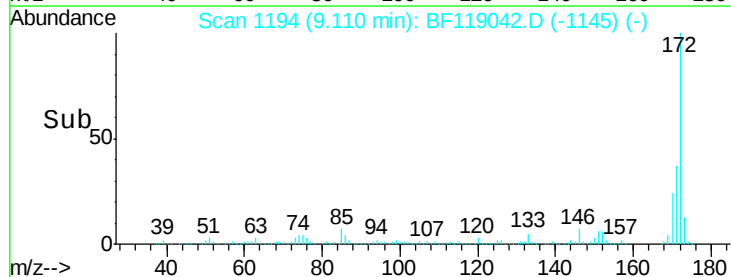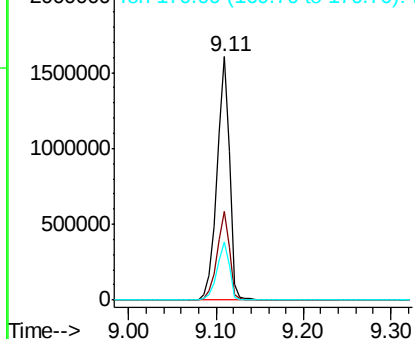

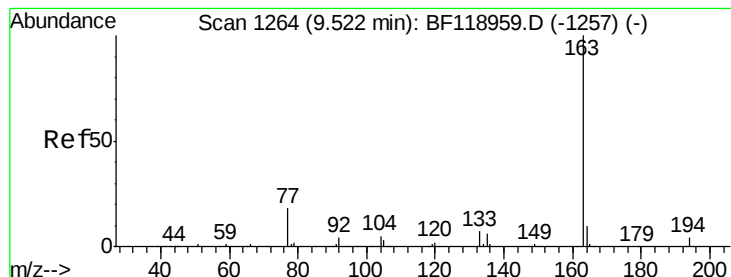

#50

Dimethylphthalate

Concen: 4.193 ng

RT: 9.50 min Scan# 1261

Delta R.T. -0.02 min

Lab File: BF119042.D

Acq: 25 Feb 2020 1:25

Instrument :

BNA_F

ClientSampleId :

DUNR-TS007-01


Tot Ion:163 Resp: 124705

Ion Ratio Lower Upper




163 100

194 4.3 3.4 5.2

164 9.8 8.2 12.2

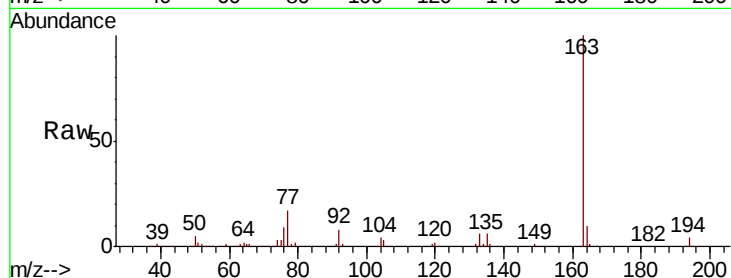

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

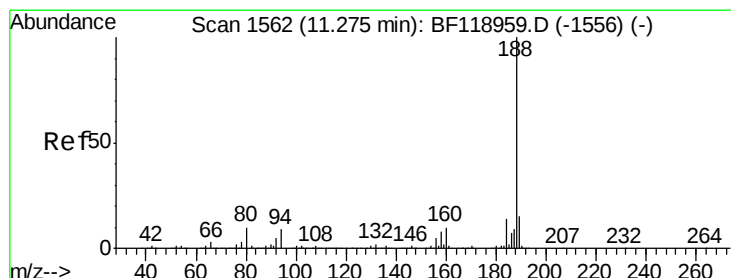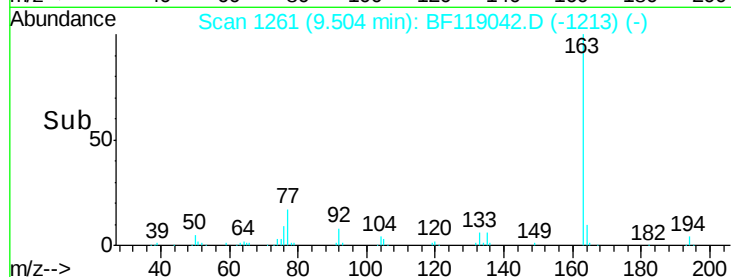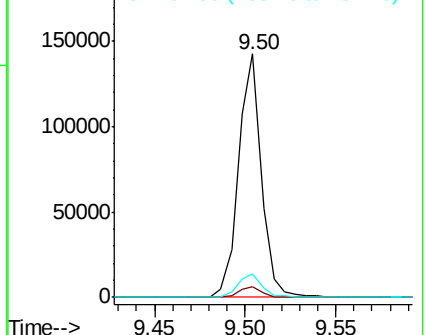

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.27 min Scan# 1561

Delta R.T. -0.01 min

Lab File: BF119042.D

Acq: 25 Feb 2020 1:25


Tgt Ion:188 Resp: 684773

Ion Ratio Lower Upper



188 100


94 8.2 7.0 10.6

80 9.1 7.9 11.9

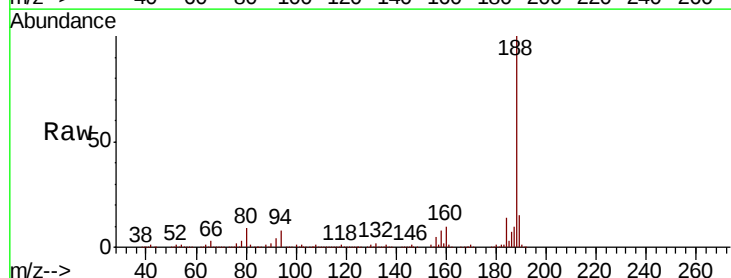

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1


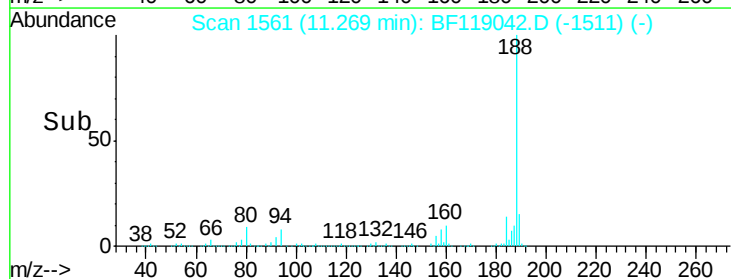
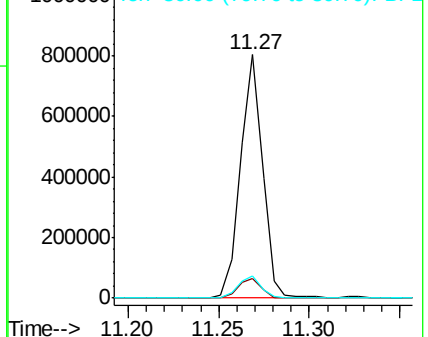


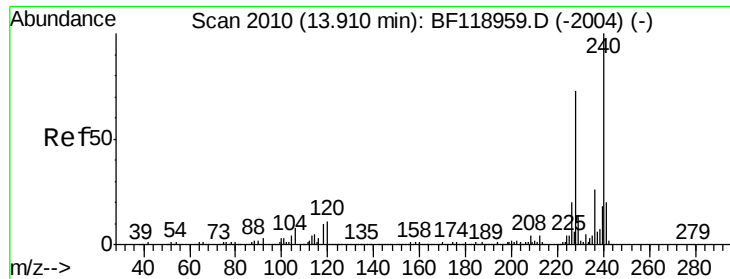

#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 13.90 min Scan# 2009
 Delta R.T. -0.01 min
 Lab File: BF119042.D
 Acq: 25 Feb 2020 1:25




Instrument :
 BNA_F
 ClientSampleId :
 DUNR-TS007-01


Tot Ion:240 Resp: 407745
 Ion Ratio Lower Upper
 240 100
 120 9.6 8.9 13.3
 236 26.5 20.6 30.8

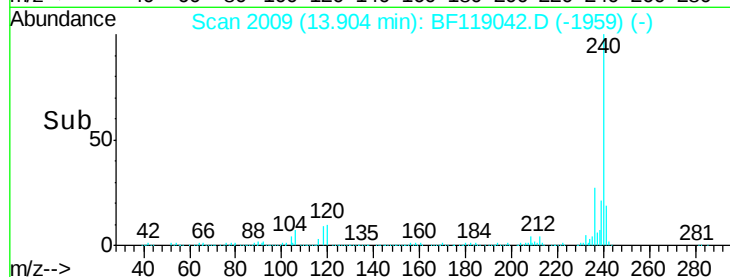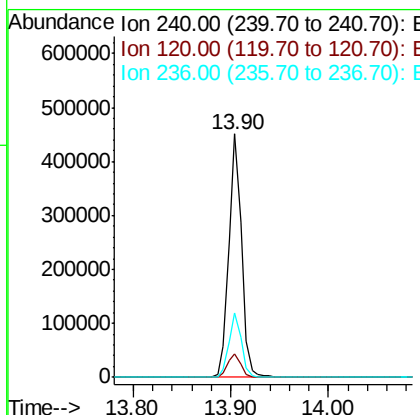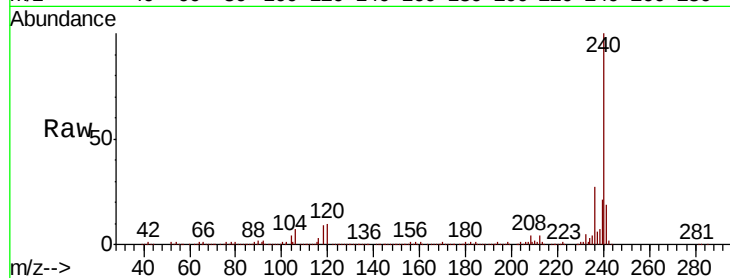

#79
 Terphenyl-d14
 Concen: 69.084 ng
 RT: 12.85 min Scan# 1830
 Delta R.T. -0.01 min
 Lab File: BF119042.D
 Acq: 25 Feb 2020 1:25

Tgt Ion:244 Resp: 1636121
 Ion Ratio Lower Upper
 244 100
 212 7.3 6.3 9.5
 122 10.6 8.4 12.6

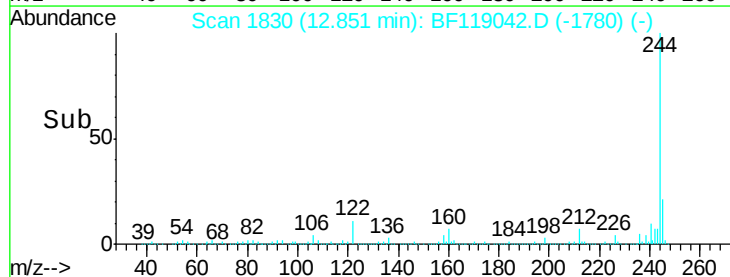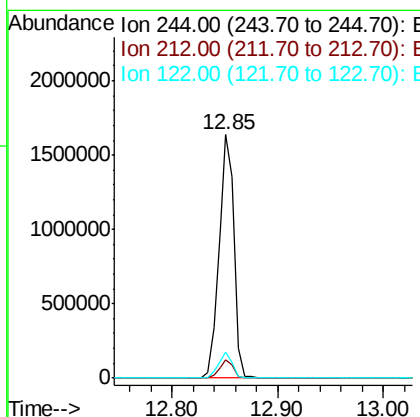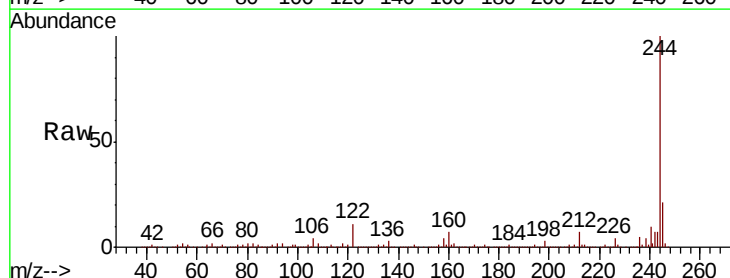

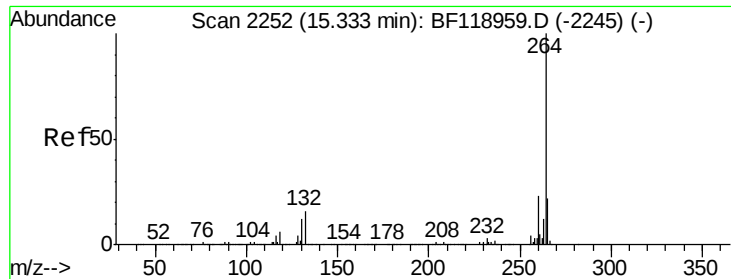

#87
Pervlene-d12
Concen: 20.000 ng
RT: 15.33 min Scan# 2252
Delta R.T. 0.00 min
Lab File: BF119042.D
Acq: 25 Feb 2020 1:25

Instrument :
BNA_F
ClientSampleId :
DUNR-TS007-01

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.2	18.6	28.0
265	21.2	17.3	25.9

