

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF022420\
 Data File : BF119023.D
 Acq On : 24 Feb 2020 15:09
 Operator : CG/JU
 Sample : PB126979BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB126979BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.387	557	561	584	rBV	2879931	2888663	59.31%	9.809%
2	6.398	728	733	748	rBV	2885482	2820542	57.91%	9.577%
3	6.751	790	793	801	rBV	915994	826360	16.97%	2.806%
4	6.910	816	820	824	rBV	2987727	2610286	53.60%	8.863%
5	7.316	884	889	892	rBV	1944642	1909833	39.21%	6.485%
6	8.034	1007	1011	1024	rBV	1182894	1115550	22.91%	3.788%
7	9.110	1189	1194	1197	rBV	4415305	4193484	86.10%	14.239%
8	9.786	1304	1309	1323	rBB	1626035	1445694	29.68%	4.909%
9	10.575	1439	1443	1462	rBV	2689083	2733394	56.12%	9.281%
10	11.269	1557	1561	1565	rBV	1714538	1539095	31.60%	5.226%
11	12.857	1826	1831	1834	rBV	4932545	4870293	100.00%	16.538%
12	13.904	2005	2009	2020	rVB	1271861	1218071	25.01%	4.136%
13	14.668	2136	2139	2143	rBV	55814	62036	1.27%	0.211%
14	14.992	2190	2194	2200	rBV	67071	77136	1.58%	0.262%
15	15.333	2247	2252	2261	rBV	759960	1018396	20.91%	3.458%
16	15.763	2321	2325	2331	rVB	45805	67043	1.38%	0.228%
17	16.239	2401	2406	2413	rVB2	29764	54048	1.11%	0.184%


Sum of corrected areas: 29449924

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF022420\
Data File : BF119023.D
Acq On : 24 Feb 2020 15:09
Operator : CG/JU
Sample : PB126979BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB126979BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

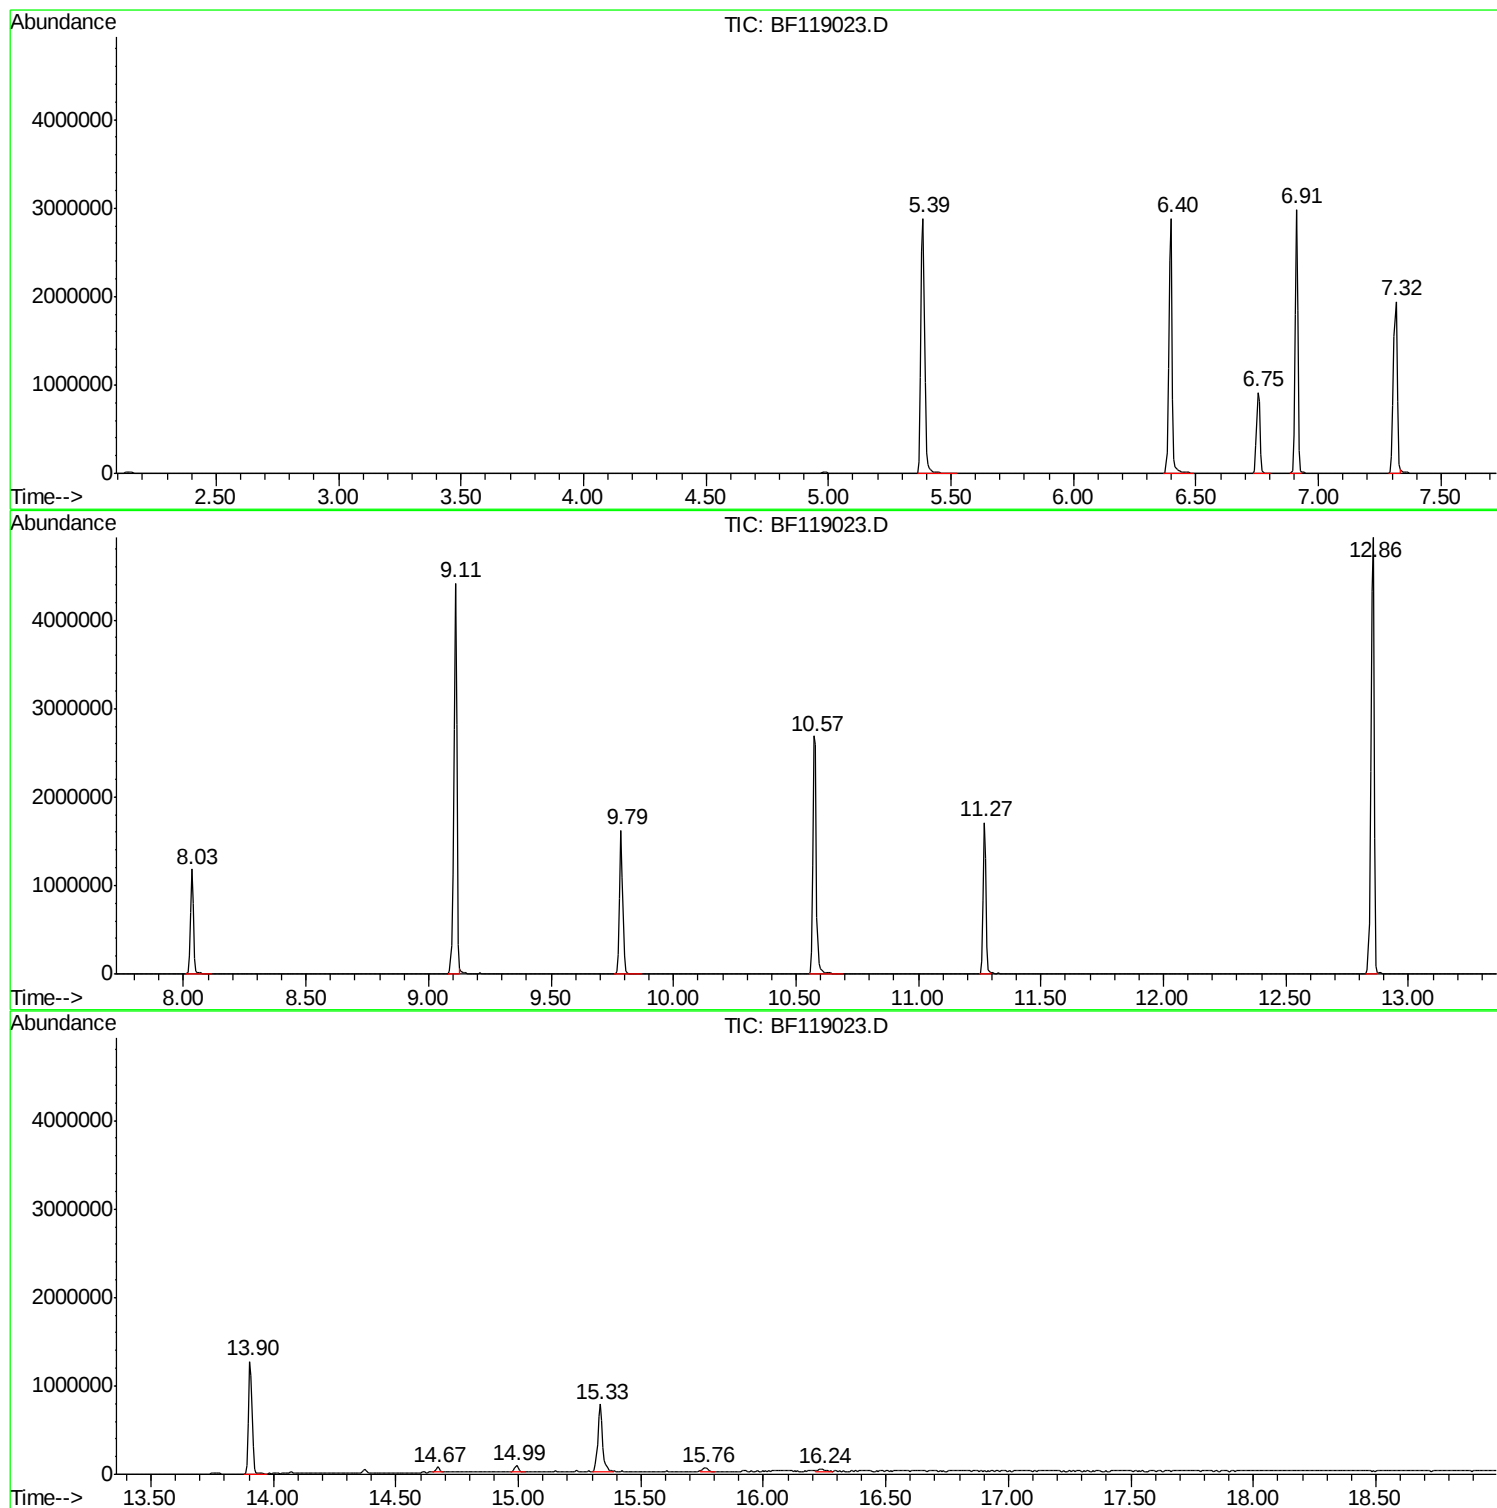

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF022420\
Data_File : BF119023.D
Acq_On : 24 Feb 2020 15:099
Operator : CG/JUU
Sample : PB126979BLL
Misc :
ALS_Vial : 11 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
PB126979BL

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022020.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
