

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF022420\
 Data File : BF119025.D
 Acq On : 24 Feb 2020 16:08
 Operator : CG/JU
 Sample : PB127021BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB127021BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.386	556	561	582	rBV	3404736	3603395	60.12%	10.345%
2	6.398	728	733	736	rBV	3429772	3454141	57.63%	9.917%
3	6.751	790	793	802	rBV	942078	843301	14.07%	2.421%
4	6.910	816	820	824	rBV	3458403	3215414	53.65%	9.231%
5	7.316	884	889	892	rBV	2390450	2380371	39.72%	6.834%
6	8.033	1007	1011	1026	rBV	1243909	1142351	19.06%	3.280%
7	9.110	1189	1194	1198	rBV	4967024	5193204	86.65%	14.909%
8	9.786	1304	1309	1313	rBV	1658510	1450699	24.20%	4.165%
9	10.580	1439	1444	1447	rBV	3537752	3401037	56.75%	9.764%
10	11.268	1557	1561	1569	rBV	1834402	1556037	25.96%	4.467%
11	12.857	1826	1831	1834	rBV	6046634	5993428	100.00%	17.207%
12	13.904	2005	2009	2017	rBV	1350887	1220657	20.37%	3.504%
13	14.674	2136	2140	2143	rBV	58279	60512	1.01%	0.174%
14	14.992	2190	2194	2199	rVB	76335	78632	1.31%	0.226%
15	15.333	2247	2252	2262	rBV	794801	1060389	17.69%	3.044%
16	15.762	2320	2325	2331	rVB	61744	90128	1.50%	0.259%
17	16.239	2400	2406	2414	rVB2	47845	88080	1.47%	0.253%


Sum of corrected areas: 34831776

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF022420\
Data File : BF119025.D
Acq On : 24 Feb 2020 16:08
Operator : CG/JU
Sample : PB127021BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB127021BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

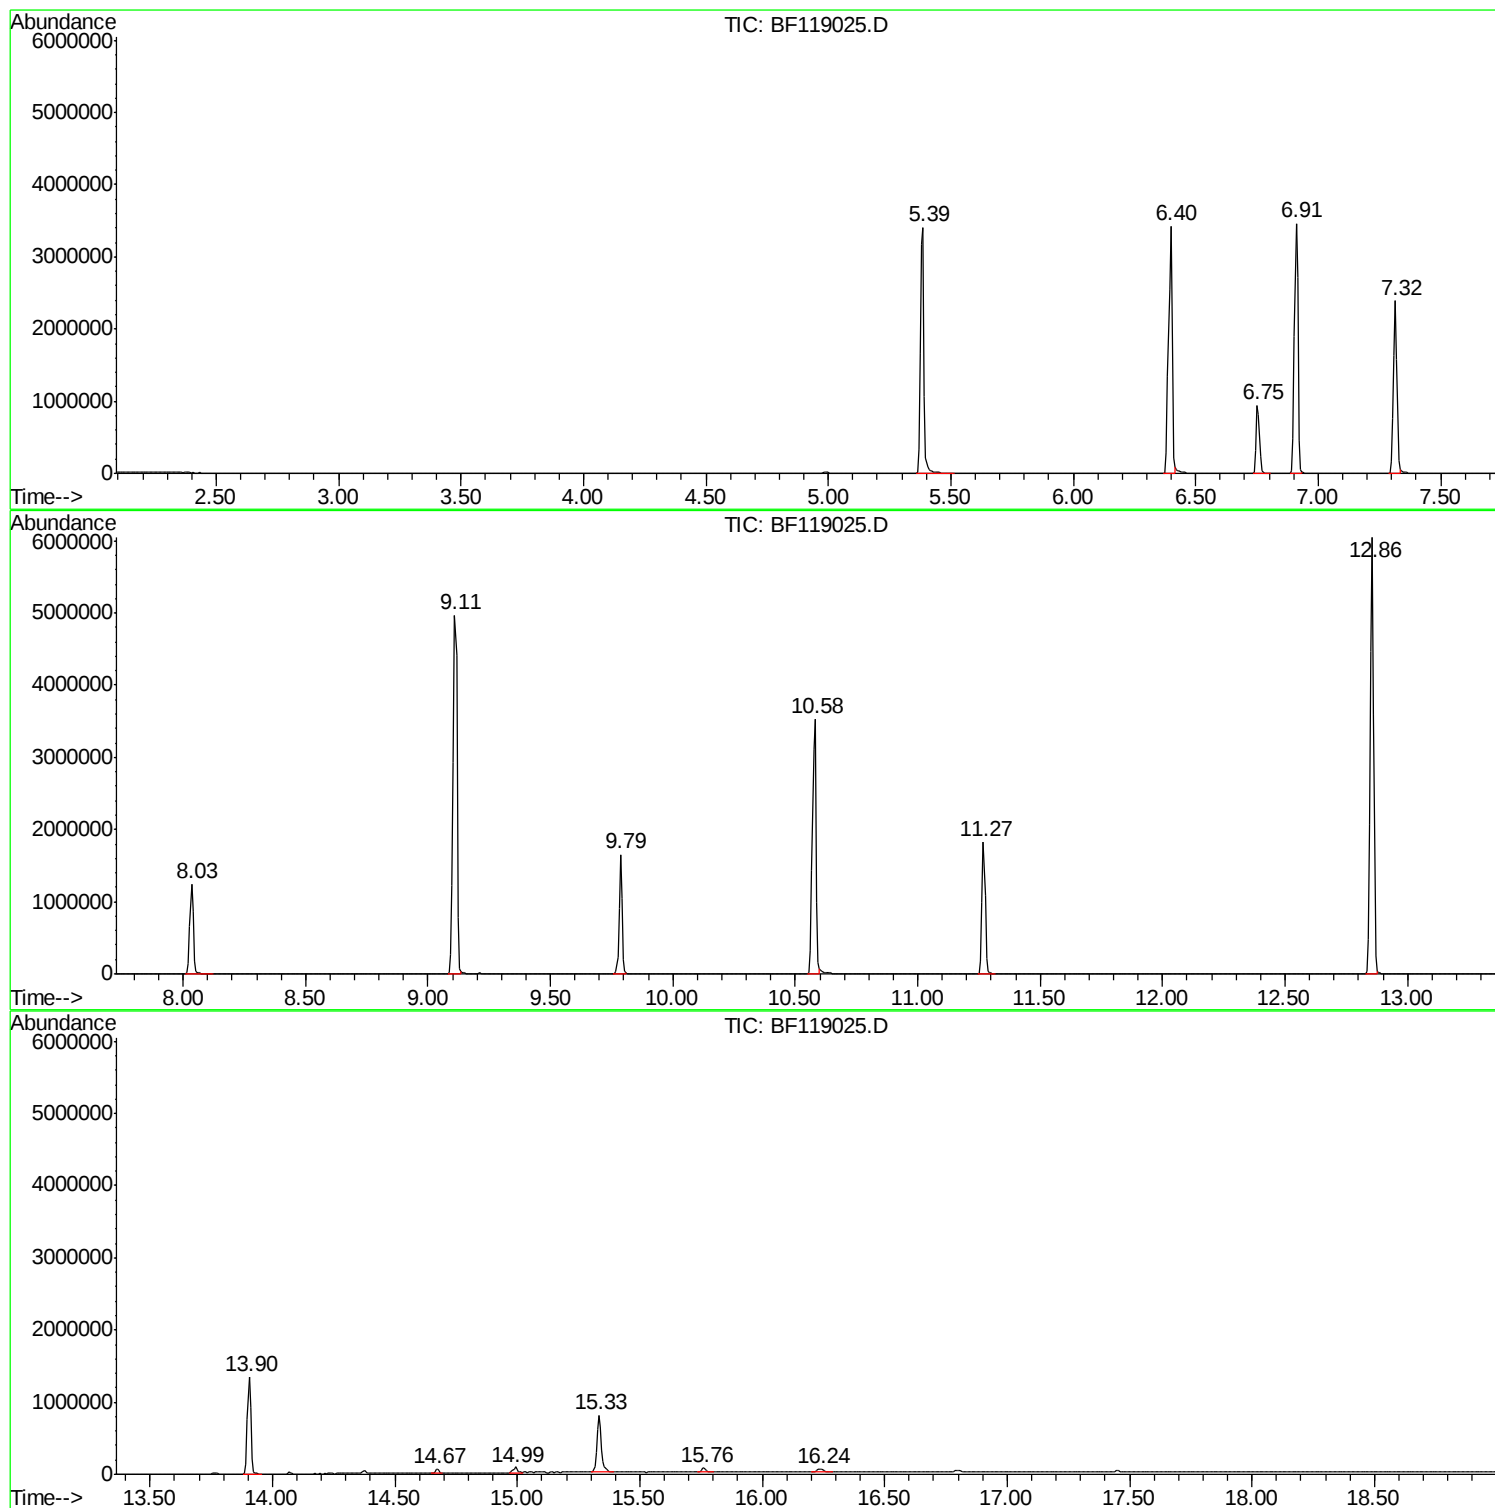

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF022420\
Data_File : BF119025.D
Acq_On : 24 Feb 2020 16:088
Operator : CG/JUU
Sample : PB127021BLL
Misc :
ALS_Vial : 13 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
PB127021BL

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022020.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
