


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF022420\
 Data File : BF119013.D
 Acq On : 24 Feb 2020 9:42
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Feb 20 17:40:17 2020

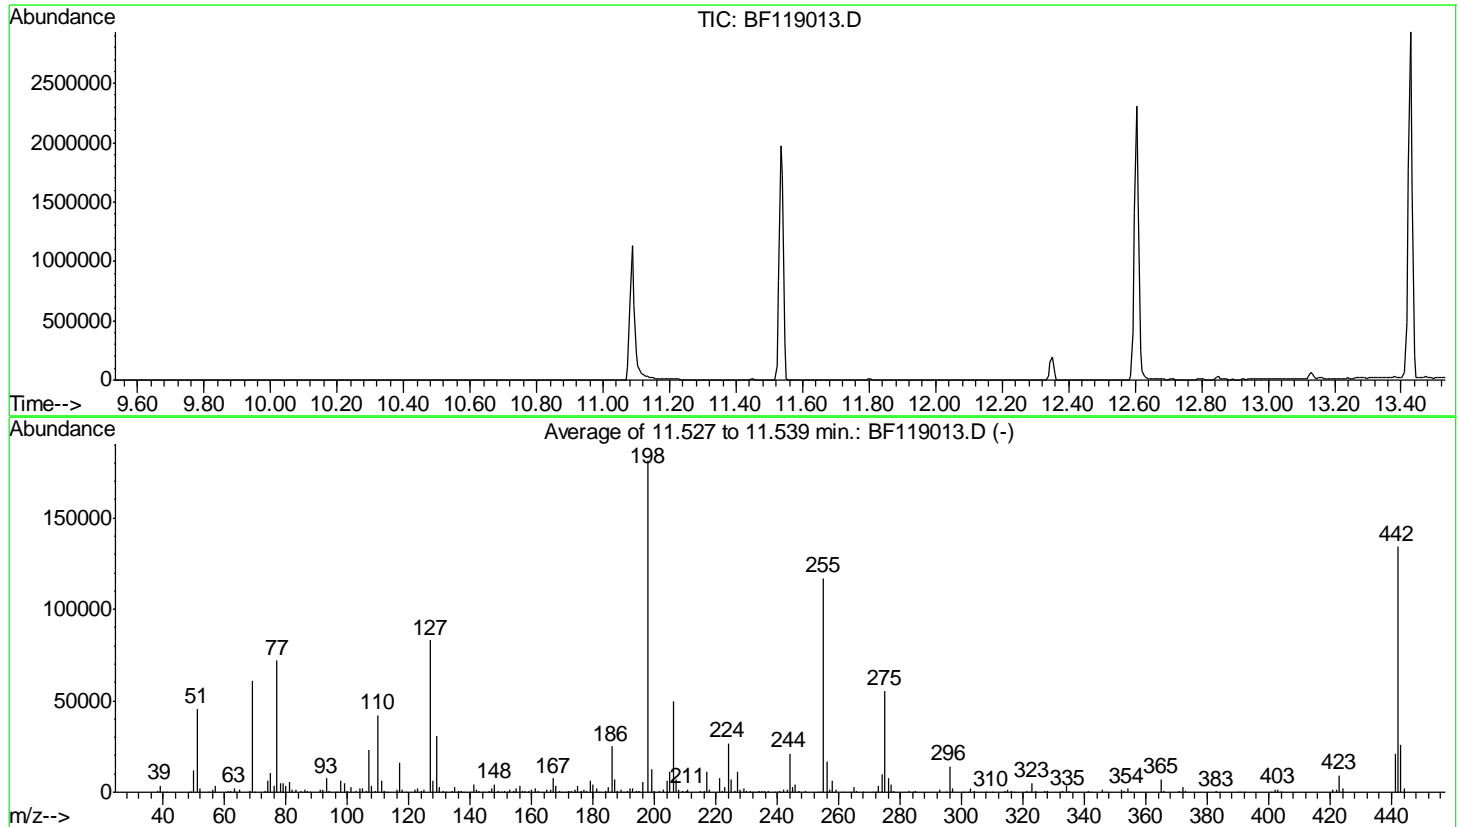

AutoFind: Scans 1605, 1606, 1607; Background Corrected with Scan 1600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.1	45533	PASS
68	69	0.00	2	1.5	896	PASS
69	198	0.00	100	33.4	60605	PASS
70	69	0.00	2	0.3	152	PASS
127	198	10	80	45.8	83141	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	181360	PASS
199	198	5	9	6.8	12379	PASS
275	198	10	60	30.6	55552	PASS
365	198	1	100	3.9	7126	PASS
441	198	0.01	100	11.7	21270	PASS
442	198	50	100	74.0	134154	PASS
443	442	15	24	19.2	25691	PASS