


Data Path : Z:\SVOASRV\HPCHEM1\BNA\_F\DATA\BF022420\  
 Data File : BF119026.D  
 Acq On : 24 Feb 2020 17:18  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF022020.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Thu Feb 20 17:40:17 2020

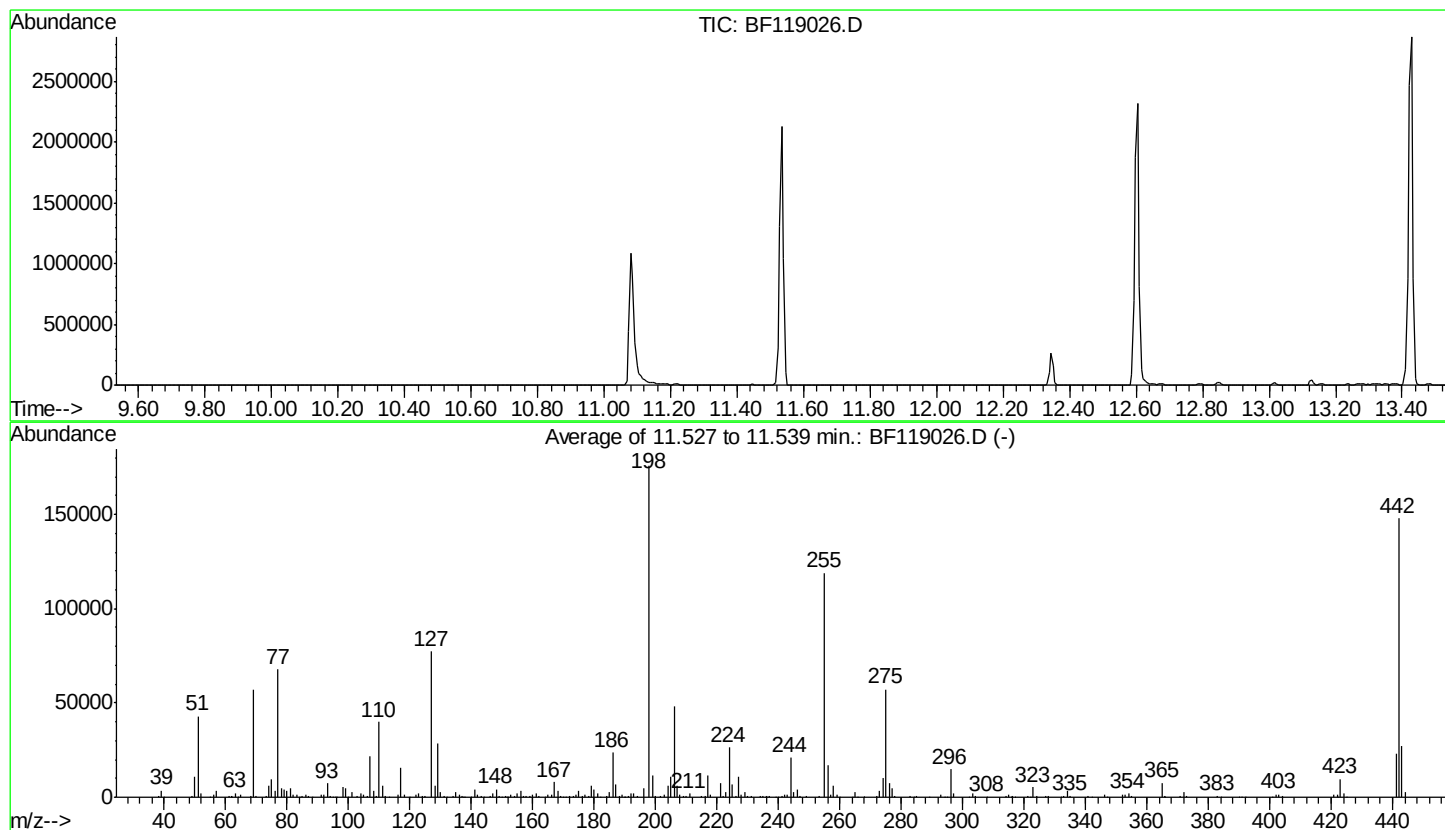

AutoFind: Scans 1605, 1606, 1607; Background Corrected with Scan 1600

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 24.5         | 43048      | PASS                |
| 68             | 69              | 0.00            | 2               | 0.8          | 431        | PASS                |
| 69             | 198             | 0.00            | 100             | 32.4         | 57013      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.7          | 392        | PASS                |
| 127            | 198             | 10              | 80              | 44.0         | 77304      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 175888     | PASS                |
| 199            | 198             | 5               | 9               | 6.7          | 11780      | PASS                |
| 275            | 198             | 10              | 60              | 32.5         | 57136      | PASS                |
| 365            | 198             | 1               | 100             | 4.3          | 7497       | PASS                |
| 441            | 198             | 0.01            | 100             | 13.0         | 22801      | PASS                |
| 442            | 198             | 50              | 100             | 84.1         | 147957     | PASS                |
| 443            | 442             | 15              | 24              | 18.4         | 27159      | PASS                |