


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF022420\
 Data File : BF119051.D
 Acq On : 25 Feb 2020 6:16
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Feb 20 17:40:17 2020

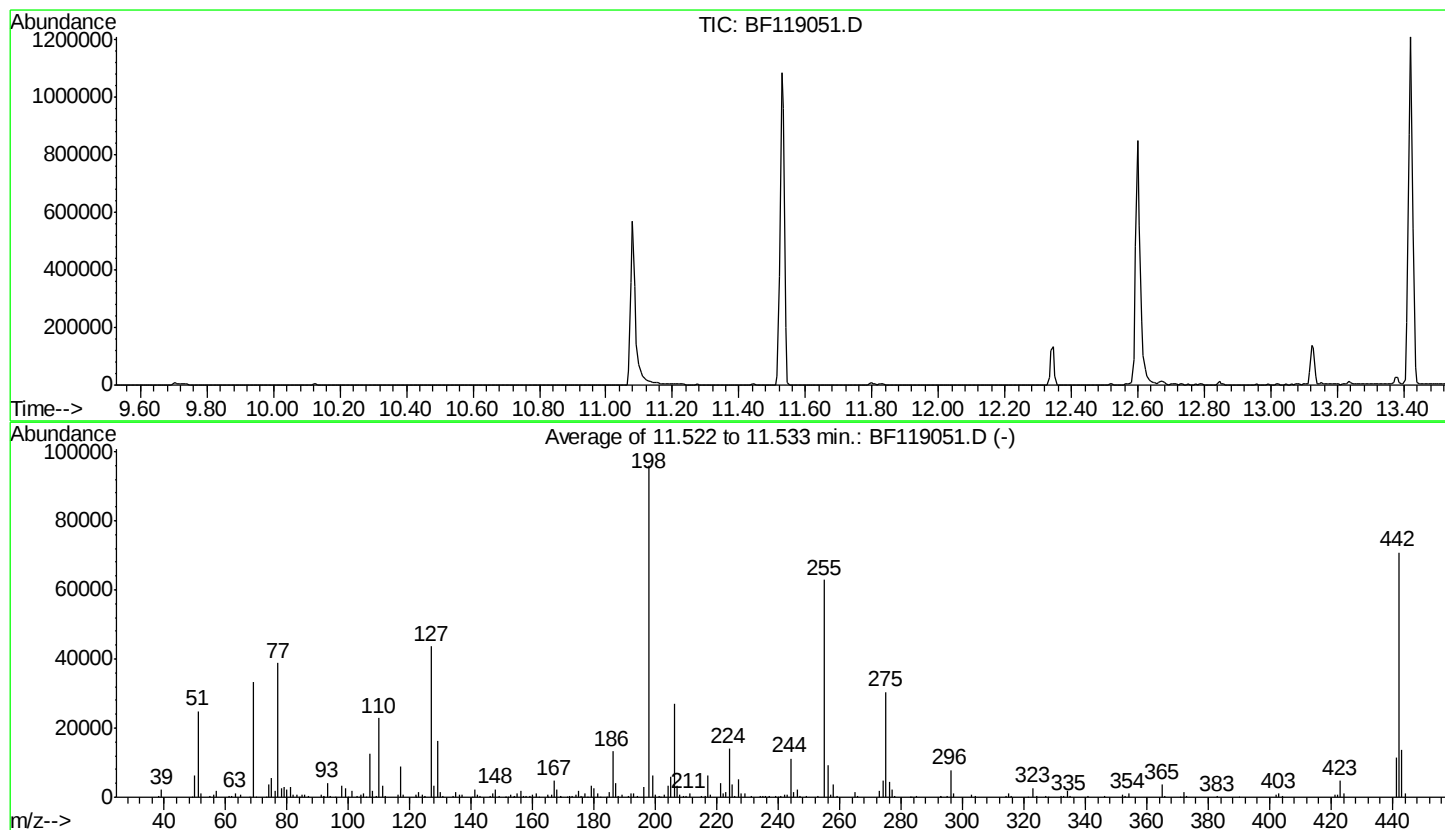

AutoFind: Scans 1604, 1605, 1606; Background Corrected with Scan 1600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.0	24917	PASS
68	69	0.00	2	0.6	197	PASS
69	198	0.00	100	34.9	33490	PASS
70	69	0.00	2	0.3	117	PASS
127	198	10	80	45.4	43600	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	95946	PASS
199	198	5	9	6.7	6449	PASS
275	198	10	60	31.7	30431	PASS
365	198	1	100	3.8	3674	PASS
441	198	0.01	100	11.9	11462	PASS
442	198	50	100	73.9	70860	PASS
443	442	15	24	19.3	13678	PASS