
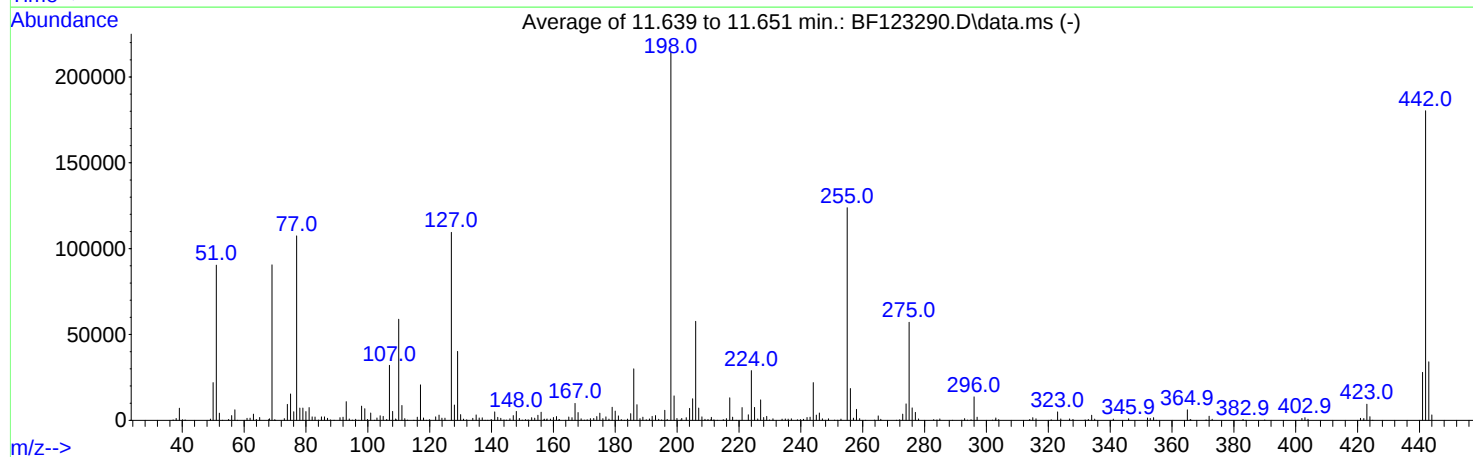


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022421\
 Data File : BF123290.D
 Acq On : 24 Feb 2021 12:37
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 19 16:08:53 2021

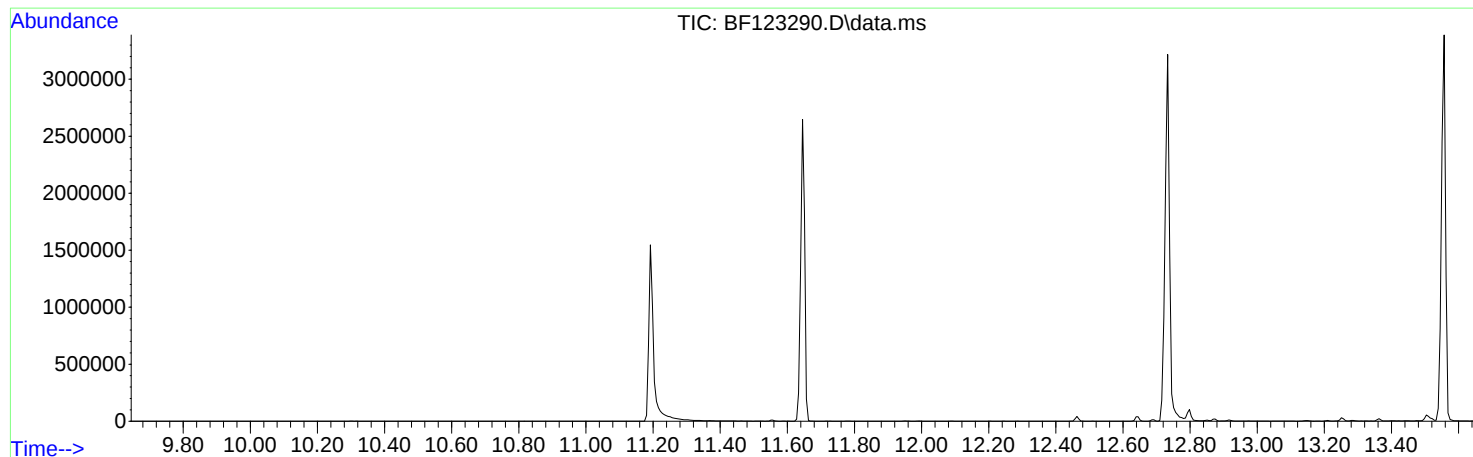




AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.2	90411	PASS
68	69	0.00	2	1.0	947	PASS
69	198	0.00	100	42.3	90584	PASS
70	69	0.00	2	0.5	415	PASS
127	198	10	80	51.1	109507	PASS
197	198	0.00	2	0.2	529	PASS
198	198	100	100	100.0	214251	PASS
199	198	5	9	6.7	14260	PASS
275	198	10	60	26.6	57093	PASS
365	198	1	100	2.9	6164	PASS
441	198	0.01	100	13.1	27999	PASS
442	442	50	100	100.0	180325	PASS
443	442	15	24	18.9	34066	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022421\
Data File : BF123290.D
Acq On : 24 Feb 2021 12:37
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 24 13:33:55 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 19 16:08:53 2021
Response via : Initial Calibration

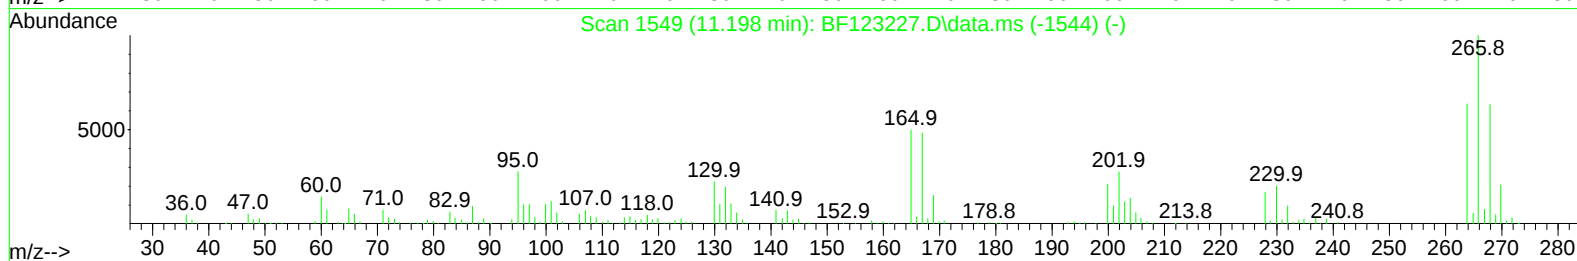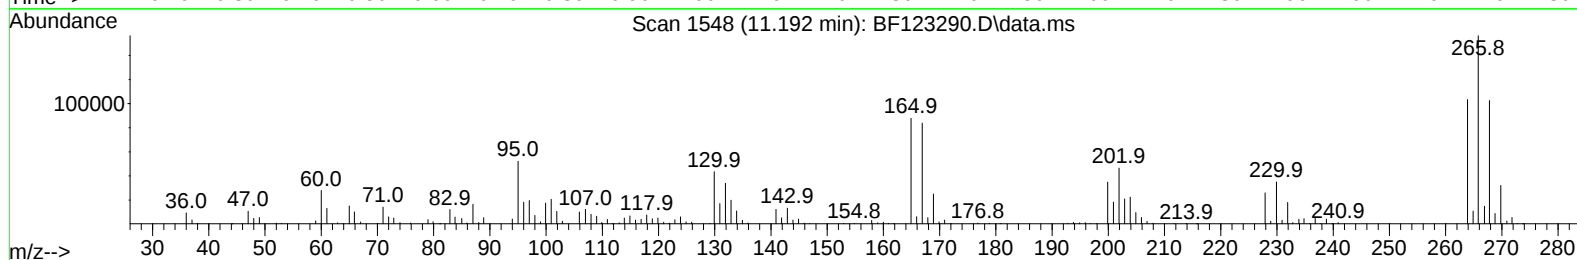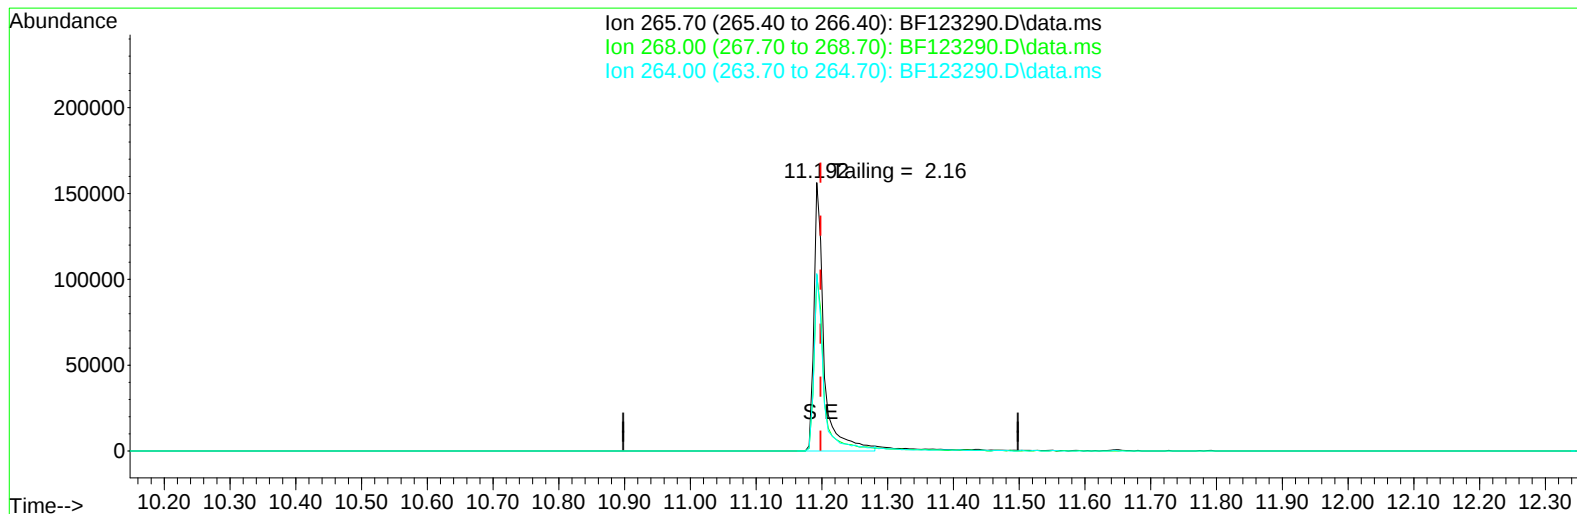

TIC: BF123290.D\data.ms

(70) Pentachlorophenol (C)

11.192min (-0.006) 22459.25 ng




response 173448

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	65.62
264.00	62.30	66.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022421\
 Data File : BF123290.D
 Acq On : 24 Feb 2021 12:37
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Feb 24 13:33:55 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 19 16:08:53 2021
 Response via : Initial Calibration

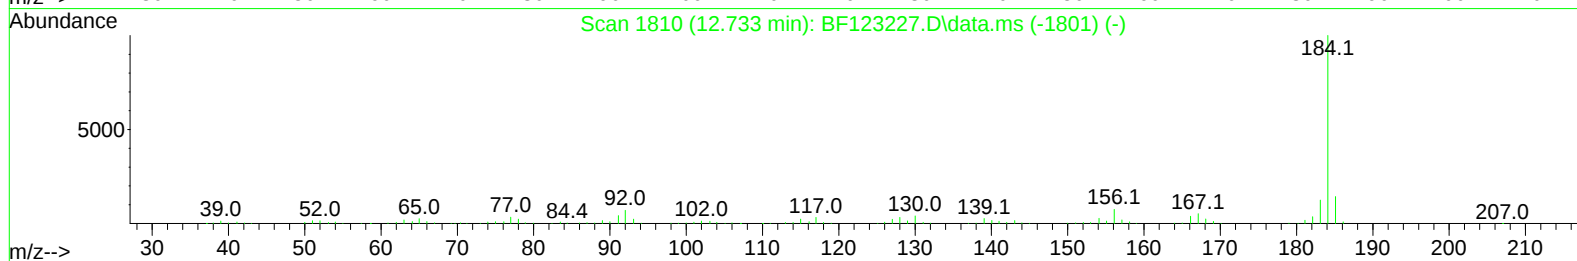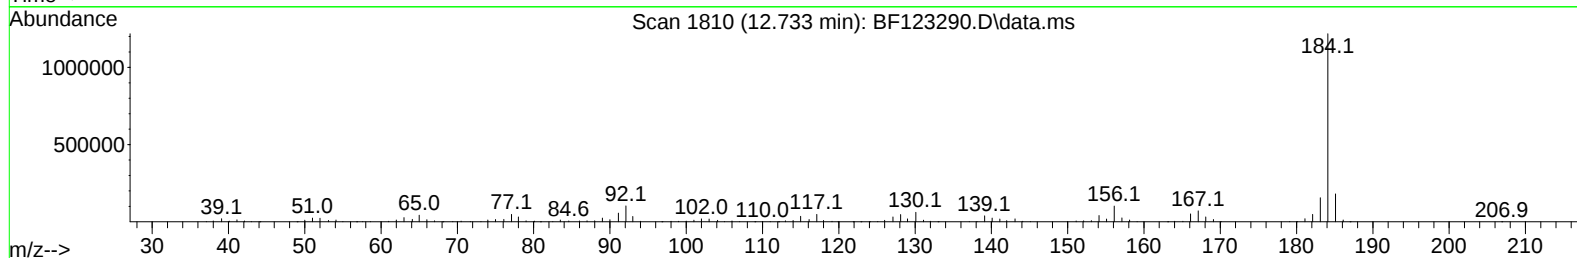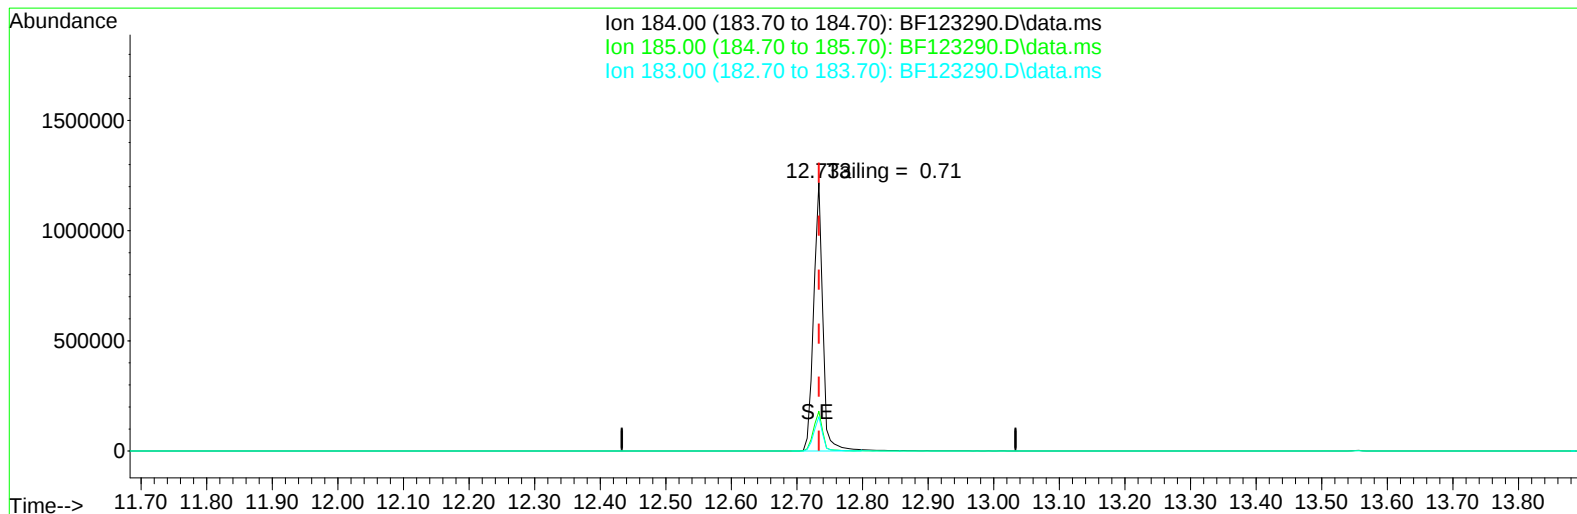

TIC: BF123290.D\data.ms

(77) Benzidine

12.733min (+ 0.000) 0.00 ng

response 1182472

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.82
183.00	12.10	12.77
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/24/2021	BNA_F	BF123290.D
Compound Name	Response	Retention Time
DDT	536759	13.55
DDD	5331	13.25
DDE	1788	12.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7119	543878	1.31

Instrument :
BNA_F
ClientSampleId :
DFTPP