


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022423\
Data File : BF132537.D
Acq On : 24 Feb 2023 11:41
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Feb 24 23:17:30 2023

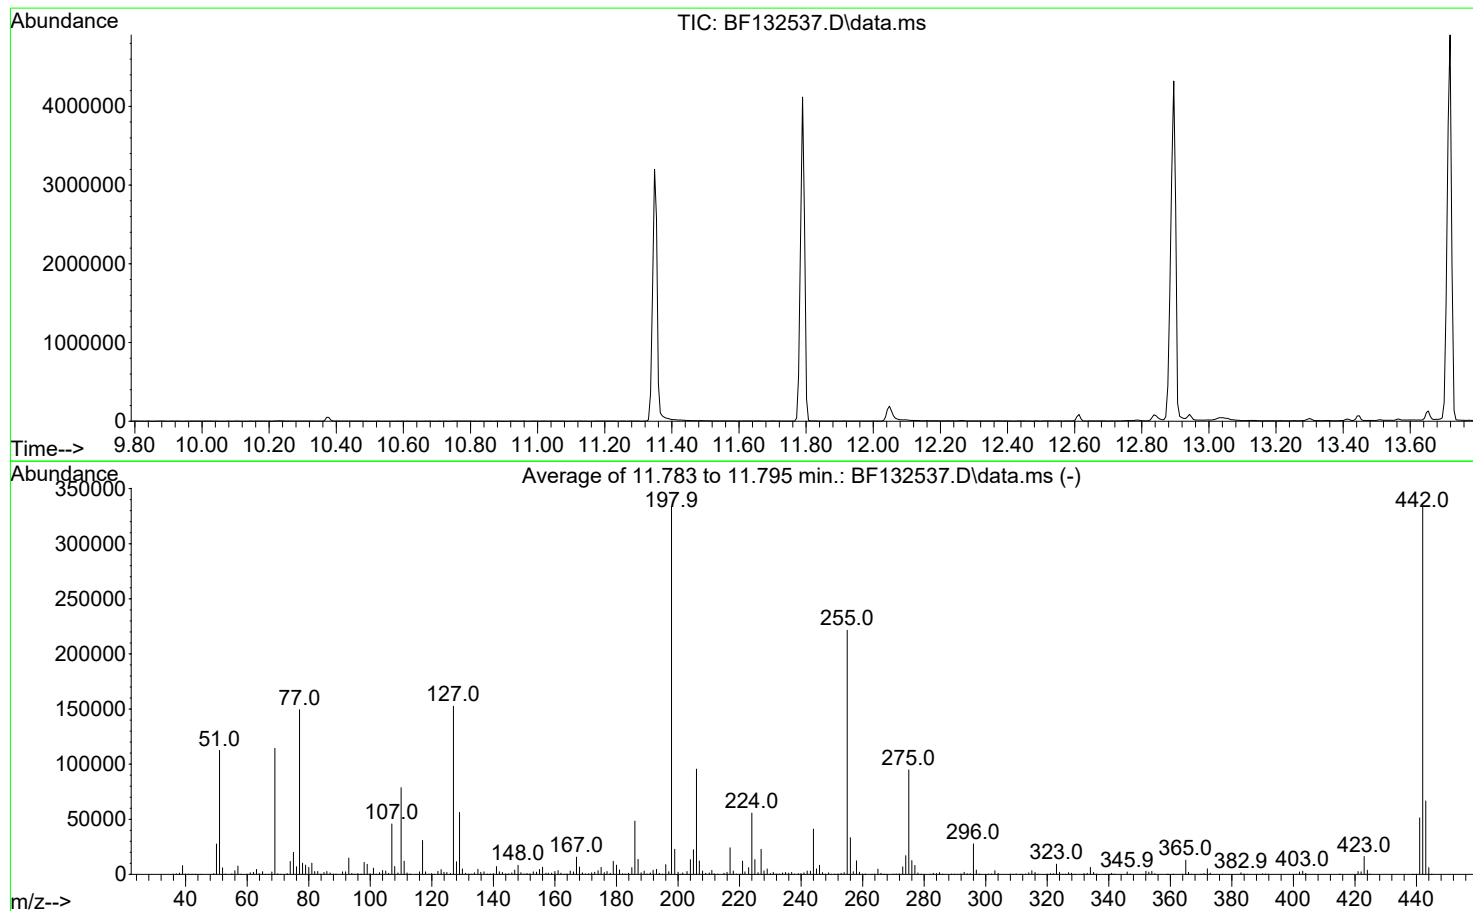

AutoFind: Scans 1521, 1522, 1523; Background Corrected with Scan 1516

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.7	112477	PASS
68	69	0.00	2	1.8	2117	PASS
69	198	0.00	100	34.3	114456	PASS
70	69	0.00	2	0.5	620	PASS
127	198	10	80	45.7	152632	PASS
197	198	0.00	2	0.7	2419	PASS
198	198	100	100	100.0	333781	PASS
199	198	5	9	6.8	22848	PASS
275	198	10	60	28.4	94755	PASS
365	198	1	100	3.9	12993	PASS
441	198	0.01	100	15.3	51197	PASS
442	442	50	100	100.0	333739	PASS
443	442	15	24	20.0	66603	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/24/2023	BNA_F	<u>BF132537.D</u>
Compound Name	Response	Retention Time
DDT	886664	13.719
DDD	15161	13.448
DDE	830	13.07
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15991	902655	1.77

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022423\
Data File : BF132537.D
Acq On : 24 Feb 2023 11:41
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 25 00:09:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 24 23:17:30 2023
Response via : Initial Calibration

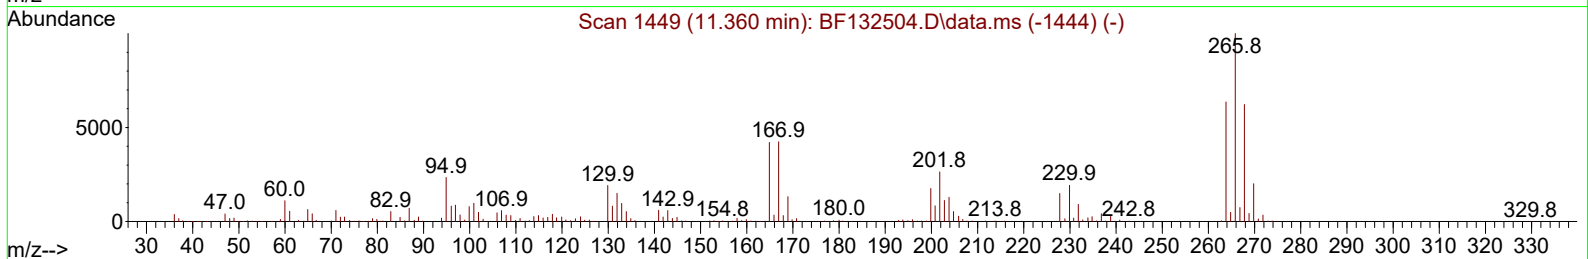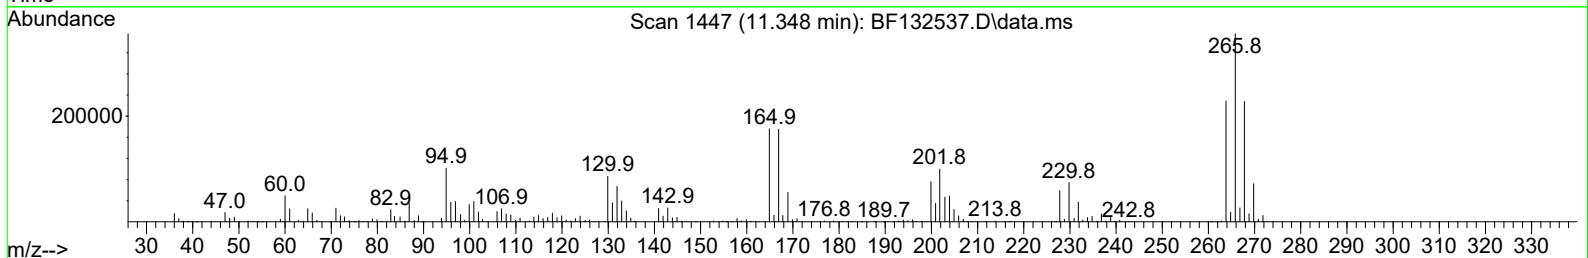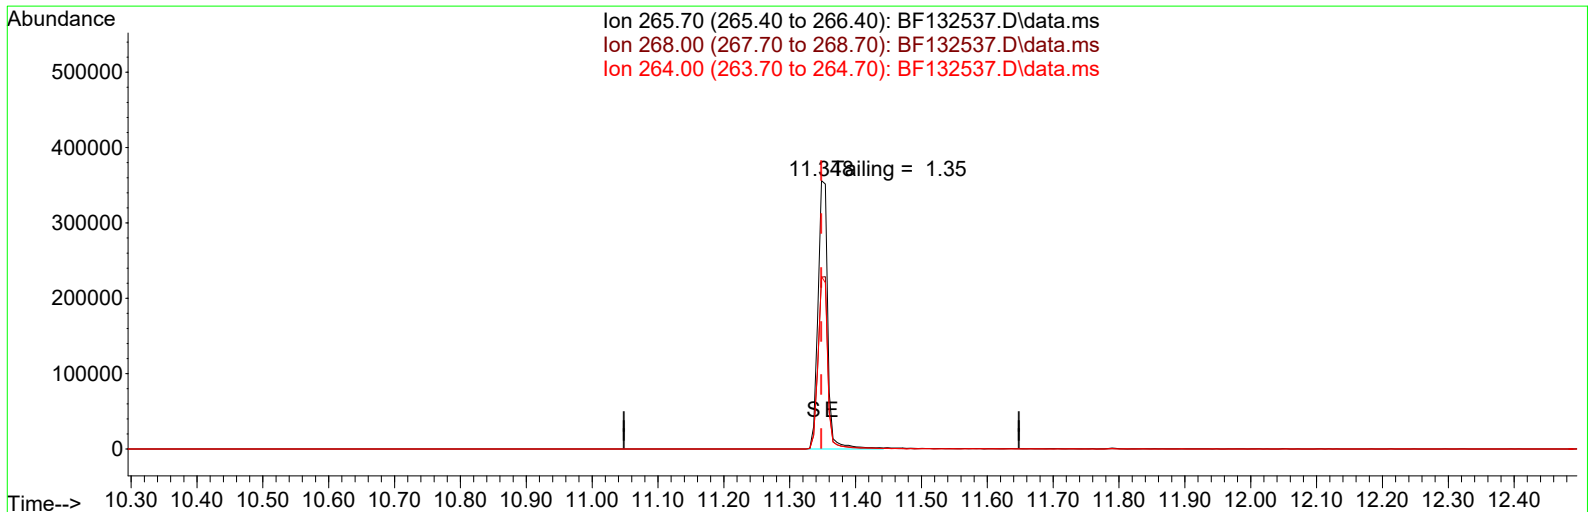

TIC: BF132537.D\data.ms

(70) Pentachlorophenol (C)

11.348min (+ 0.000) 770717.28 ng




response 371133

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.06
264.00	63.60	64.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022423\
Data File : BF132537.D
Acq On : 24 Feb 2023 11:41
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 25 00:09:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 24 23:17:30 2023
Response via : Initial Calibration

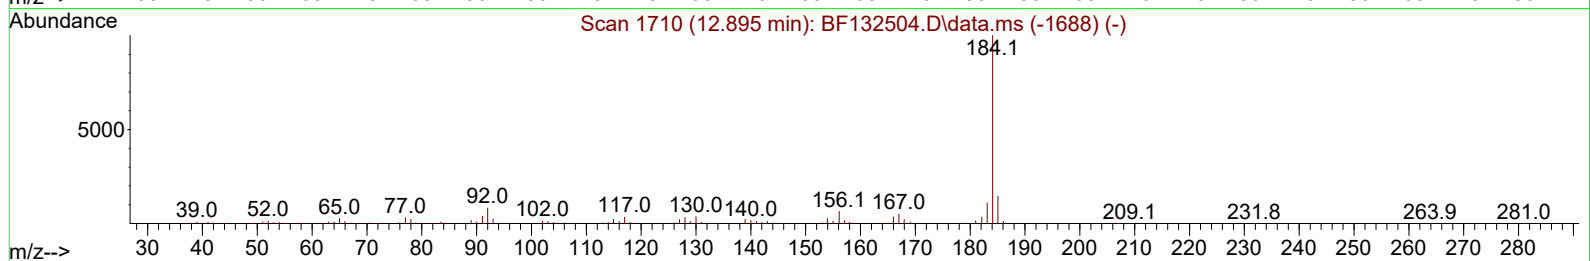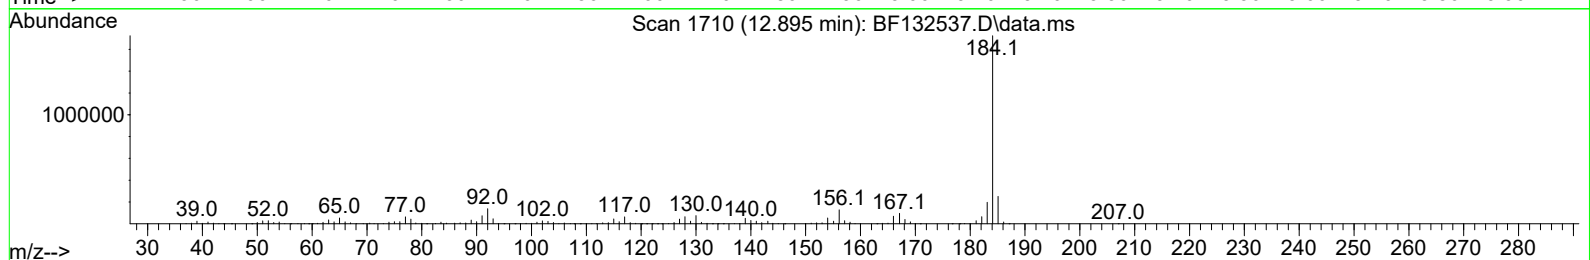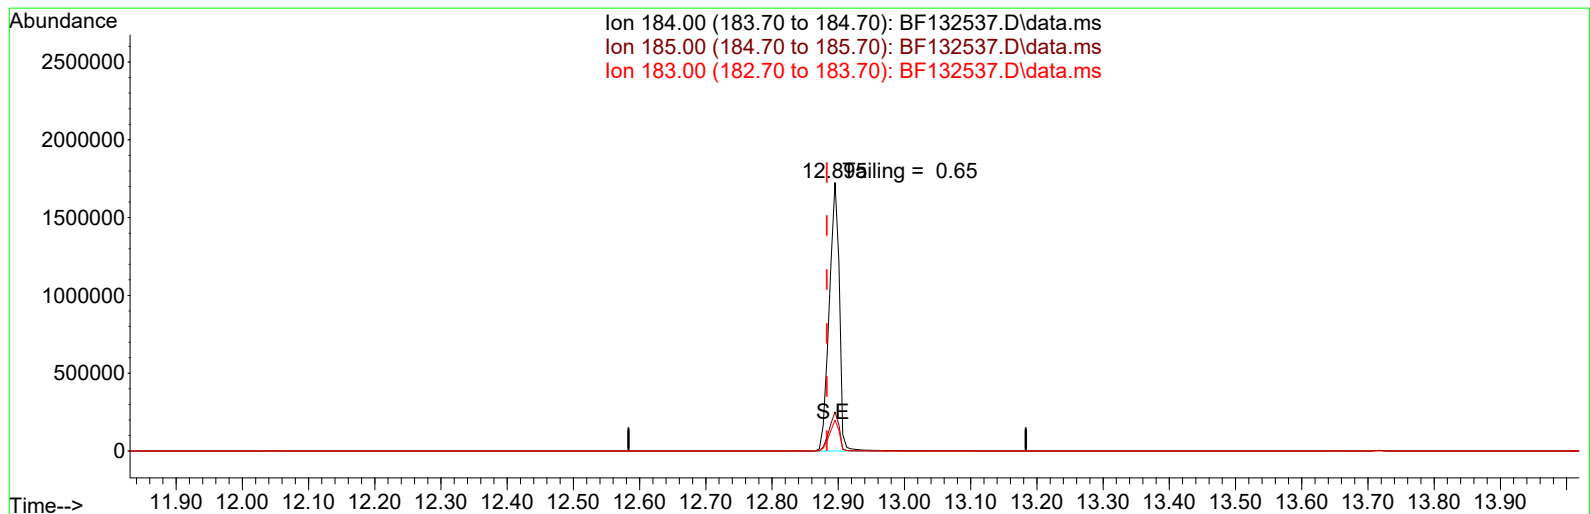

TIC: BF132537.D\data.ms

(77) Benzidine

12.895min (+ 0.012) 80716.34 ng

response 1837150

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.57
183.00	10.90	11.46
0.00	0.00	0.00