
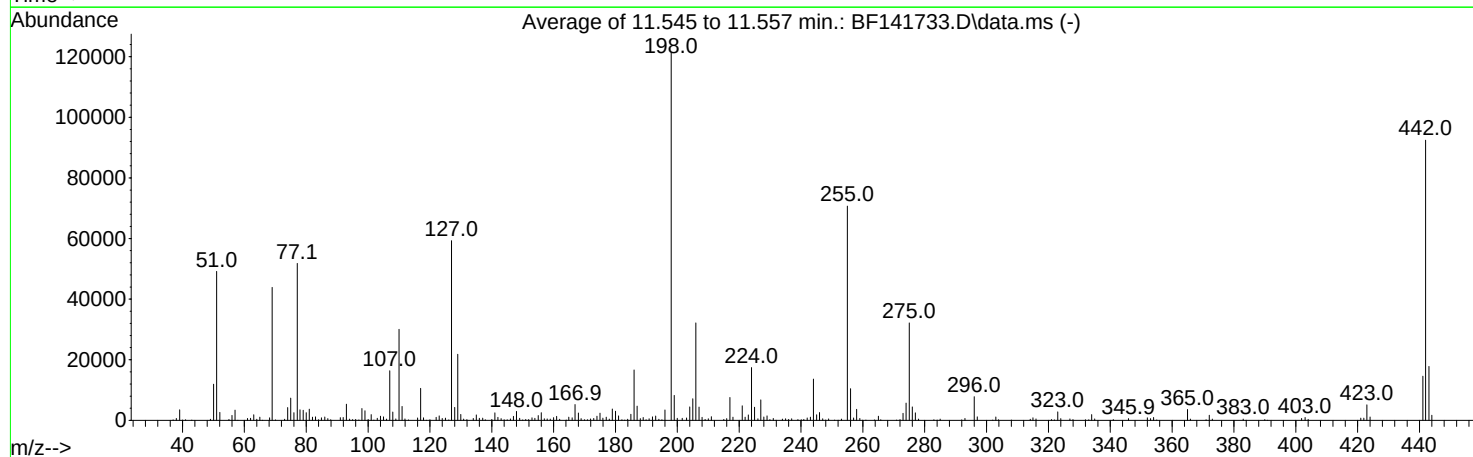


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022425\
Data File : BF141733.D
Acq On : 24 Feb 2025 09:23
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 06 16:58:59 2025

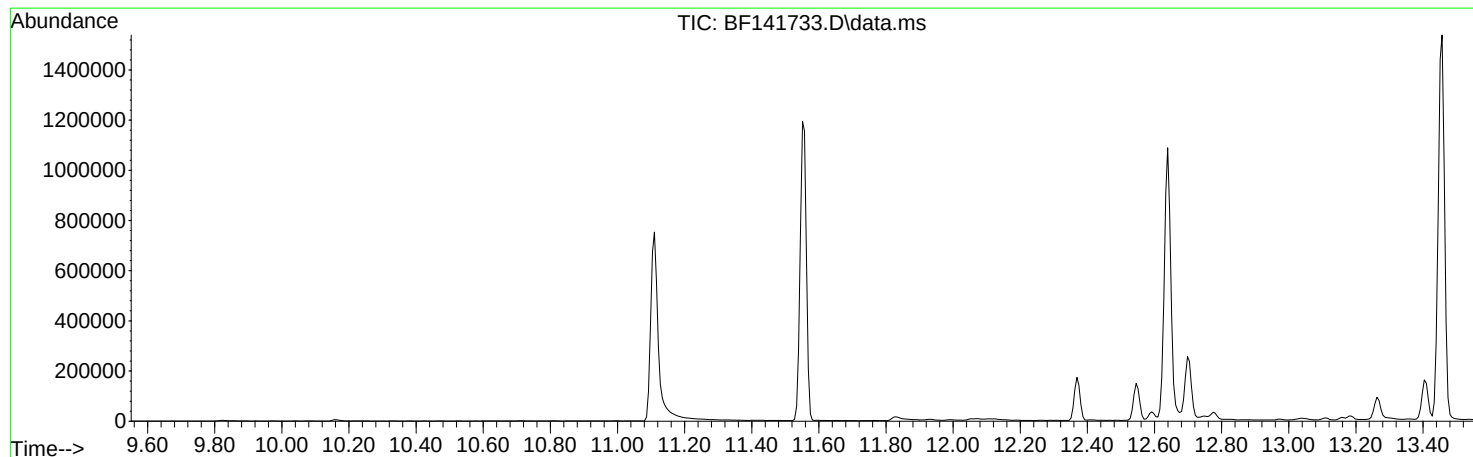

AutoFind: Scans 1607, 1608, 1609; Background Corrected with Scan 1601

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.5	49141	PASS
68	69	0.00	2	2.0	862	PASS
69	198	0.00	100	36.1	43853	PASS
70	69	0.00	2	0.4	180	PASS
127	198	10	80	48.8	59288	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	121379	PASS
199	198	5	9	6.8	8254	PASS
275	198	10	60	26.5	32165	PASS
365	198	1	100	3.0	3618	PASS
441	198	0.01	100	12.0	14598	PASS
442	442	50	100	100.0	92464	PASS
443	442	15	24	19.3	17808	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/24/2025	BNA_F	<u>BF141733.D</u>
Compound Name	Response	Retention Time
DDT	398328	13.457
DDD	8590	13.186
DDE	476	12.822
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9066	407394	2.23

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022425\
Data File : BF141733.D
Acq On : 24 Feb 2025 09:23
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 24 11:02:38 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 16:58:59 2025
Response via : Initial Calibration

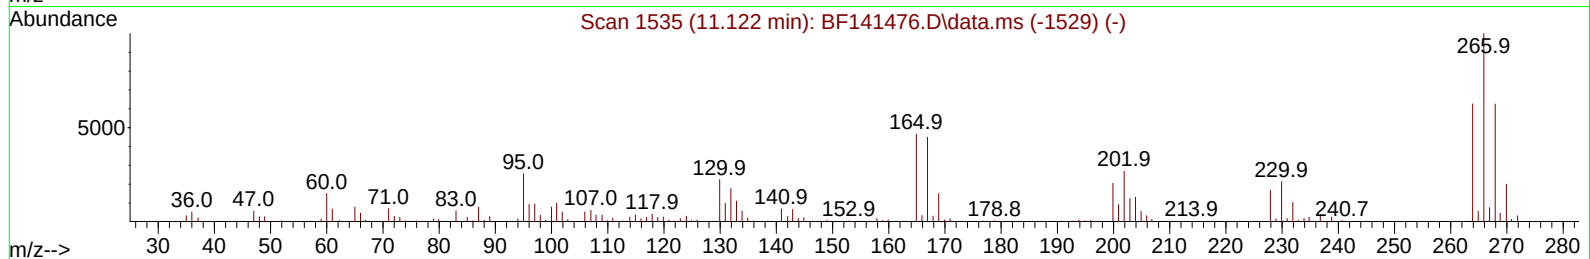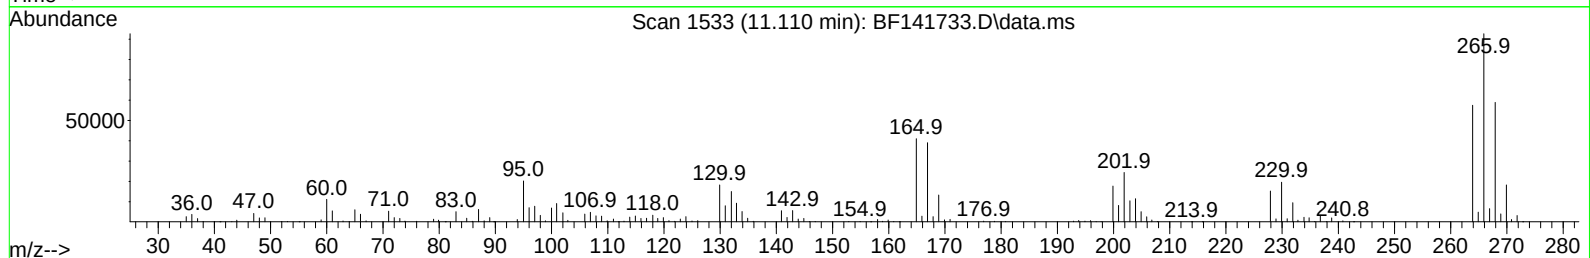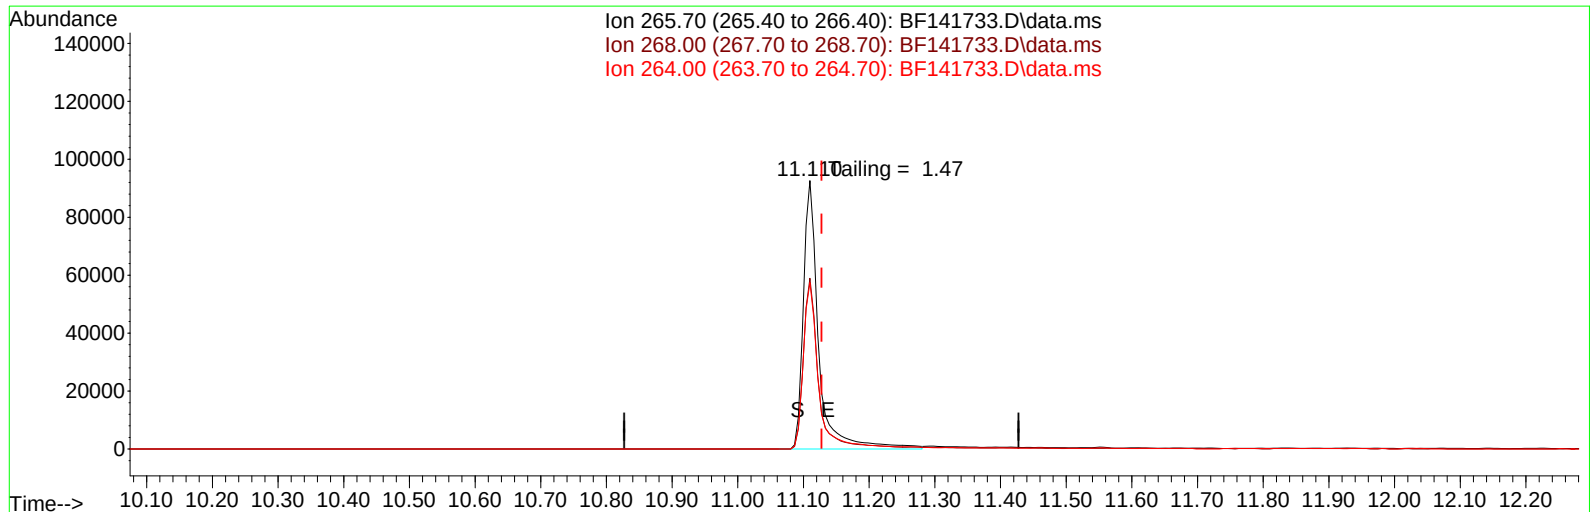

TIC: BF141733.D\data.ms

(70) Pentachlorophenol (C)

11.110min (-0.017) 26925.78 ng




response 150984

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	63.59
264.00	62.60	62.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022425\
Data File : BF141733.D
Acq On : 24 Feb 2025 09:23
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 24 11:02:38 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 16:58:59 2025
Response via : Initial Calibration

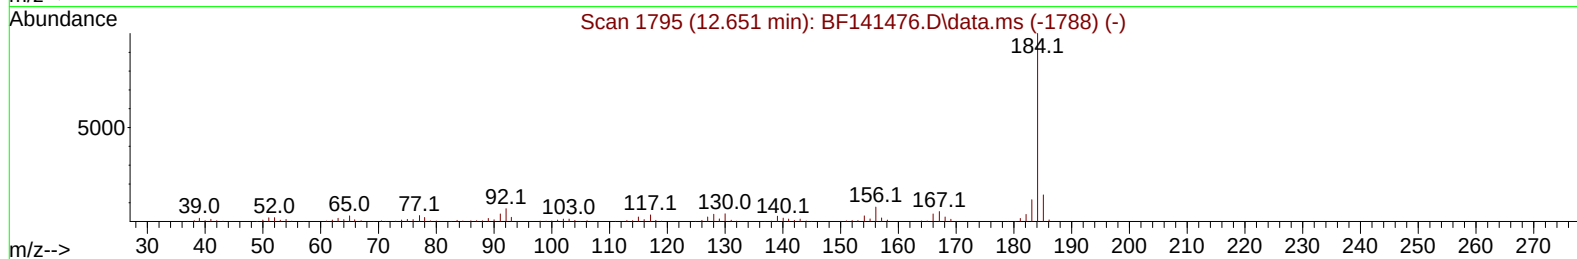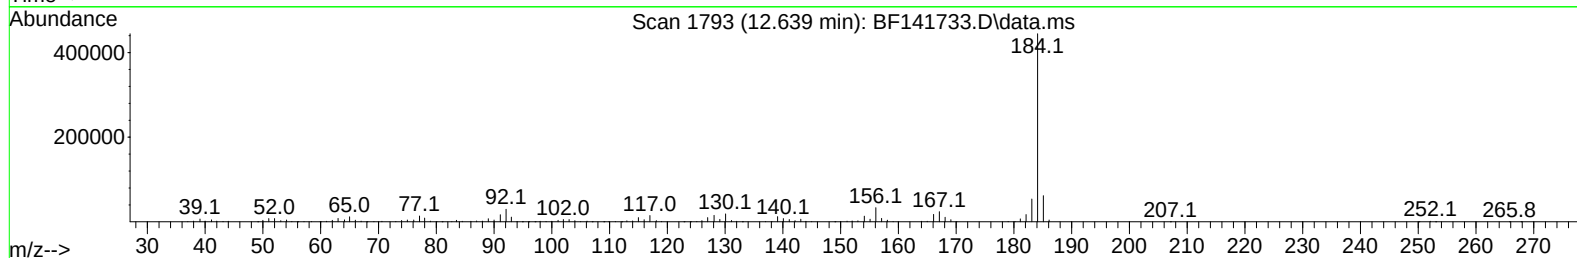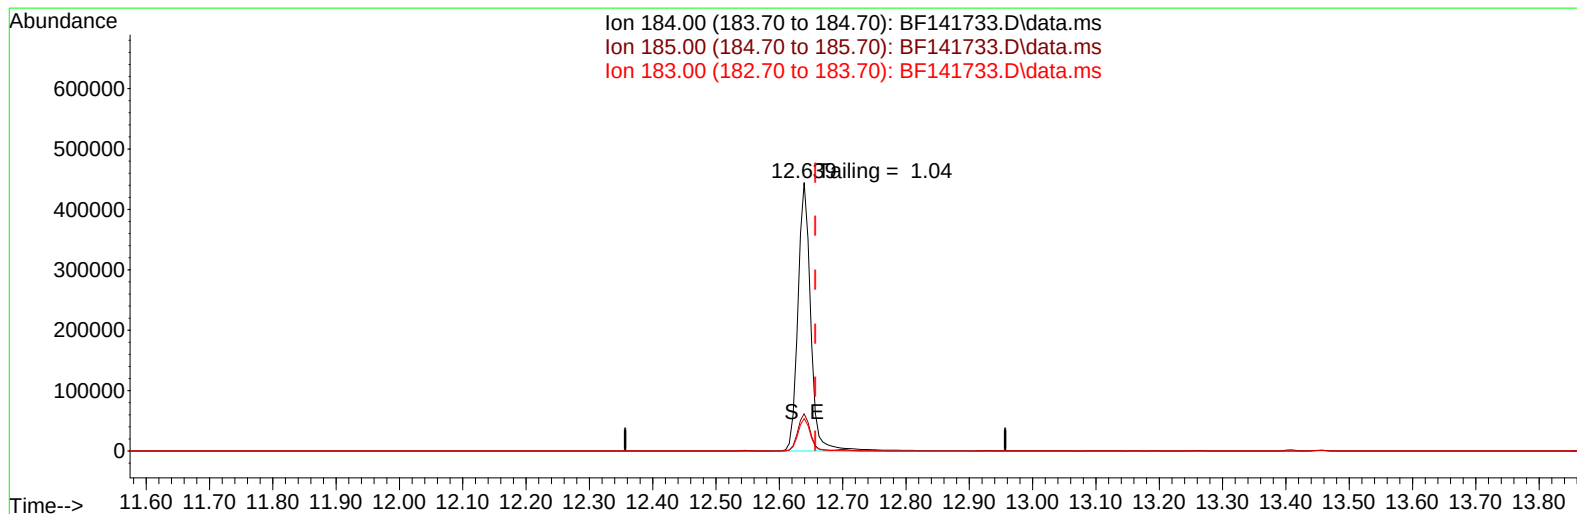

TIC: BF141733.D\data.ms

(77) Benzidine

12.639min (-0.017) 0.00 ng

response 628483

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.90
183.00	11.60	12.09
0.00	0.00	0.00