


Data Path : Z:\HPCHEM1\BNA_F\Data\BF022515\
 Data File : BF077428.D
 Acq On : 25 Feb 2015 11:33
 Operator : IZ / TP
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Feb 19 16:57:32 2015

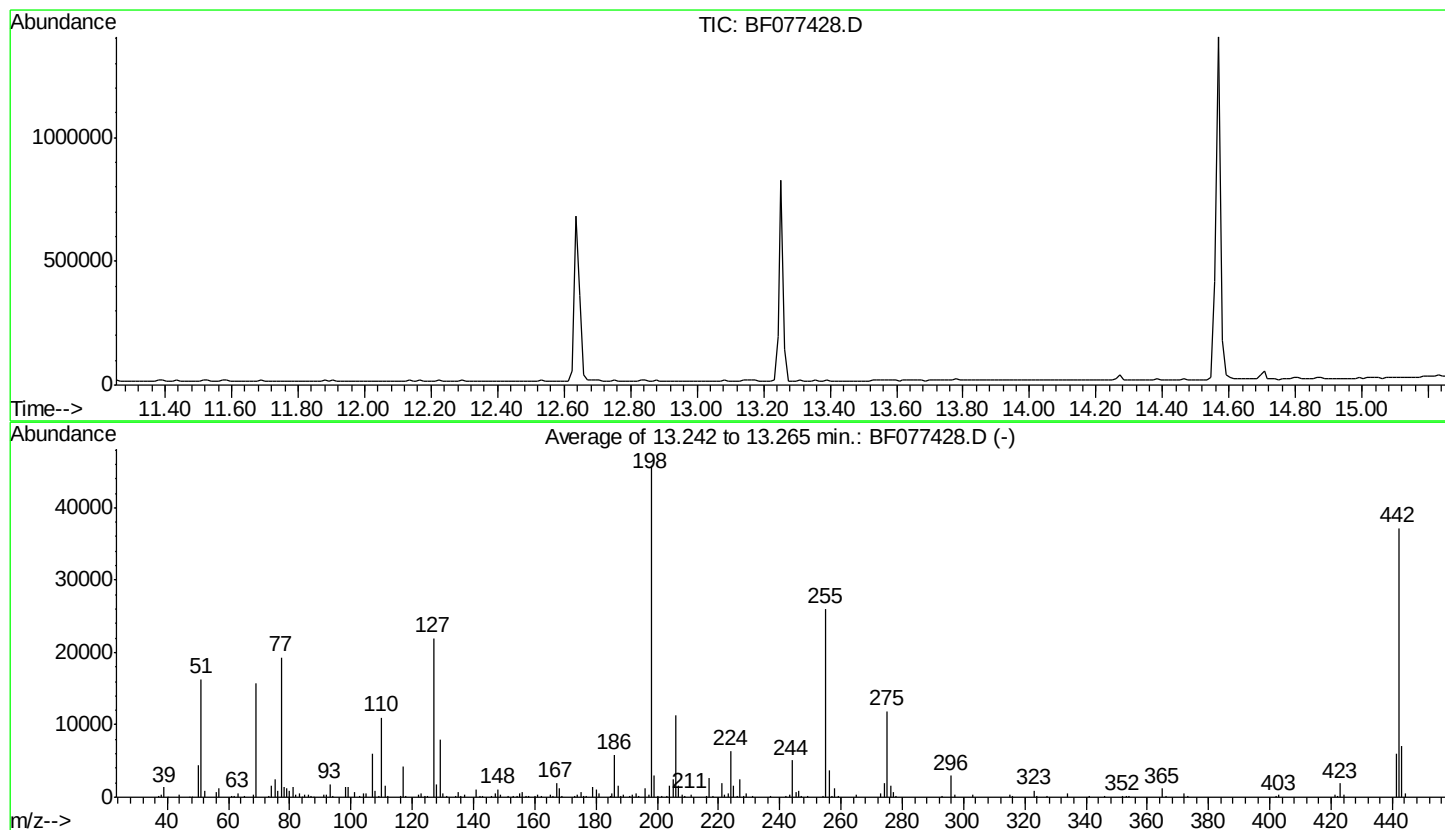

AutoFind: Scans 1081, 1082, 1083; Background Corrected with Scan 1078

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.6	16305	PASS
68	69	0.00	2	1.8	284	PASS
69	198	0.00	100	34.5	15818	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.0	22006	PASS
197	198	0.00	2	0.6	275	PASS
198	198	100	100	100.0	45810	PASS
199	198	5	9	6.4	2947	PASS
275	198	10	60	26.0	11908	PASS
365	198	1	100	2.5	1162	PASS
441	442	0.01	24	16.1	5992	PASS
442	198	50	100	81.2	37202	PASS
443	442	15	24	19.2	7130	PASS