

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF022515\
 Data File : BF077435.D
 Acq On : 25 Feb 2015 15:58
 Operator : IZ / TP
 Sample : G1353-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FB

Quant Time: Feb 26 03:36:41 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021915.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 26 03:18:41 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.29	152	77282	20.00	ng	0.00
21) Naphthalene-d8	8.86	136	306200	20.00	ng	0.00
38) Acenaphthene-d10	11.04	164	156540	20.00	ng	0.00
63) Phenanthrene-d10	12.88	188	301352	20.00	ng	-0.01
75) Chrysene-d12	16.17	240	328062	20.00	ng	-0.01
86) Perylene-d12	17.94	264	334337	20.00	ng	0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.58	112	235383	50.85	ng	0.00
7) Phenol-d6	6.84	99	195380	32.83	ng	0.00
23) Nitrobenzene-d5	7.97	82	480736	97.63	ng	-0.01
41) 2,4,6-Tribromophenol	12.02	330	159855	106.06	ng	0.00
44) 2-Fluorobiphenyl	10.21	172	1084626	108.04	ng	0.00
78) Terphenyl-d14	14.88	244	1234556	87.97	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF022515\
Data File : BF077435.D
Acq On : 25 Feb 2015 15:58
Operator : IZ / TP
Sample : G1353-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FB

Quant Time: Feb 26 03:36:41 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 26 03:18:41 2015
Response via : Initial Calibration

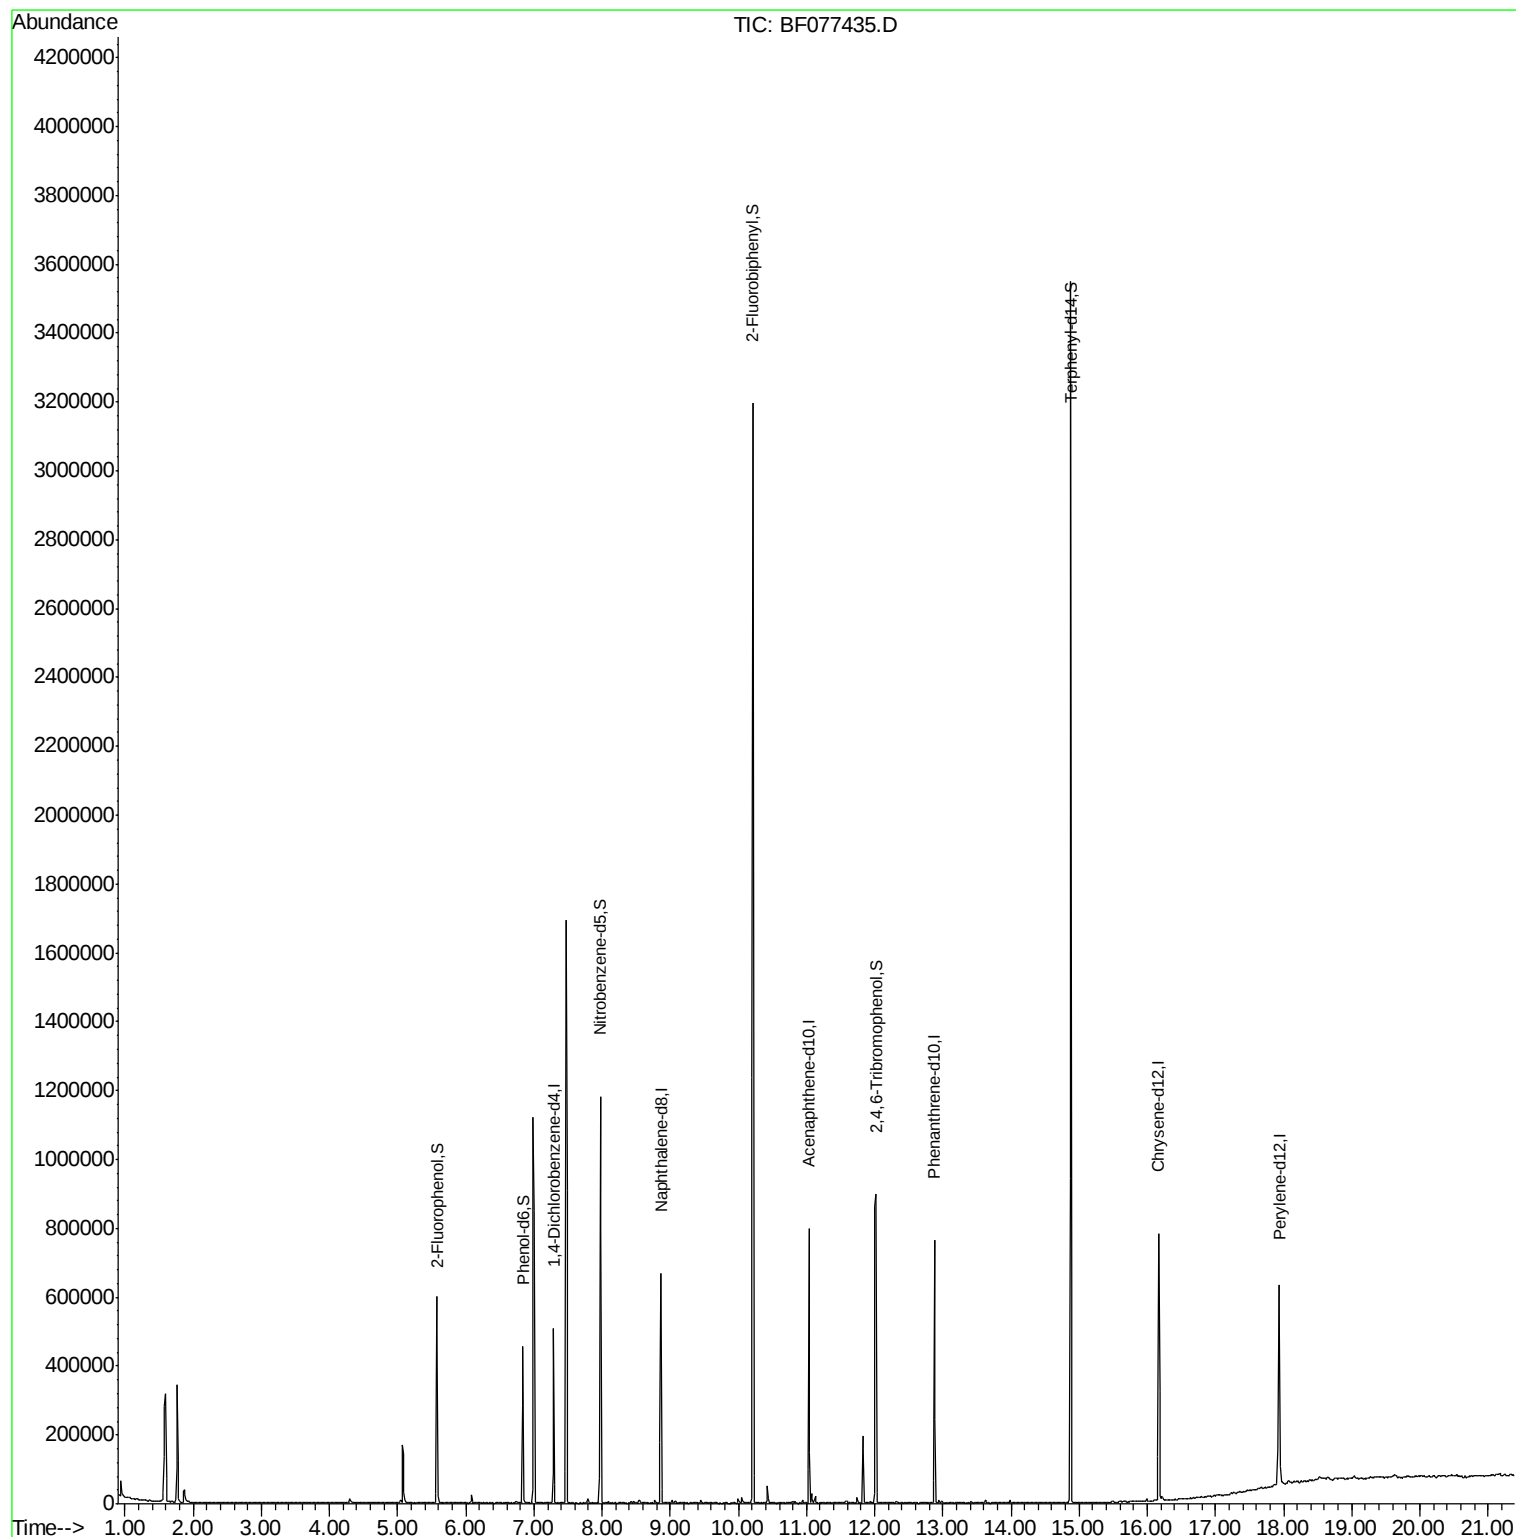




#1




1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 7.29 min Scan# 560
 Delta R.T. -0.00 min
 Lab File: BF077435.D
 Acq: 25 Feb 2015 15:58

Instrument :
 BNA_F
 ClientSampleId :
 FB

Tgt Ion:152 Resp: 77282
 Ion Ratio Lower Upper
 152 100
 150 154.9 124.0 186.0
 115 58.8 49.4 74.2

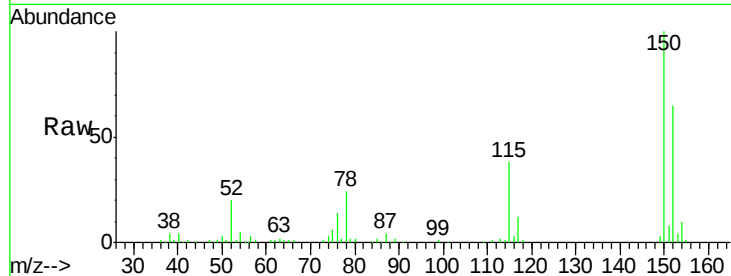


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

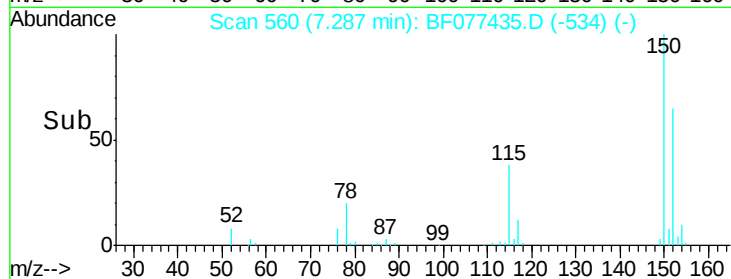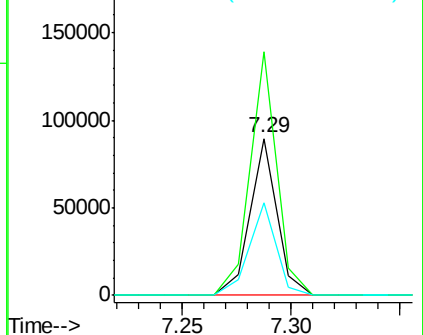



#5


2-Fluorophenol
 Concen: 50.85 ng
 RT: 5.58 min Scan# 411
 Delta R.T. -0.00 min
 Lab File: BF077435.D
 Acq: 25 Feb 2015 15:58

Tgt Ion:112 Resp: 235383
 Ion Ratio Lower Upper
 112 100
 64 47.3 48.5 72.7#
 63 24.2 25.0 37.4#

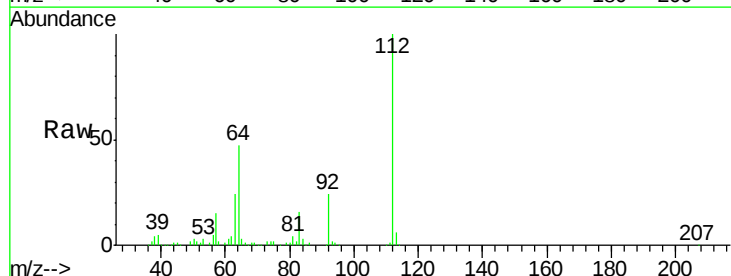

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0

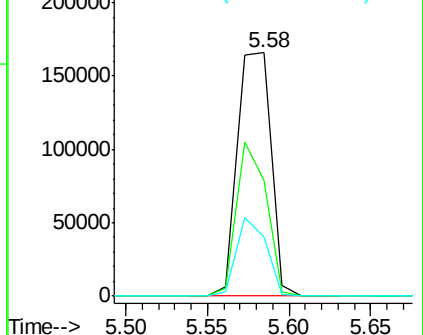



#7

Phenol-d6

Concen: 32.83 ng

RT: 6.84 min Scan# 521

Delta R.T. -0.00 min

Lab File: BF077435.D

Acq: 25 Feb 2015 15:58

Instrument :

BNA_F

ClientSampleId :

FB


Tgt Ion: 99 Resp: 195380

Ion Ratio Lower Upper




99 100

42 14.1 16.2 24.4#

71 28.5 26.7 40.1

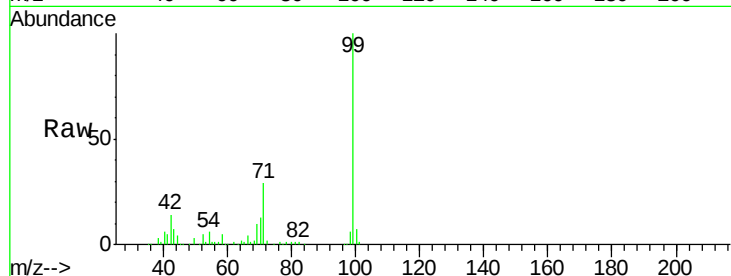

Abundance Ion 99.00 (98.70 to 99.70): BF0
Ion 42.00 (41.70 to 42.70): BF0
Ion 71.00 (70.70 to 71.70): BF0

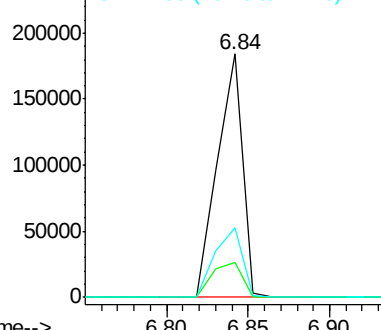

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.86 min Scan# 698

Delta R.T. -0.00 min

Lab File: BF077435.D

Acq: 25 Feb 2015 15:58

Tgt Ion: 136 Resp: 306200


Ion Ratio Lower Upper

136 100



137 10.8 8.6 13.0


54 6.6 6.2 9.4

68 5.2 5.0 7.6



Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0

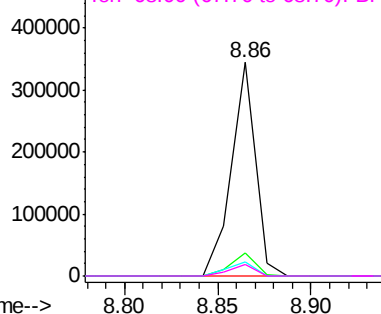



#23

Nitrobenzene-d5

Concen: 97.63 ng

RT: 7.97 min Scan# 620

Delta R.T. -0.01 min

Lab File: BF077435.D

Acq: 25 Feb 2015 15:58

Instrument :

BNA_F

ClientSampleId :

FB


Tgt Ion: 82 Resp: 480736

Ion Ratio Lower Upper

82 100

128 41.2 43.8 65.8#




54 52.5 36.7 55.1

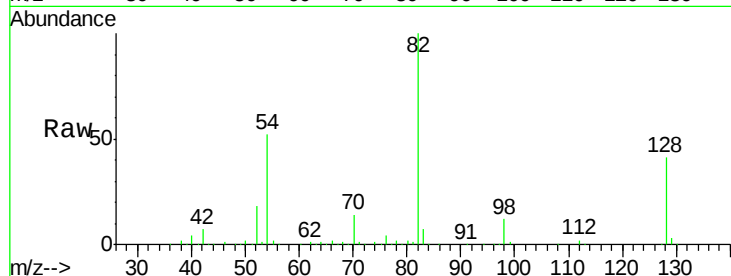

Abundance Ion 82.00 (81.70 to 82.70): BF077379.D (-621) (-)

Ion 128.00 (127.70 to 128.70): BF077379.D (-621) (-)

Ion 54.00 (53.70 to 54.70): BF077379.D (-621) (-)

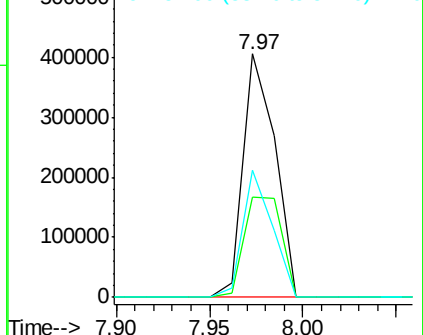

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 11.04 min Scan# 888

Delta R.T. -0.00 min

Lab File: BF077435.D

Acq: 25 Feb 2015 15:58


Tgt Ion: 164 Resp: 156540

Ion Ratio Lower Upper

164 100

162 104.8 83.2 124.8



160 46.6 34.6 52.0




Abundance Ion 164.00 (163.70 to 164.70): BF077379.D (-889) (-)

Ion 162.00 (161.70 to 162.70): BF077379.D (-889) (-)

Ion 160.00 (159.70 to 160.70): BF077379.D (-889) (-)

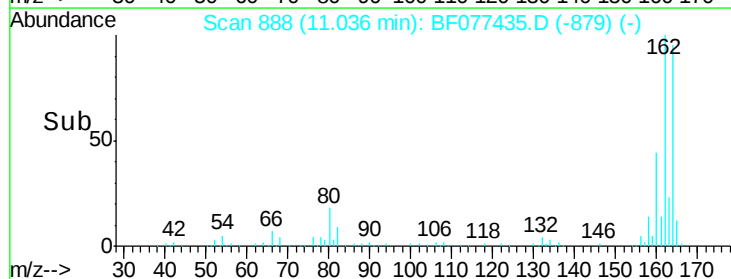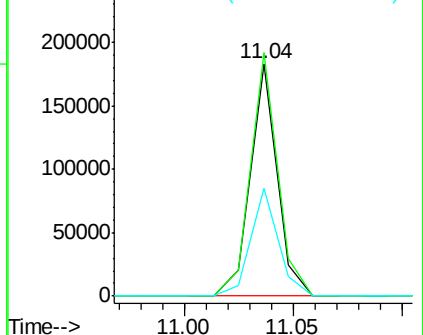


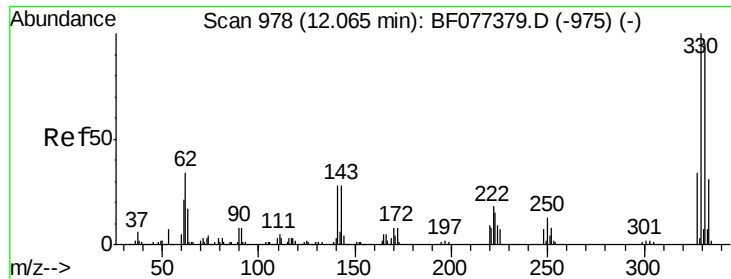




#41
 2,4,6-Tribromophenol
 Concen: 106.06 ng
 RT: 12.02 min Scan# 974
 Delta R.T. -0.00 min
 Lab File: BF077435.D
 Acq: 25 Feb 2015 15:58

Instrument :
 BNA_F
 ClientSampleId :
 FB

Tgt Ion:330 Resp: 159855
 Ion Ratio Lower Upper
 330 100
 332 96.3 77.4 116.2
 141 34.4 28.8 43.2




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


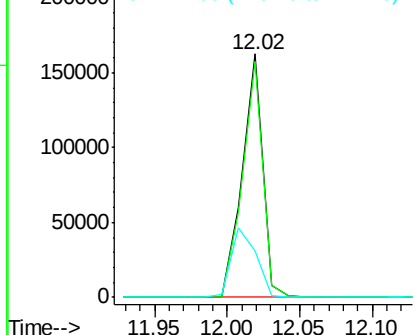



#44
 2-Fluorobiphenyl
 Concen: 108.04 ng
 RT: 10.21 min Scan# 816
 Delta R.T. -0.00 min
 Lab File: BF077435.D
 Acq: 25 Feb 2015 15:58

Tgt Ion:172 Resp: 1084626
 Ion Ratio Lower Upper
 172 100
 171 36.0 28.9 43.3
 170 24.0 19.4 29.2



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

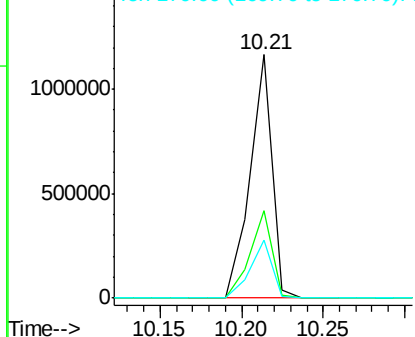







#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 12.88 min Scan# 1049
Delta R.T. -0.01 min
Lab File: BF077435.D
Acq: 25 Feb 2015 15:58

Instrument :
BNA_F
ClientSampleId :
FB

Tgt Ion:188 Resp: 301352
Ion Ratio Lower Upper
188 100
94 10.5 7.4 11.2
80 11.5 8.0 12.0

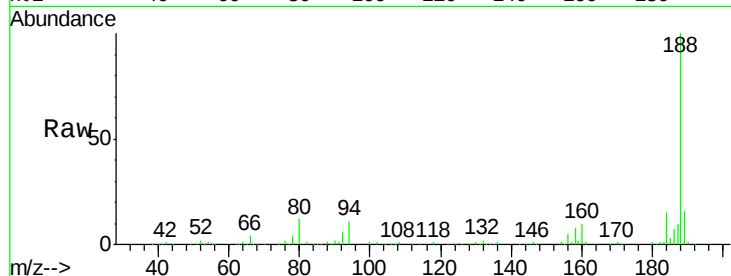


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0


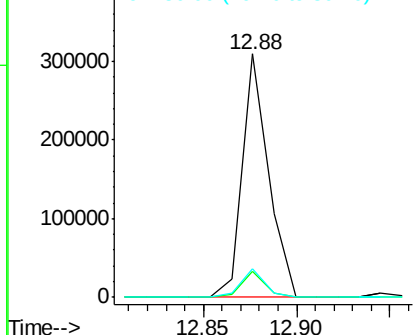



#75
Chrysene-d12
Concen: 20.00 ng
RT: 16.17 min Scan# 1337
Delta R.T. -0.01 min
Lab File: BF077435.D
Acq: 25 Feb 2015 15:58

Tgt Ion:240 Resp: 328062
Ion Ratio Lower Upper
240 100
120 12.3 8.8 13.2
236 25.2 20.7 31.1



Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E




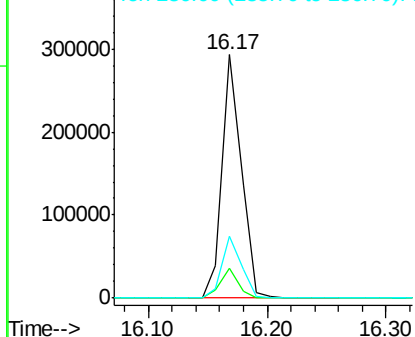


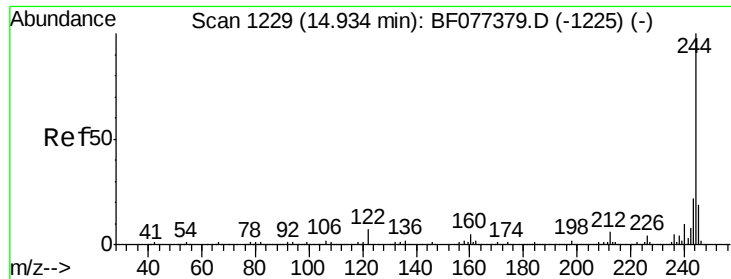

#78
 Terphenyl-d14
 Concen: 87.97 ng
 RT: 14.88 min Scan# 1224
 Delta R.T. -0.00 min
 Lab File: BF077435.D
 Acq: 25 Feb 2015 15:58

Instrument :
 BNA_F
 ClientSampleId :
 FB

Tgt Ion:244 Resp: 1234556
 Ion Ratio Lower Upper
 244 100
 212 7.0 5.2 7.8
 122 11.9 7.8 11.8#

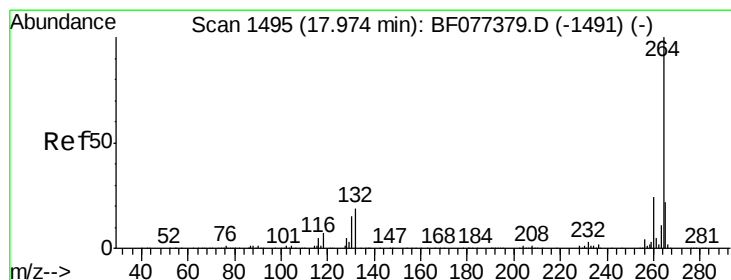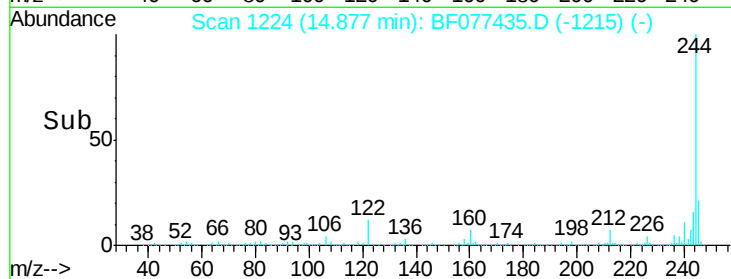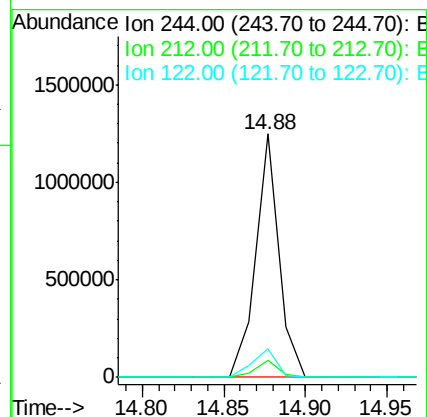

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 17.94 min Scan# 1492
 Delta R.T. 0.02 min
 Lab File: BF077435.D
 Acq: 25 Feb 2015 15:58

Tgt Ion:264 Resp: 334337
 Ion Ratio Lower Upper
 264 100
 260 22.4 19.3 28.9
 265 20.6 16.8 25.2

