


Data Path : Z:\HPCHEM1\BNA_F\Data\BF022515\
 Data File : BF077449.D
 Acq On : 25 Feb 2015 23:35
 Operator : IZ / TP
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Feb 26 17:14:46 2015

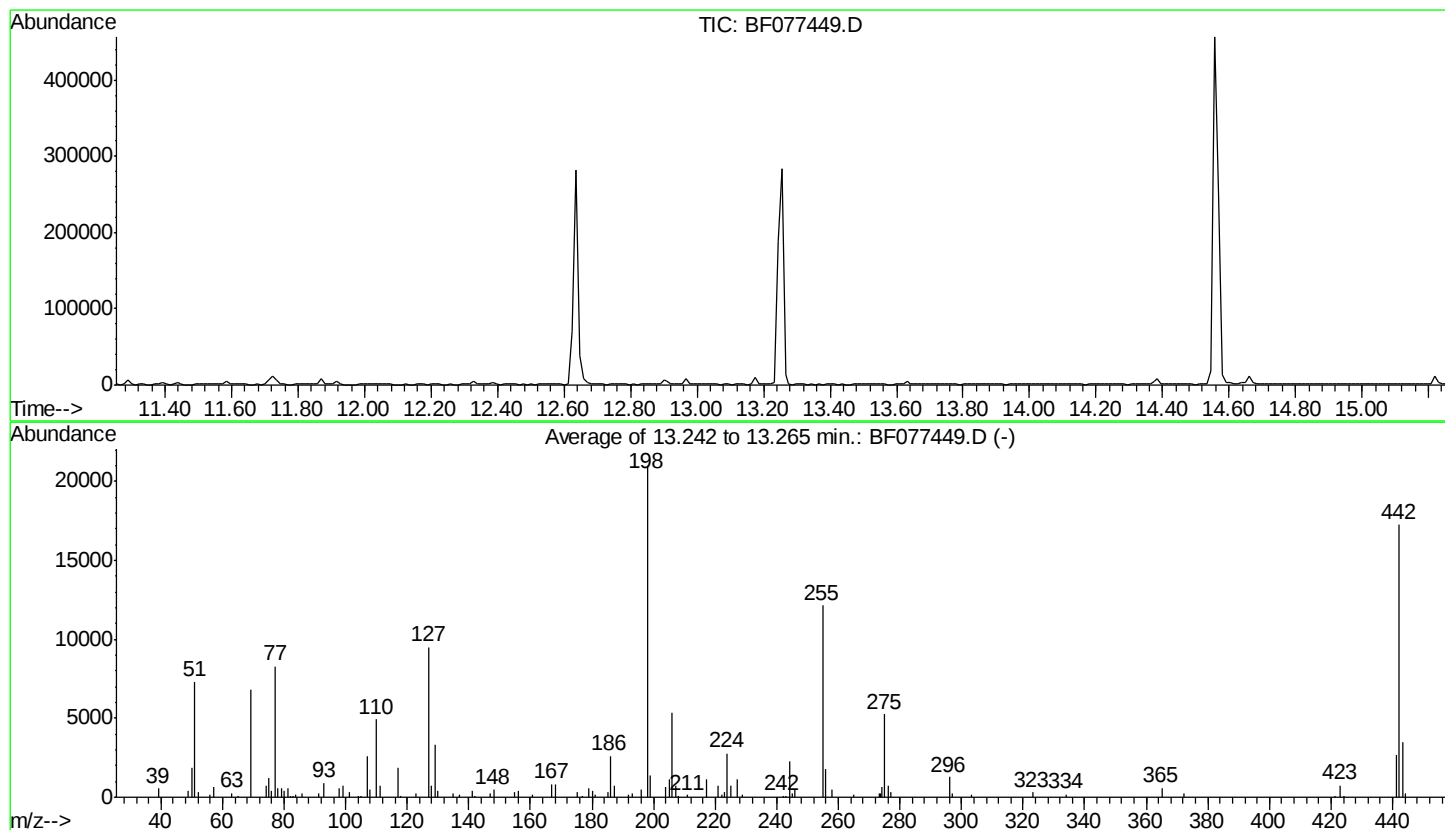

AutoFind: Scans 1081, 1082, 1083; Background Corrected with Scan 1077

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.7	7293	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.4	6792	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.2	9486	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	20991	PASS
199	198	5	9	6.6	1392	PASS
275	198	10	60	25.0	5248	PASS
365	198	1	100	2.8	597	PASS
441	442	0.01	24	15.3	2644	PASS
442	198	50	100	82.2	17255	PASS
443	442	15	24	20.0	3459	PASS