
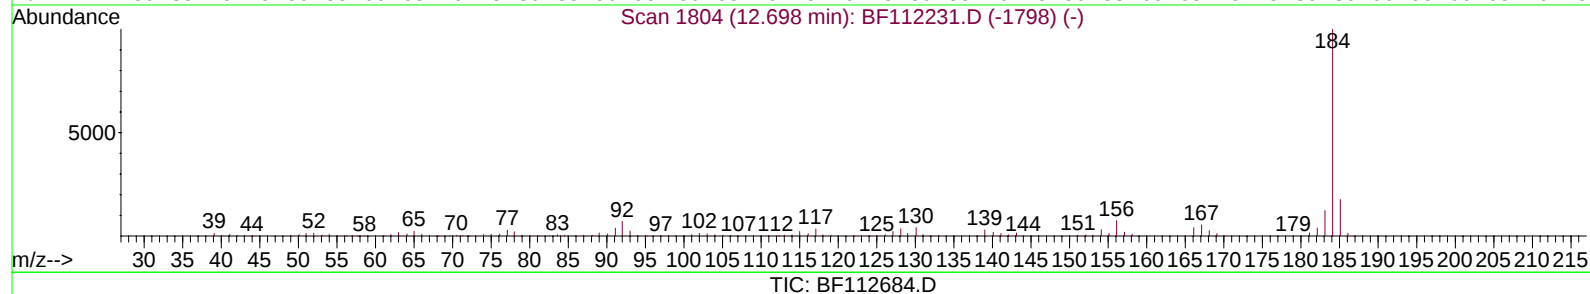
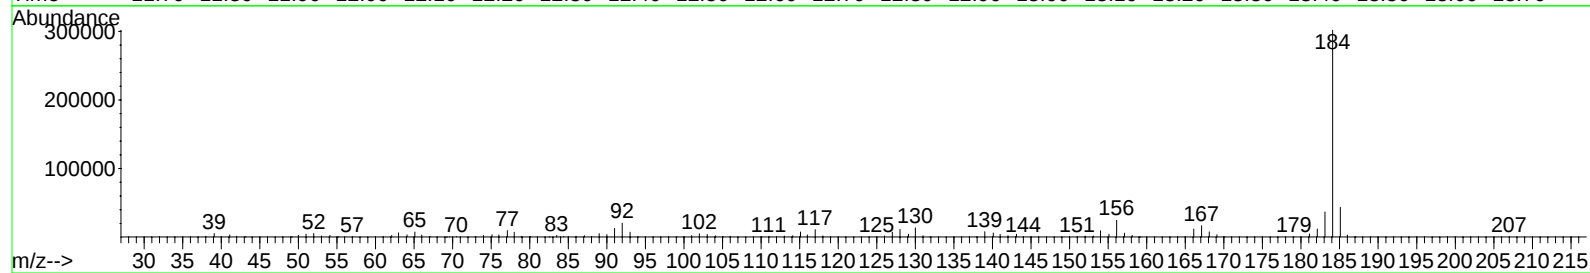


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF022519\
 Data File : BF112684.D
 Acq On : 25 Feb 2019 10:57
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 25 17:46:01 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 28 10:38:18 2019
 Response via : Initial Calibration

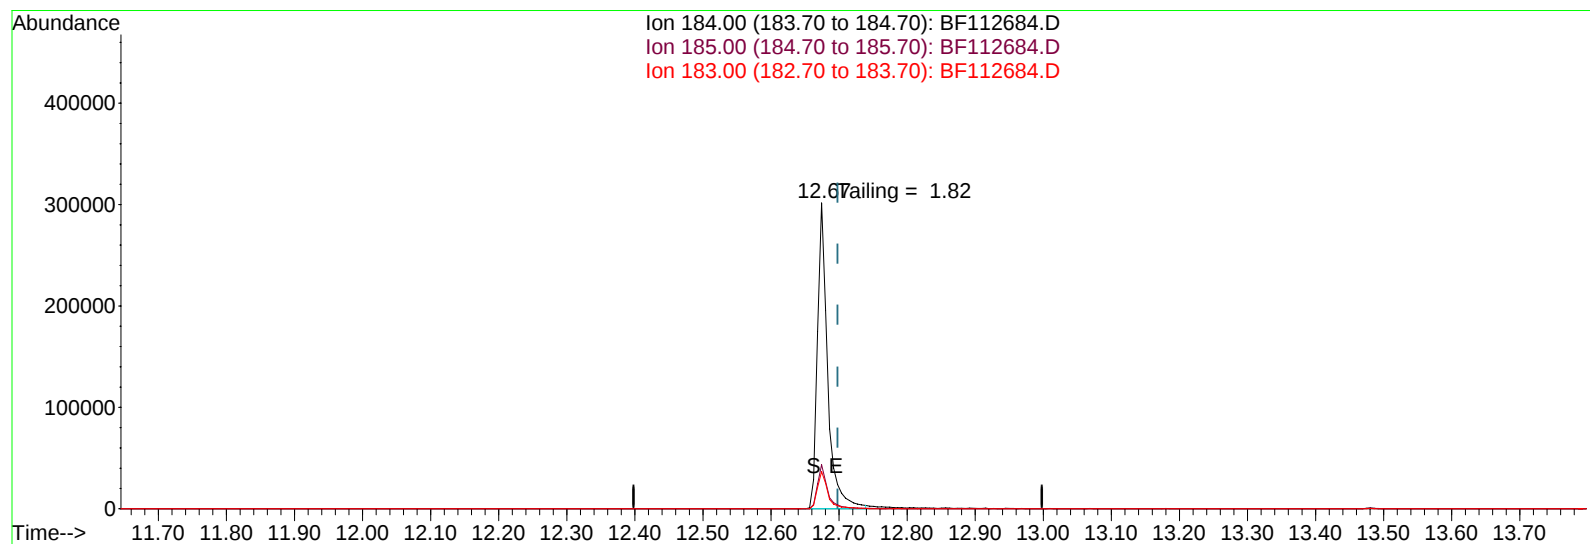

(77) Benzidine




12.674min (-0.024) 0.00ng

response 321632

Ion	Exp%	Act%
184.00	100	100
185.00	17.40	14.41
183.00	12.50	12.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF022519\
Data File : BF112684.D
Acq On : 25 Feb 2019 10:57
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 25 17:46:01 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 28 10:38:18 2019
Response via : Initial Calibration

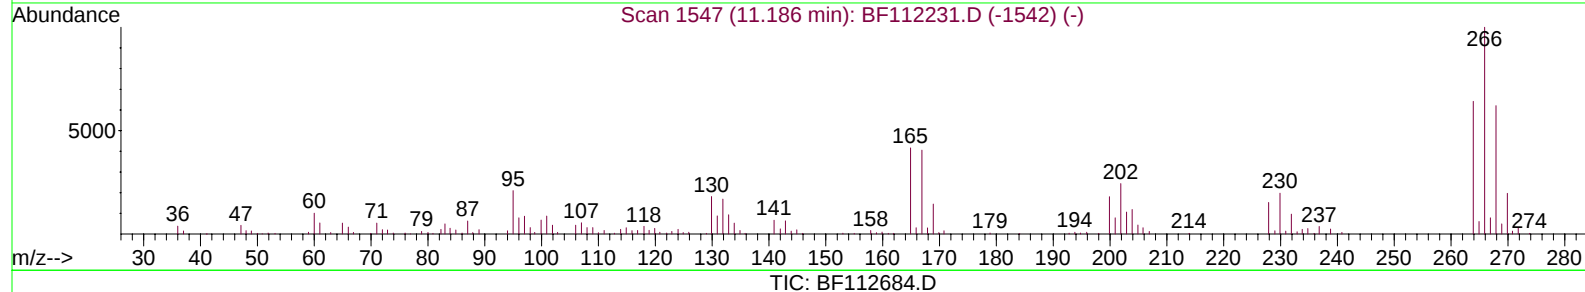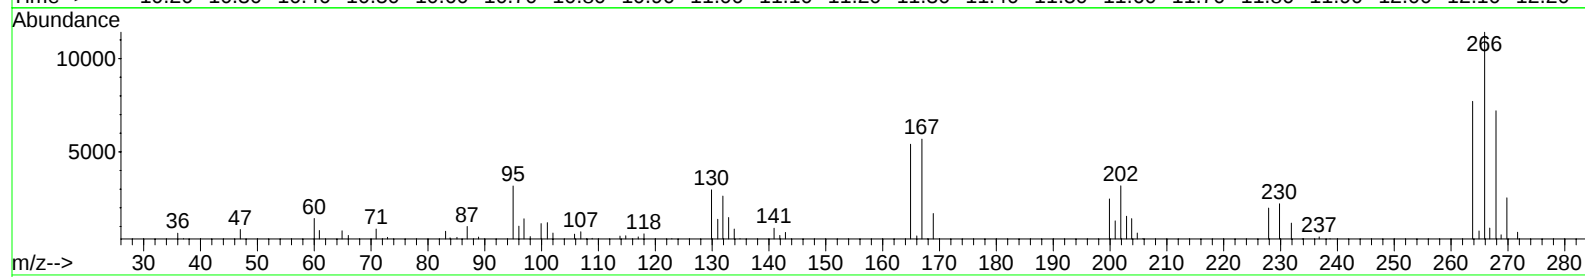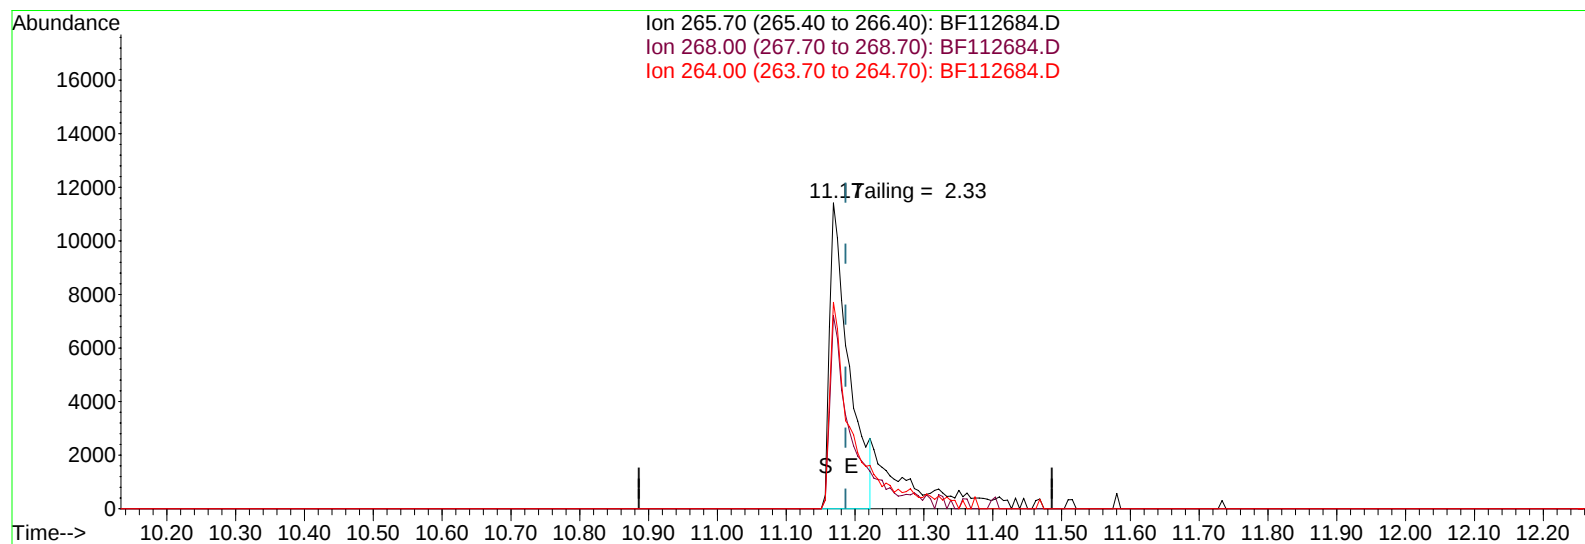

(70) Pentachlorophenol (C)

11.169min (-0.018) 44756.27ng

response 25711

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	63.10
264.00	63.60	67.52
0.00	0.00	0.00