

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF022519\
 Data File : BF112695.D
 Acq On : 25 Feb 2019 16:31
 Operator : JU/SJ
 Sample : K1596-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 COMP-14

Quant Time: Feb 26 00:13:56 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 28 10:38:18 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.82	152	70166	20.00	ng	-0.03
21) Naphthalene-d8	8.10	136	250164	20.00	ng	-0.03
39) Acenaphthene-d10	9.85	164	101299	20.00	ng	-0.04
64) Phenanthrene-d10	11.34	188	162577	20.00	ng	-0.03
76) Chrysene-d12	13.99	240	170624	20.00	ng	-0.02
87) Perylene-d12	15.46	264	164416	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.47	112	517514	156.66	ng	0.00
7) Phenol-d6	6.48	99	561024	122.22	ng	-0.01
23) Nitrobenzene-d5	7.38	82	440502	101.46	ng	-0.03
42) 2,4,6-Tribromophenol	10.65	330	159290	135.10	ng	-0.04
45) 2-Fluorobiphenyl	9.17	172	794602	110.94	ng	-0.04
79) Terphenyl-d14	12.92	244	705311	77.86	ng	-0.04


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF022519\
Data File : BF112695.D
Acq On : 25 Feb 2019 16:31
Operator : JU/SJ
Sample : K1596-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP-14

Quant Time: Feb 26 00:13:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 28 10:38:18 2019
Response via : Initial Calibration

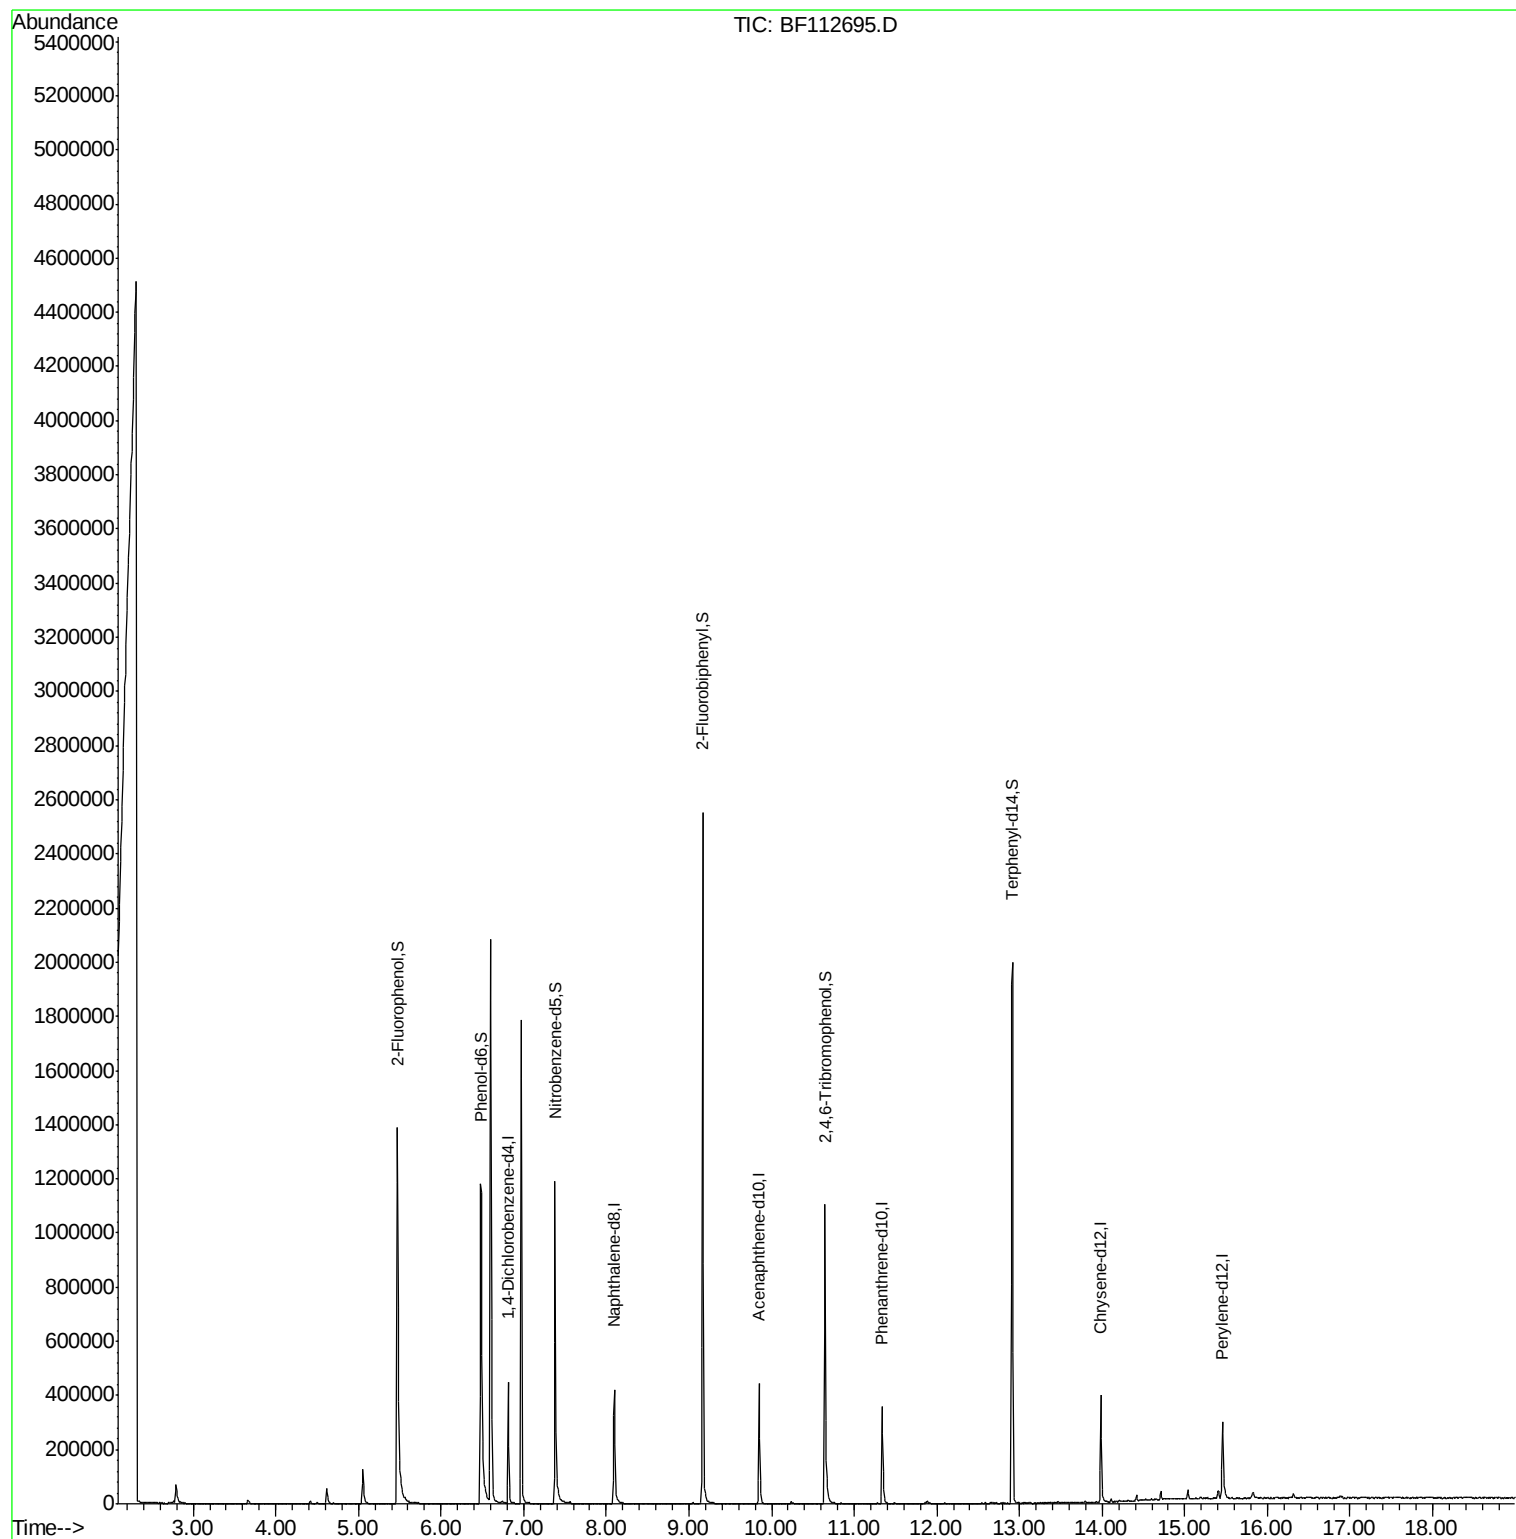

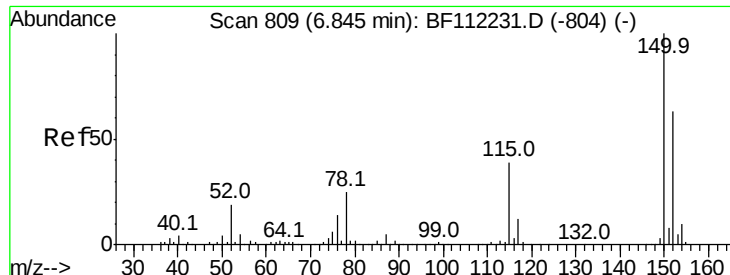


#1



1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.82 min Scan# 804
 Delta R.T. -0.03 min
 Lab File: BF112695.D
 Acq: 25 Feb 2019 16:31

Instrument :
 BNA_F
 ClientSampleId :
 COMP-14

Tot Ion:152 Resp: 70166
 Ion Ratio Lower Upper
 152 100
 150 154.8 127.4 191.0
 115 60.2 45.5 68.3

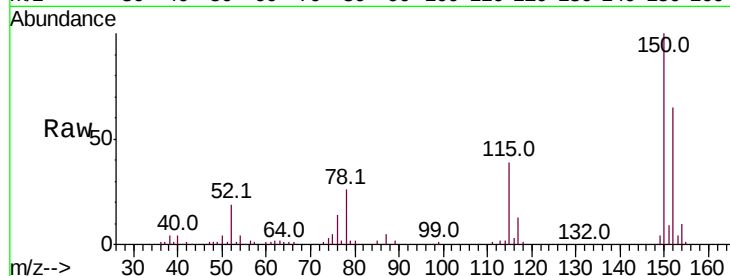


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

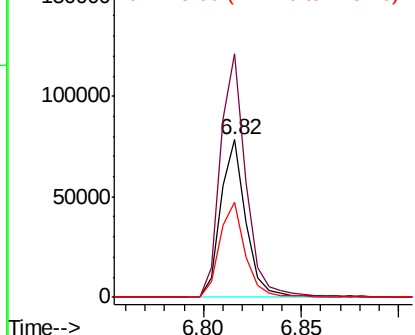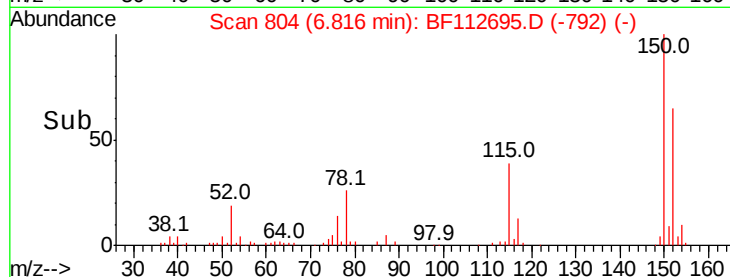



#5

2-Fluorophenol
 Concen: 156.662 ng
 RT: 5.47 min Scan# 576
 Delta R.T. -0.01 min
 Lab File: BF112695.D
 Acq: 25 Feb 2019 16:31

Tgt Ion:112 Resp: 517514
 Ion Ratio Lower Upper
 112 100
 64 54.2 45.7 68.5
 63 30.8 23.6 35.4

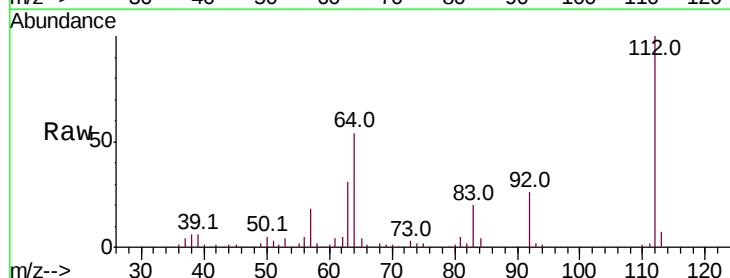

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF1
 Ion 63.00 (62.70 to 63.70): BF1

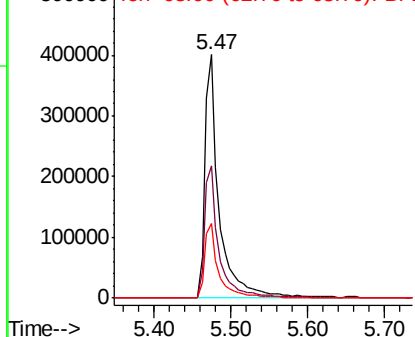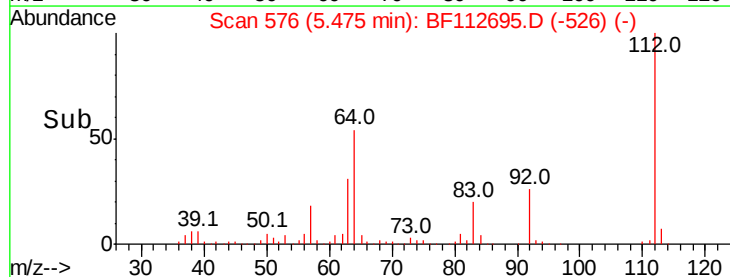



#7

Phenol-d6

Concen: 122.222 ng

RT: 6.48 min Scan# 747

Delta R.T. -0.01 min

Lab File: BF112695.D

Acq: 25 Feb 2019 16:31

Instrument :

BNA_F

ClientSampled :

COMP-14


Tot Ion: 99 Resp: 561024

Ion Ratio Lower Upper




99 100

42 20.4 15.1 22.7

71 39.6 26.9 40.3

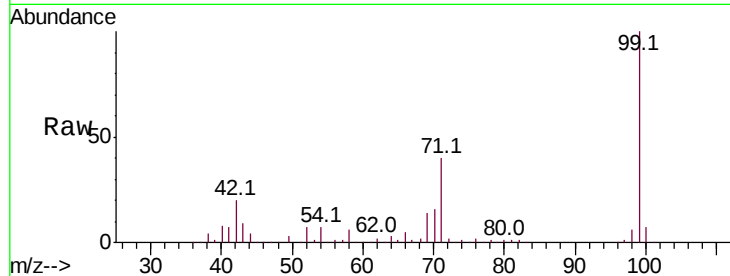

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

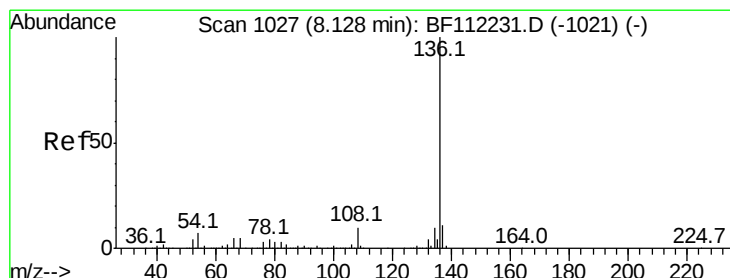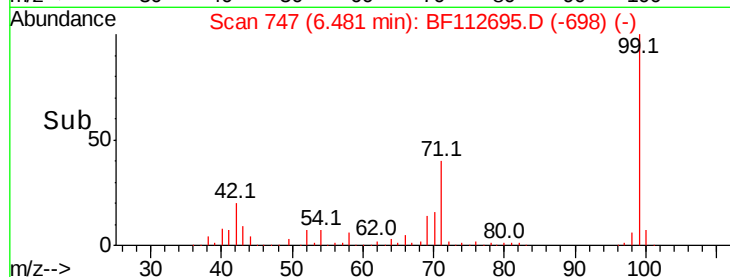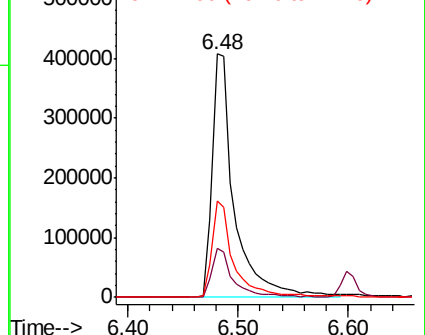

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.10 min Scan# 1022

Delta R.T. -0.03 min

Lab File: BF112695.D

Acq: 25 Feb 2019 16:31

Tgt Ion:136 Resp: 250164


Ion Ratio Lower Upper

136 100



137 10.9 9.1 13.7


54 6.2 5.9 8.9

68 4.2 5.1 7.7#

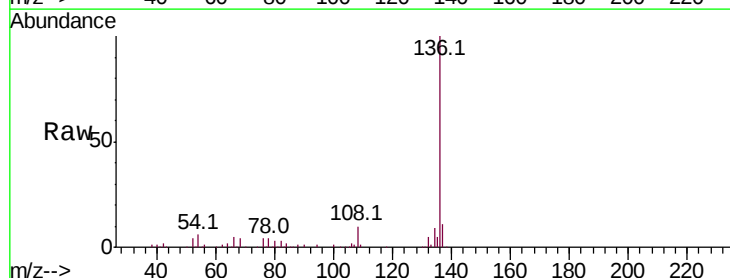

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

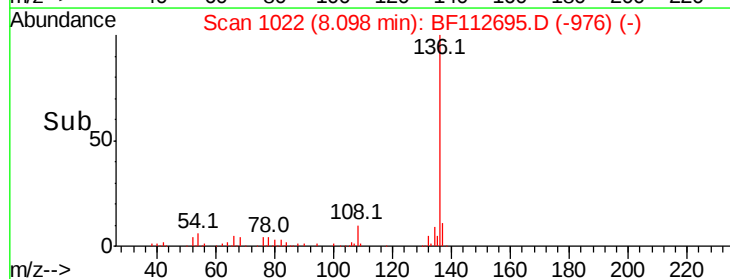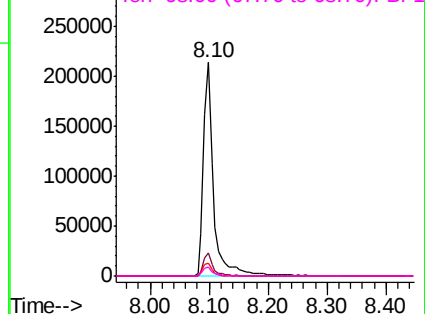


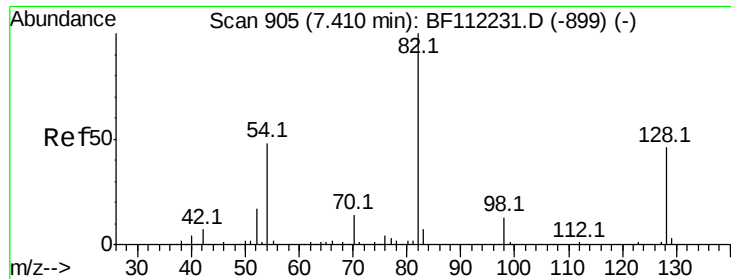




#23
Nitrobenzene-d5
Concen: 101.460 ng
RT: 7.38 min Scan# 900
Delta R.T. -0.03 min
Lab File: BF112695.D
Acq: 25 Feb 2019 16:31

Instrument :
BNA_F
ClientSampleId :
COMP-14

Tot Ion: 82 Resp: 440502
Ion Ratio Lower Upper
82 100
128 43.3 37.8 56.8
54 49.1 39.7 59.5

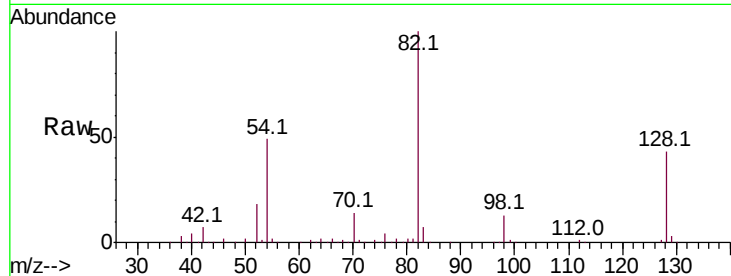


Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF1

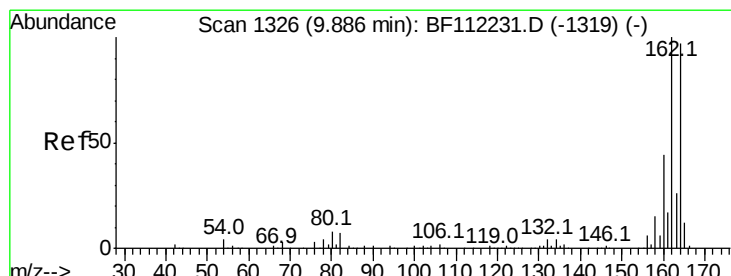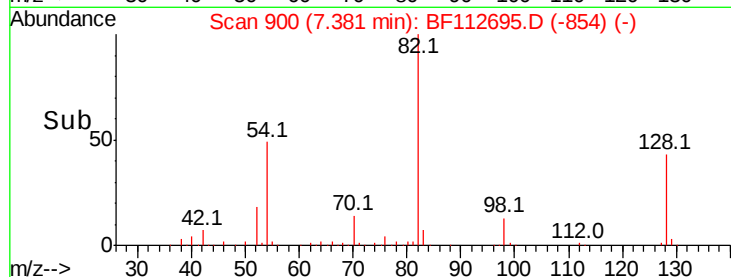
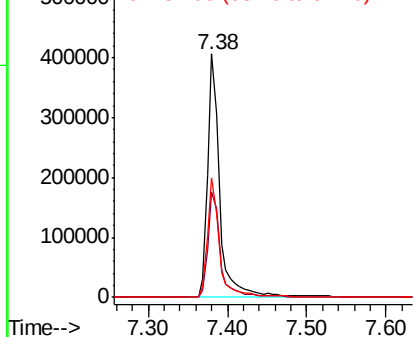


#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.85 min Scan# 1320
Delta R.T. -0.04 min
Lab File: BF112695.D
Acq: 25 Feb 2019 16:31

Tgt Ion:164 Resp: 101299
Ion Ratio Lower Upper
164 100
162 104.1 82.2 123.4
160 46.3 36.2 54.4

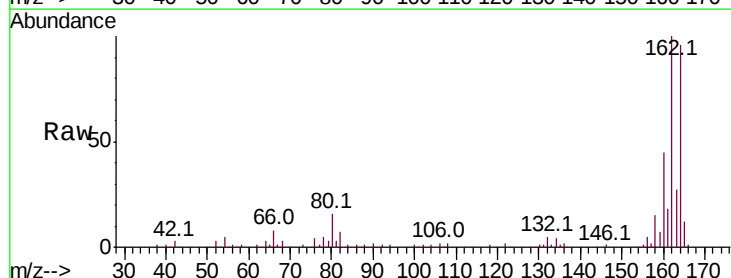

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

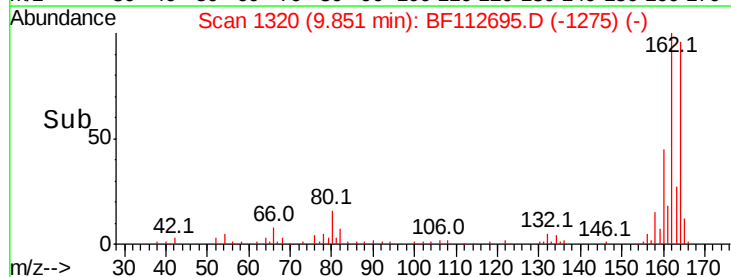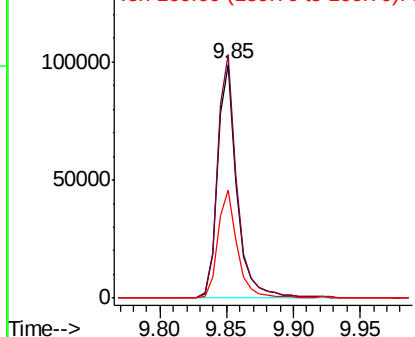







#42
 2,4,6-Tribromophenol
 Concen: 135.095 ng
 RT: 10.65 min Scan# 1455
 Delta R.T. -0.04 min
 Lab File: BF112695.D
 Acq: 25 Feb 2019 16:31

Instrument :
 BNA_F
 ClientSampleId :
 COMP-14

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.7	76.6	114.8
141	34.8	24.3	36.5

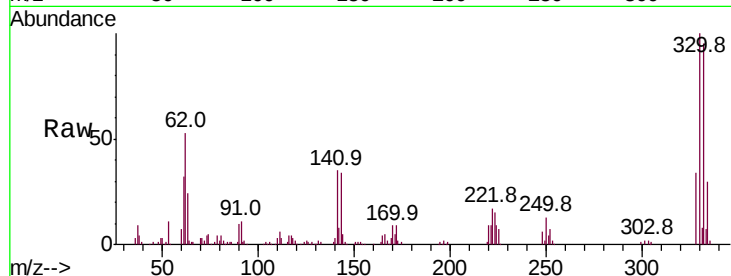


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

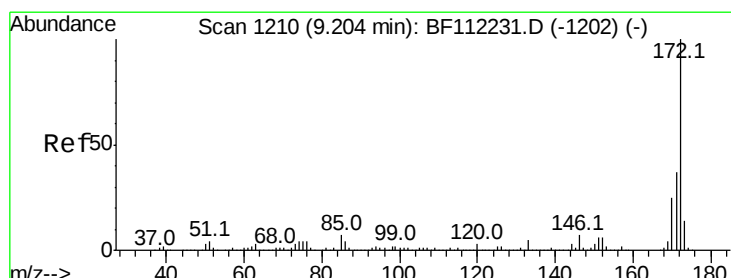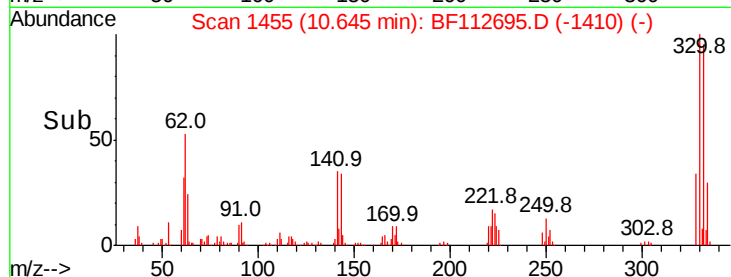
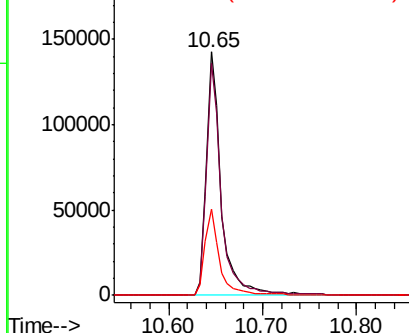


#45
 2-Fluorobiphenyl
 Concen: 110.942 ng
 RT: 9.17 min Scan# 1204
 Delta R.T. -0.04 min
 Lab File: BF112695.D
 Acq: 25 Feb 2019 16:31

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.6	30.5	45.7
170	23.6	20.2	30.4

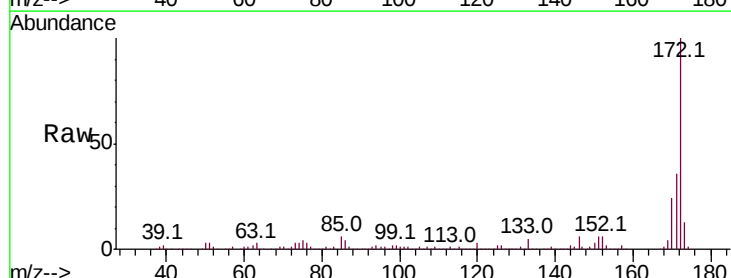

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



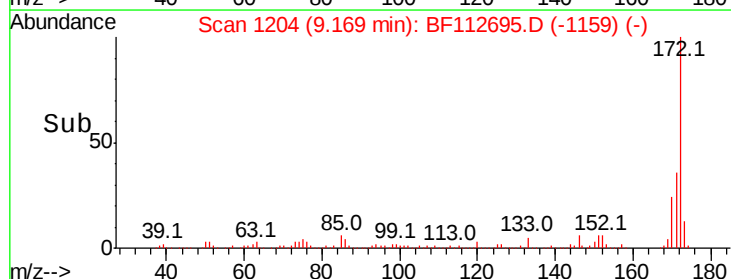
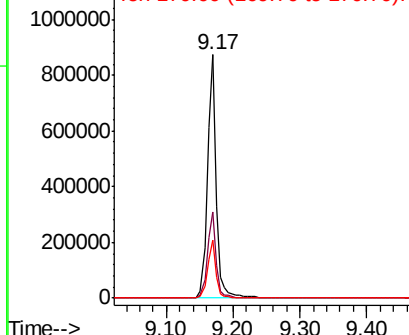




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.34 min Scan# 1573
Delta R.T. -0.03 min
Lab File: BF112695.D
Acq: 25 Feb 2019 16:31




Instrument :
BNA_F
ClientSampleId :
COMP-14


Tot Ion:188 Resp: 162577
Ion Ratio Lower Upper
188 100
94 8.1 8.2 12.2#
80 8.6 8.9 13.3#

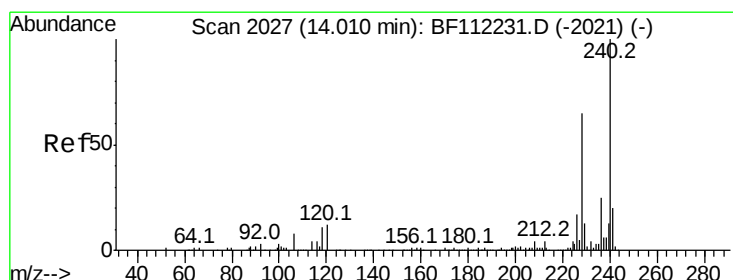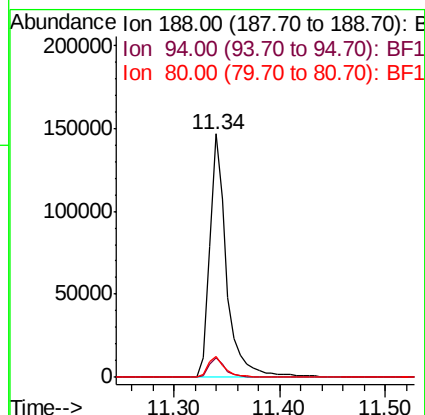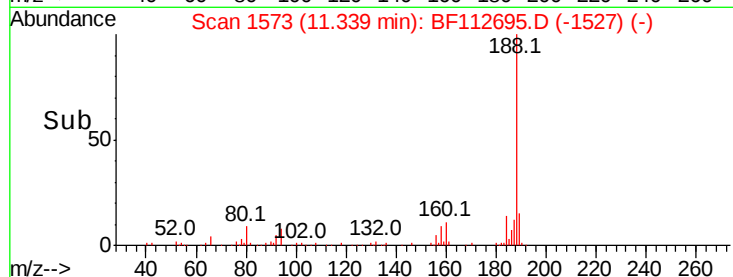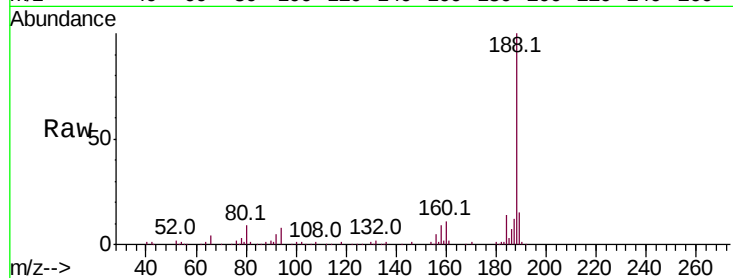

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.99 min Scan# 2023
Delta R.T. -0.02 min
Lab File: BF112695.D
Acq: 25 Feb 2019 16:31

Tgt Ion:240 Resp: 170624
Ion Ratio Lower Upper
240 100
120 9.9 9.0 13.6
236 25.5 20.7 31.1

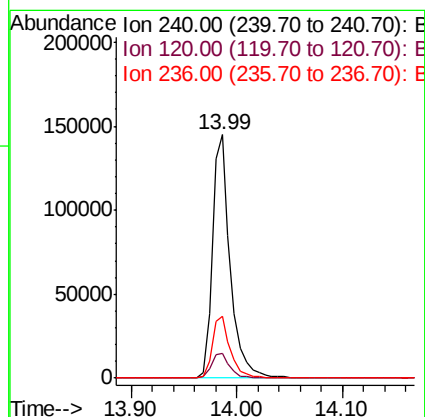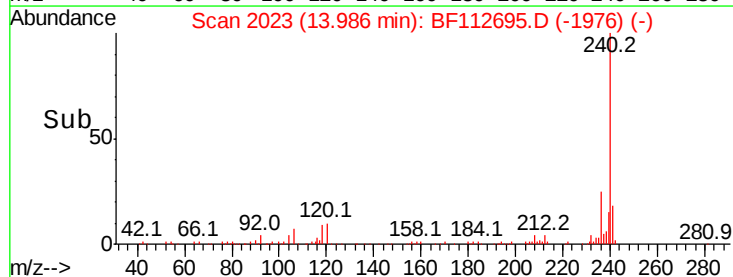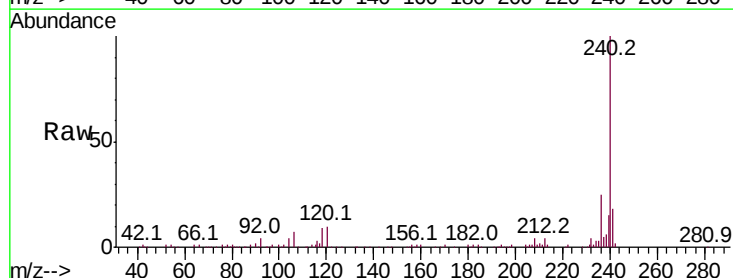


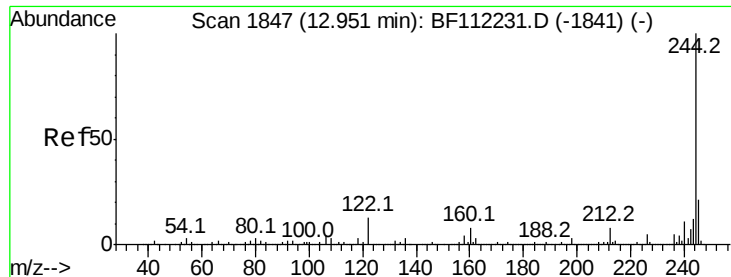




#79
 Terphenyl-d14
 Concen: 77.856 ng
 RT: 12.92 min Scan# 1841
 Delta R.T. -0.04 min
 Lab File: BF112695.D
 Acq: 25 Feb 2019 16:31

Instrument :
 BNA_F
 ClientSampleId :
 COMP-14

Tot Ion:244 Resp: 705311
 Ion Ratio Lower Upper
 244 100
 212 7.0 5.9 8.9
 122 10.5 9.8 14.6

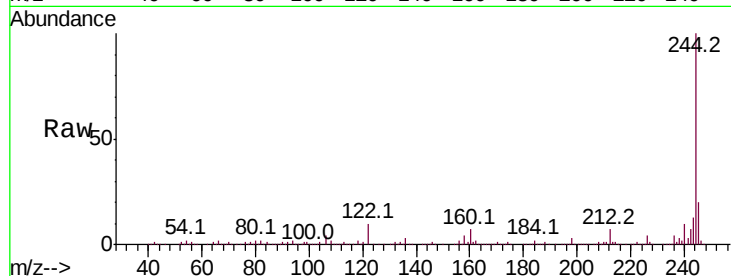


Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

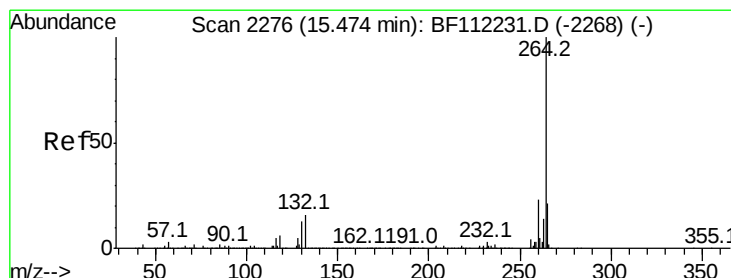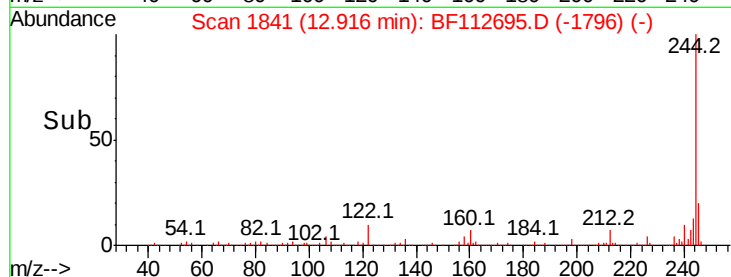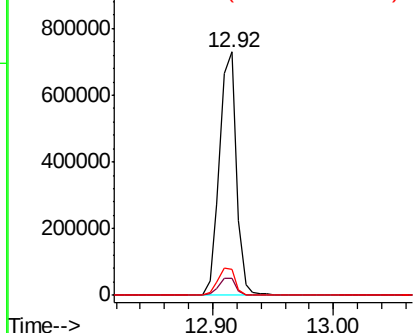

#87
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.46 min Scan# 2273
 Delta R.T. -0.02 min
 Lab File: BF112695.D
 Acq: 25 Feb 2019 16:31

Tgt Ion:264 Resp: 164416
 Ion Ratio Lower Upper
 264 100
 260 23.3 18.2 27.2
 265 21.1 17.0 25.4

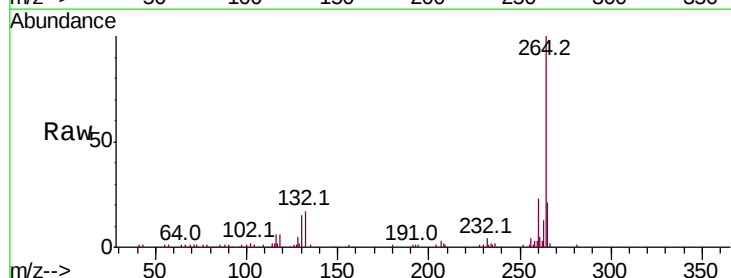

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

