

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF022519\
 Data File : BF112700.D
 Acq On : 25 Feb 2019 18:46
 Operator : JU/SJ
 Sample : K1596-02 5X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 COMP-14

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012519.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.475	573	576	594	rBV	92054	193704	33.91%	4.406%
2	6.498	747	750	765	rBV	92124	216699	37.94%	4.929%
3	6.604	765	768	784	rVB	189810	273051	47.80%	6.211%
4	6.816	801	804	815	rBV	358376	343595	60.15%	7.815%
5	6.969	827	830	844	rBV	186166	198822	34.81%	4.522%
6	7.392	899	902	917	rBV	66037	128895	22.56%	2.932%
7	8.098	1018	1022	1050	rBV	319171	415395	72.72%	9.448%
8	9.169	1201	1204	1215	rBV	169619	210146	36.79%	4.780%
9	9.574	1269	1273	1282	rBB	8293	9163	1.60%	0.208%
10	9.851	1316	1320	1337	rBV	362205	399647	69.96%	9.090%
11	10.657	1454	1457	1466	rBV	79475	111449	19.51%	2.535%
12	11.339	1569	1573	1583	rBV	331882	395315	69.21%	8.992%
13	11.957	1676	1678	1686	rVB5	4206	7162	1.25%	0.163%
14	12.398	1750	1753	1758	rBV7	4087	6986	1.22%	0.159%
15	12.563	1776	1781	1786	rBV	37791	42825	7.50%	0.974%
16	12.792	1814	1820	1825	rBV	40860	53293	9.33%	1.212%
17	12.839	1825	1828	1831	rVB5	4227	6566	1.15%	0.149%
18	12.910	1837	1840	1848	rBV	233692	221361	38.75%	5.035%
19	13.227	1890	1894	1897	rBV6	5686	8427	1.48%	0.192%
20	13.692	1969	1973	1975	rBV5	9178	9956	1.74%	0.226%
21	13.751	1979	1983	1988	rBV8	11815	23524	4.12%	0.535%
22	13.792	1988	1990	1993	rBV4	10568	15122	2.65%	0.344%
23	13.898	2006	2008	2011	rBV4	7885	8674	1.52%	0.197%
24	13.927	2011	2013	2016	rVV3	9050	8492	1.49%	0.193%
25	13.980	2018	2022	2031	rVV	452874	571219	100.00%	12.993%
26	14.409	2093	2095	2098	rBV4	19083	14520	2.54%	0.330%
27	14.709	2144	2146	2150	rBV4	19621	19351	3.39%	0.440%
28	15.039	2199	2202	2211	rVB2	57199	93921	16.44%	2.136%
29	15.456	2268	2273	2283	rVB	252489	380485	66.61%	8.654%
30	17.139	2557	2559	2560	rBV2	11929	8666	1.52%	0.197%


Sum of corrected areas: 4396431

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF022519\
Data File : BF112700.D
Acq On : 25 Feb 2019 18:46
Operator : JU/SJ
Sample : K1596-02 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampled :
COMP-14

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

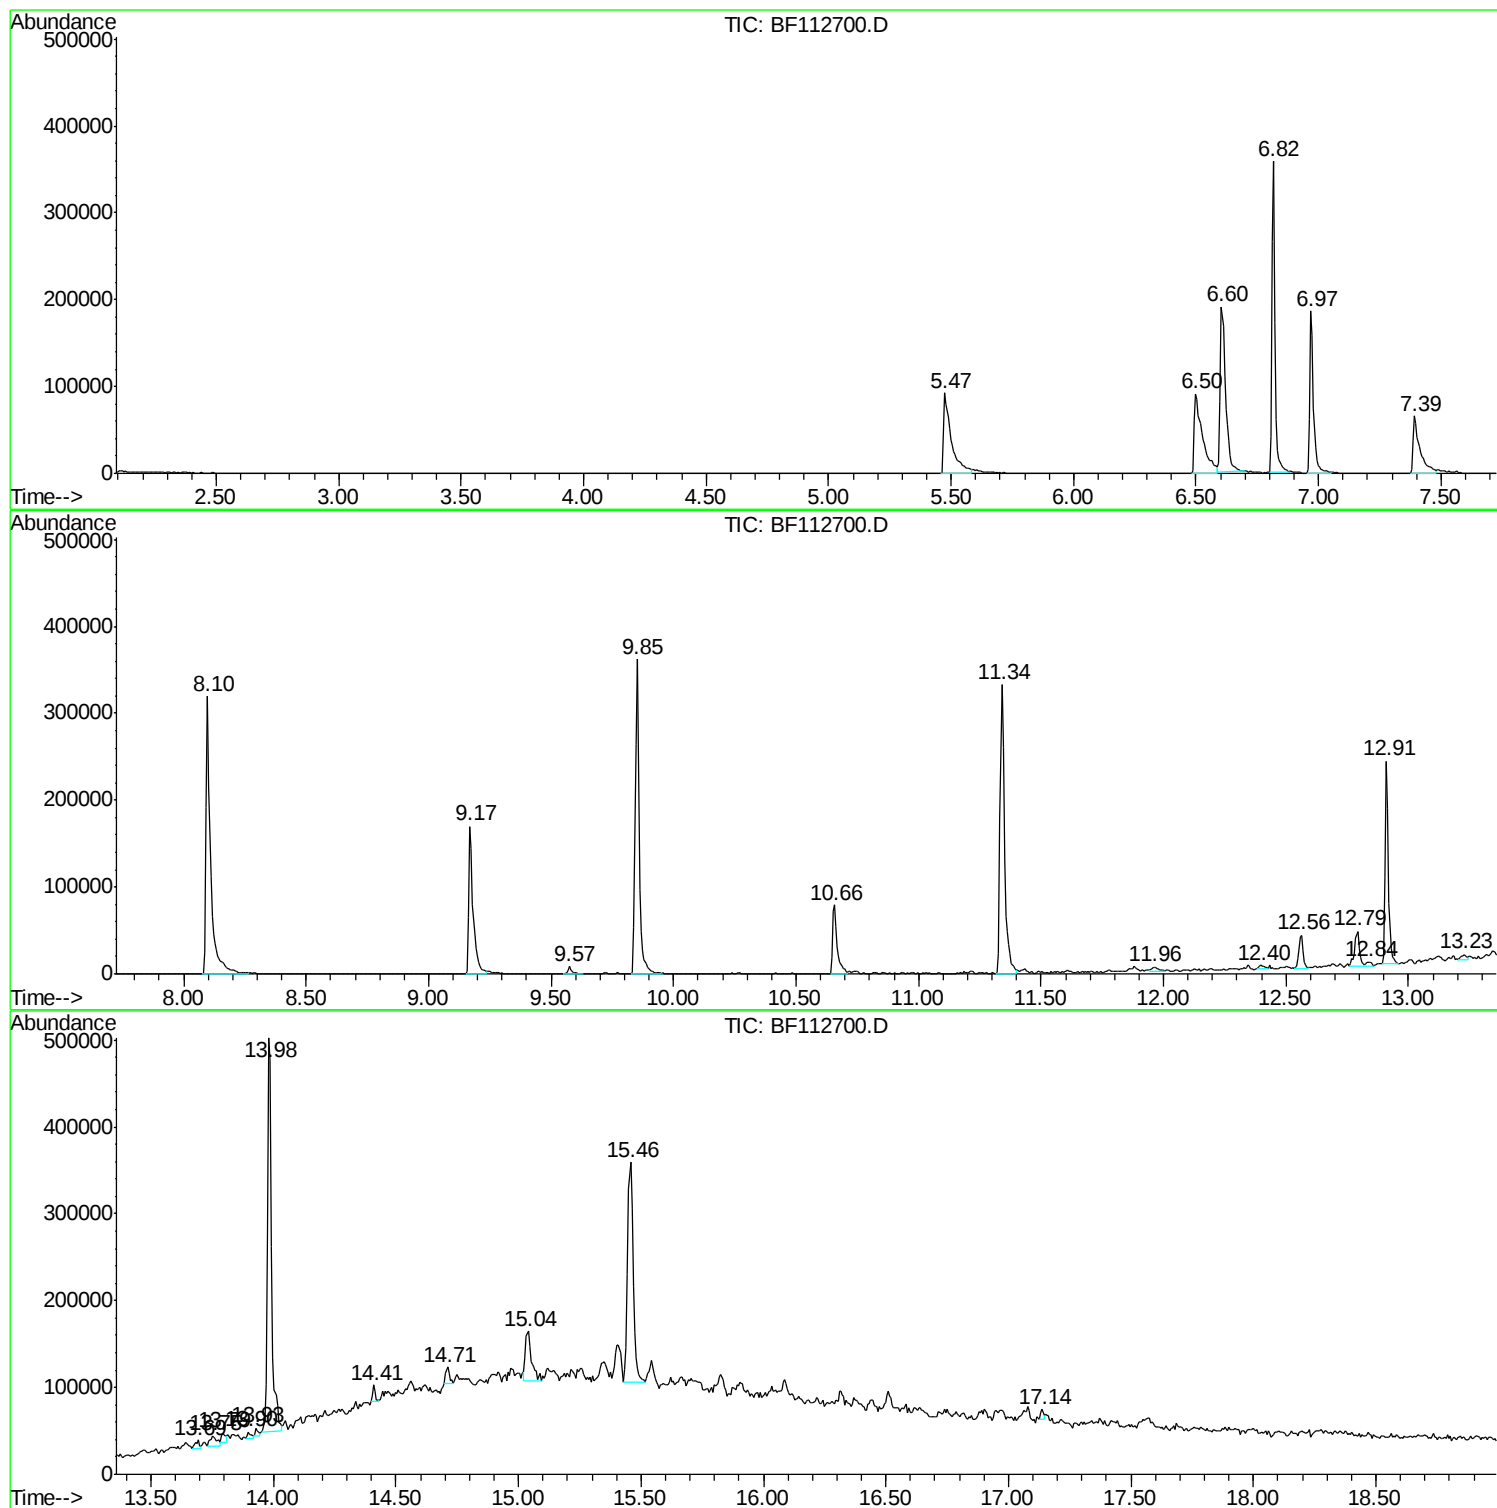

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF022519\
Data File : BF112700.D
Acq On : 25 Feb 2019 18:46
Operator : JU/SJ
Sample : K1596-02 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP-14










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.60 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.60	15.89 ng	273051	1,4-Dichlorobenzene-d4	6.82

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	5-Aminoindole	132	C8H8N2	005192-03-0	22
2		N-(-3,4-Methylenedioxyphenylisopropyl)benzaldimine	267	C17H17NO2	1000378-96-6	10
3		Bicyclo[4.2.0]octa-1,3,5-triene, 2,4-dimethyl-	132	C10H12	028749-81-7	9
4		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9
5		Xenon	132	Xe	007440-63-3	9

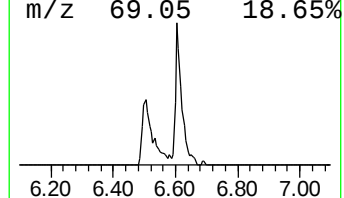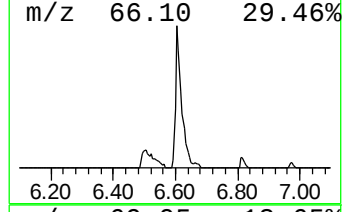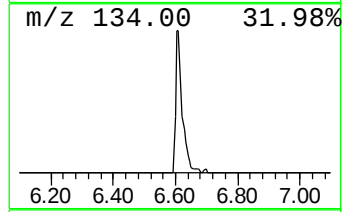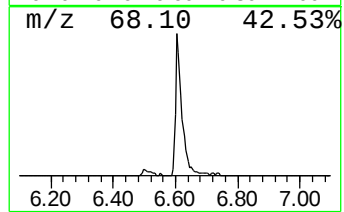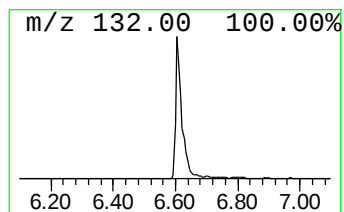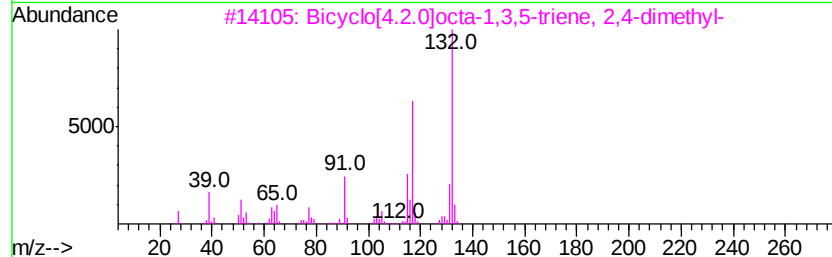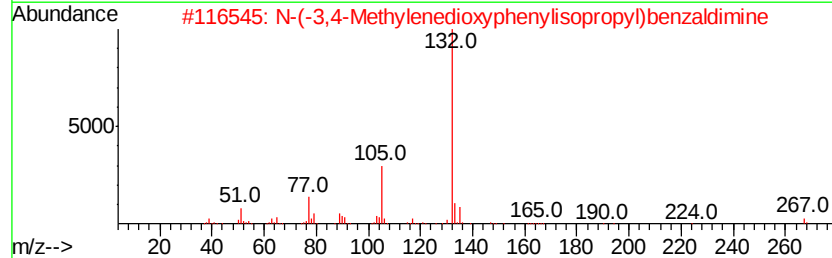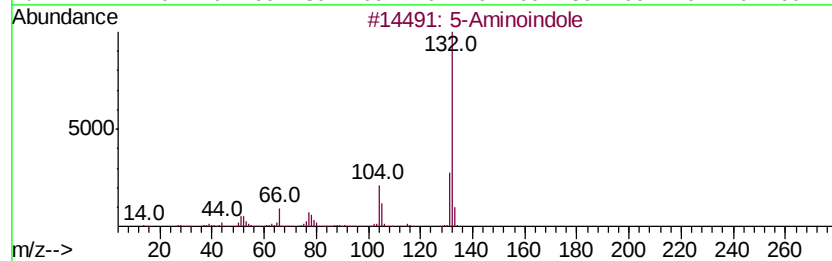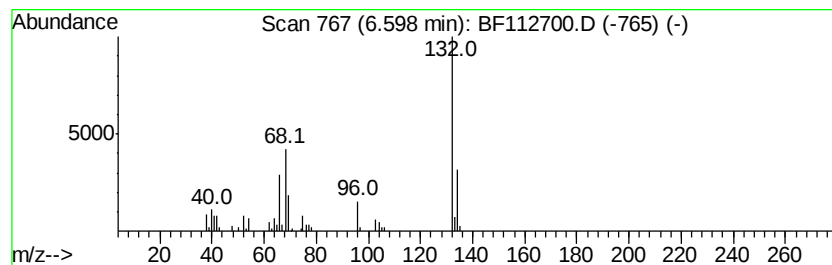

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF022519\
Data File : BF112700.D
Acq On : 25 Feb 2019 18:46
Operator : JU/SJ
Sample : K1596-02 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP-14

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.60	6.60	15.9	ng	273051	1	6.82	343595	20.0