

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF022519\
 Data File : BF112701.D
 Acq On : 25 Feb 2019 19:13
 Operator : JU/SJ
 Sample : K1596-03 5X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 COMP-15

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.475	573	576	594	rBV	83726	185604	31.79%	4.133%
2	6.498	747	750	765	rBV	88170	210095	35.98%	4.679%
3	6.604	765	768	779	rVB	180528	250852	42.96%	5.586%
4	6.816	800	804	817	rBV	338449	350084	59.96%	7.796%
5	6.969	827	830	841	rBV	191346	192261	32.93%	4.282%
6	7.393	899	902	914	rBV	65719	117480	20.12%	2.616%
7	8.098	1018	1022	1040	rBV	351212	427201	73.17%	9.514%
8	9.169	1201	1204	1215	rBV	187183	212364	36.37%	4.729%
9	9.575	1266	1273	1282	rBB2	8159	10291	1.76%	0.229%
10	9.851	1316	1320	1339	rVB	399170	437192	74.88%	9.736%
11	10.651	1453	1456	1468	rBV	92017	125088	21.42%	2.786%
12	11.339	1569	1573	1582	rBV	394305	441032	75.53%	9.822%
13	11.863	1657	1662	1664	rBV4	5356	8851	1.52%	0.197%
14	11.880	1664	1665	1671	rVB4	6625	6156	1.05%	0.137%
15	11.963	1676	1679	1682	rBV2	4810	7096	1.22%	0.158%
16	12.392	1750	1752	1755	rBV4	5866	6475	1.11%	0.144%
17	12.557	1777	1780	1787	rBV	37708	42288	7.24%	0.942%
18	12.792	1814	1820	1826	rBV	38066	47009	8.05%	1.047%
19	12.910	1837	1840	1847	rBV	263947	236547	40.51%	5.268%
20	13.016	1853	1858	1861	rBV6	4527	7245	1.24%	0.161%
21	13.322	1906	1910	1912	rBV4	4384	6064	1.04%	0.135%
22	13.351	1912	1915	1917	rVV3	9629	9635	1.65%	0.215%
23	13.433	1926	1929	1931	rVB3	7355	8225	1.41%	0.183%
24	13.686	1970	1972	1974	rBV3	6816	7449	1.28%	0.166%
25	13.927	2011	2013	2017	rBV5	9671	11644	1.99%	0.259%
26	13.980	2018	2022	2033	rVV	500015	583878	100.00%	13.003%
27	15.039	2198	2202	2209	rVB2	47235	78757	13.49%	1.754%
28	15.410	2262	2265	2269	rVB5	35561	42785	7.33%	0.953%
29	15.457	2269	2273	2281	rVB	266921	380148	65.11%	8.466%
30	16.315	2415	2419	2427	rVB	19263	40632	6.96%	0.905%


Sum of corrected areas: 4490428

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF022519\
Data File : BF112701.D
Acq On : 25 Feb 2019 19:13
Operator : JU/SJ
Sample : K1596-03 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP-15

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

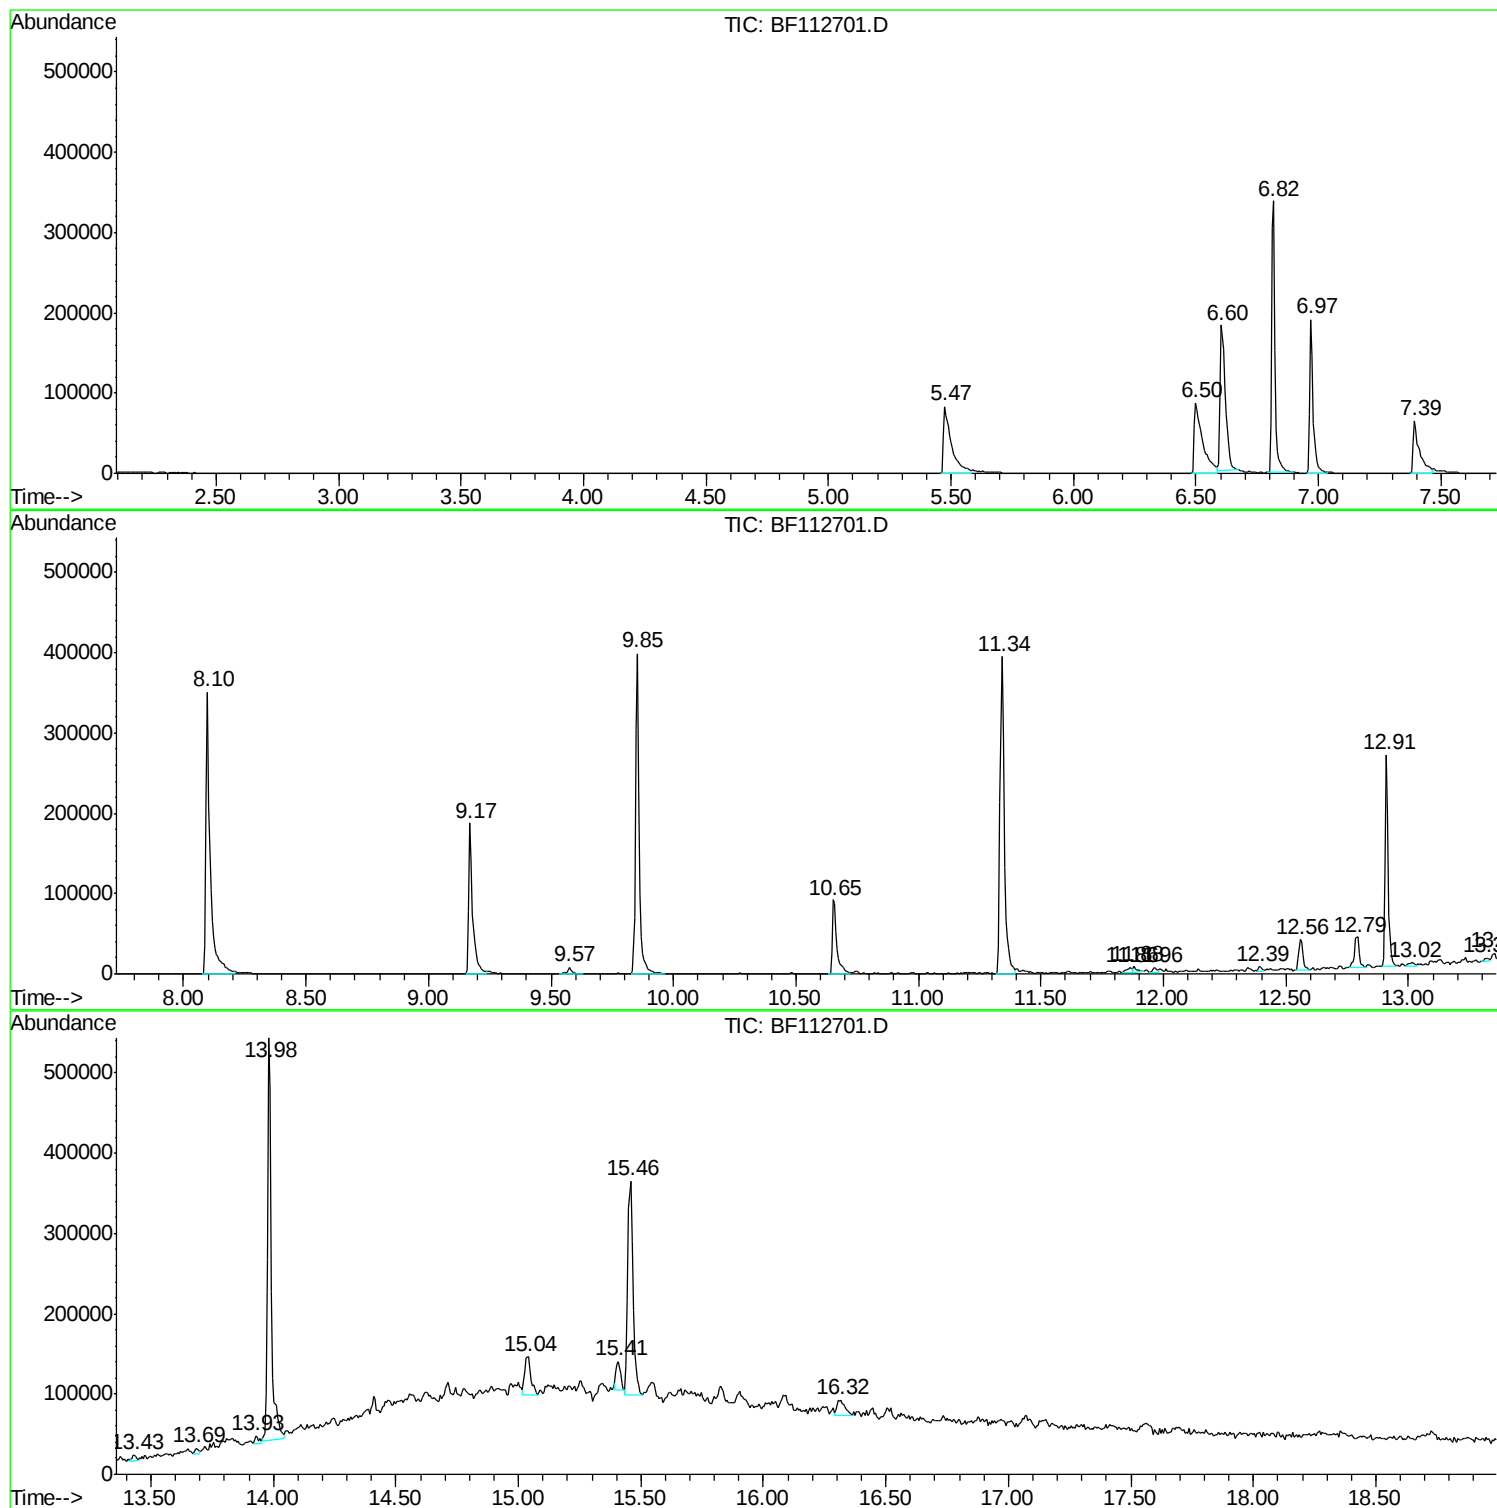

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF022519\
Data File : BF112701.D
Acq On : 25 Feb 2019 19:13
Operator : JU/SJ
Sample : K1596-03 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP-15










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.60 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.60	14.33 ng	250852	1,4-Dichlorobenzene-d4	6.82

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	5-Aminoindole	132	C8H8N2	005192-03-0	22
2		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
3		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
4		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9
5		Xenon	132	Xe	007440-63-3	9

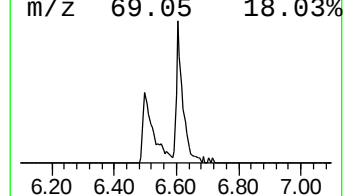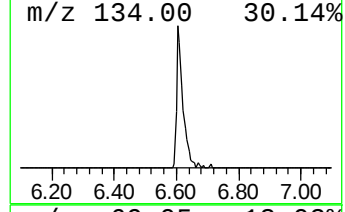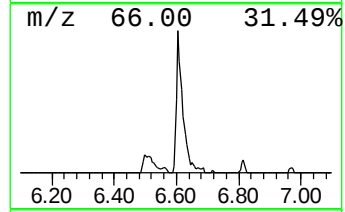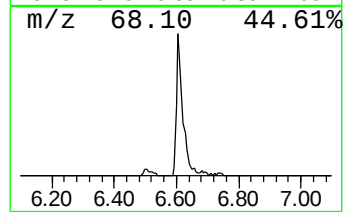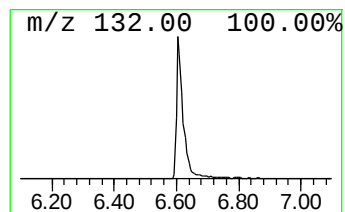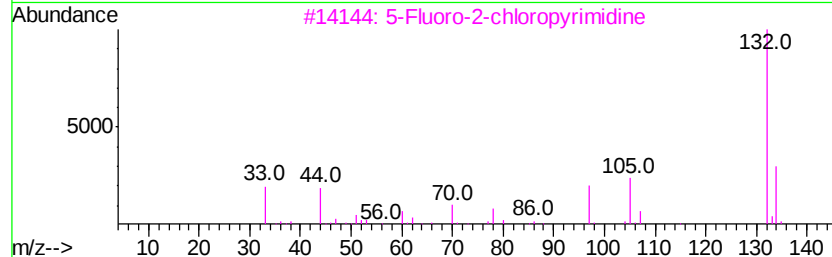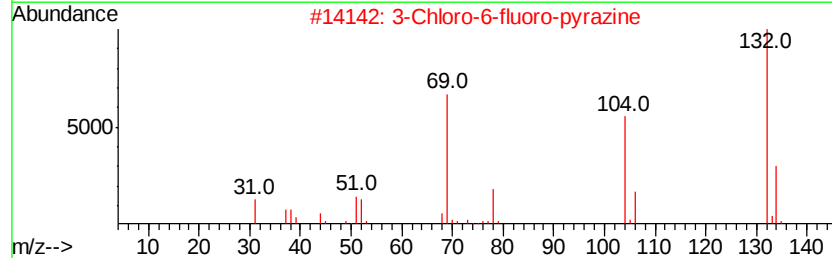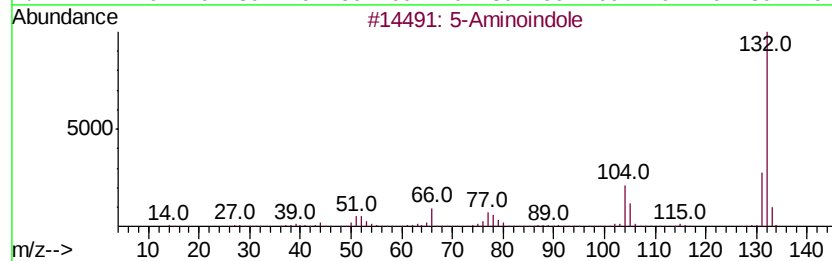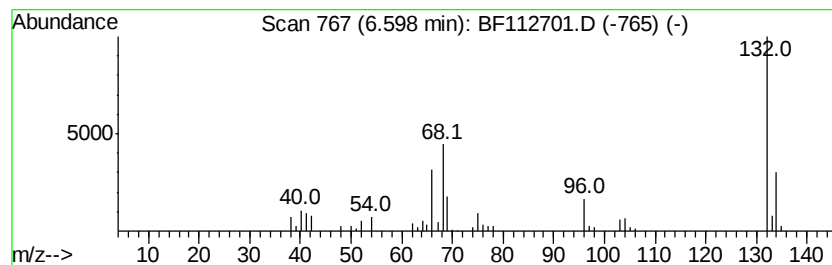

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF022519\
Data File : BF112701.D
Acq On : 25 Feb 2019 19:13
Operator : JU/SJ
Sample : K1596-03 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP-15

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.60	6.60	14.3	ng	250852	1	6.82	350084	20.0