


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022519\
 Data File : BF112684.D
 Acq On : 25 Feb 2019 10:57
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 28 10:38:18 2019

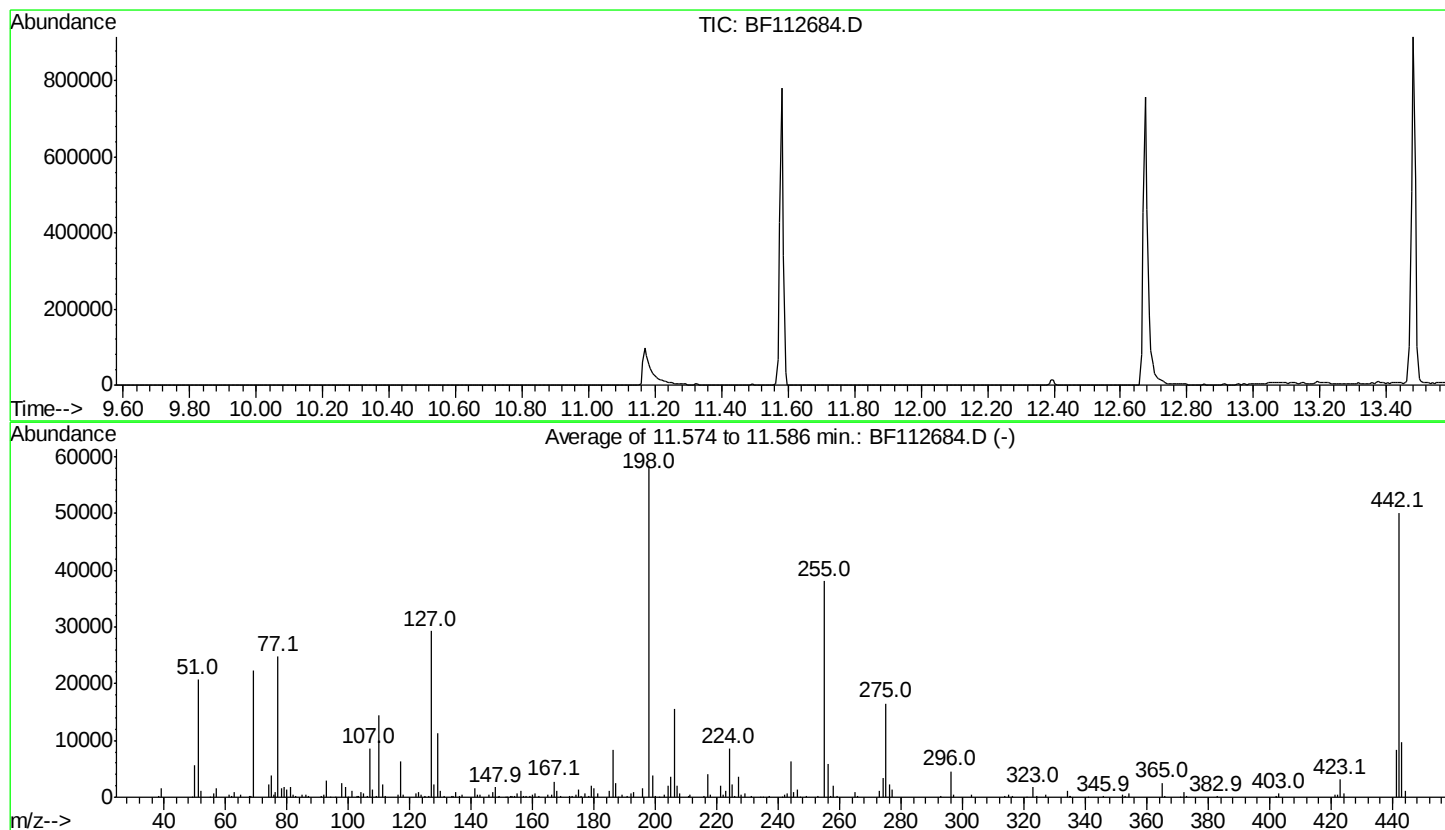

AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.4	20645	PASS
68	69	0.00	2	1.3	298	PASS
69	198	0.00	100	38.2	22314	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.1	29252	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	58394	PASS
199	198	5	9	6.6	3843	PASS
275	198	10	60	28.3	16506	PASS
365	198	1	100	4.3	2515	PASS
441	198	0.01	100	14.4	8432	PASS
442	198	50	100	85.9	50144	PASS
443	442	15	24	19.4	9751	PASS