
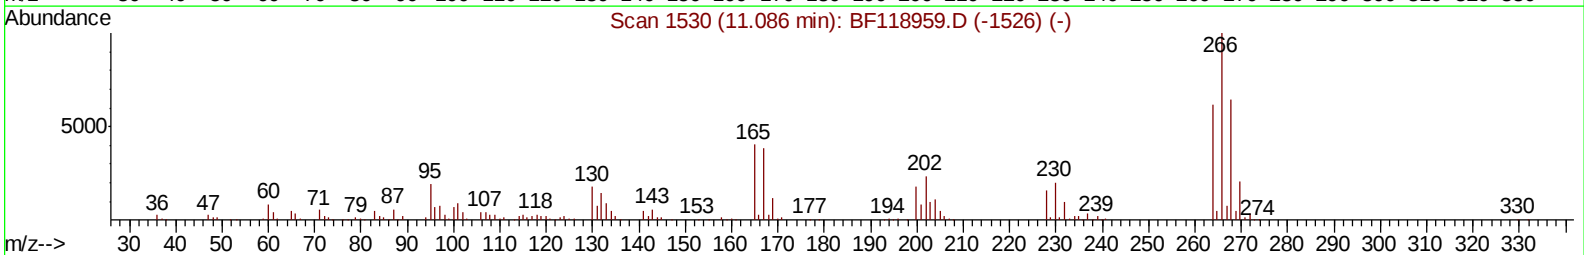
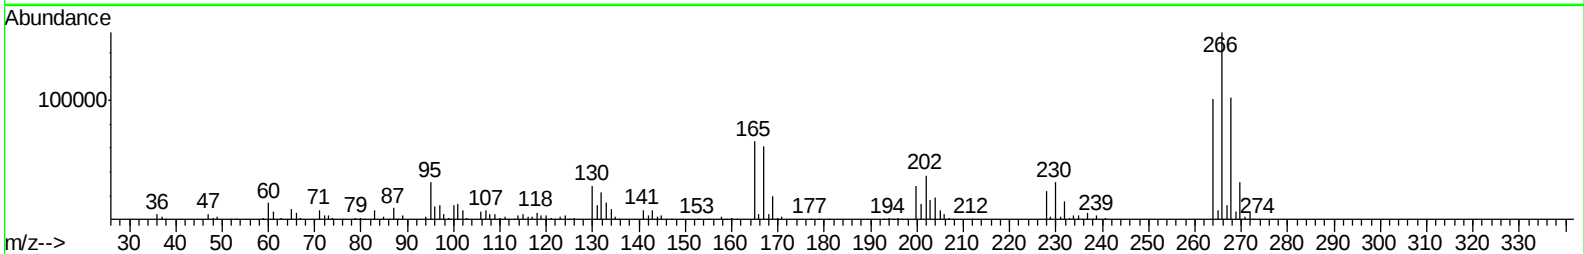


```
Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF022520\  
Data File : BF119063.D  
Acq On    : 25 Feb 2020 13:56  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1      Sample Multiplier: 1
```

Quant Time: Feb 26 06:47:45 2020
Quant Method : Z:\SV0ASRV\HPCHEM1\BNA F\METHODS\8270-BF022020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 20 17:40:17 2020
Response via : Initial Calibration

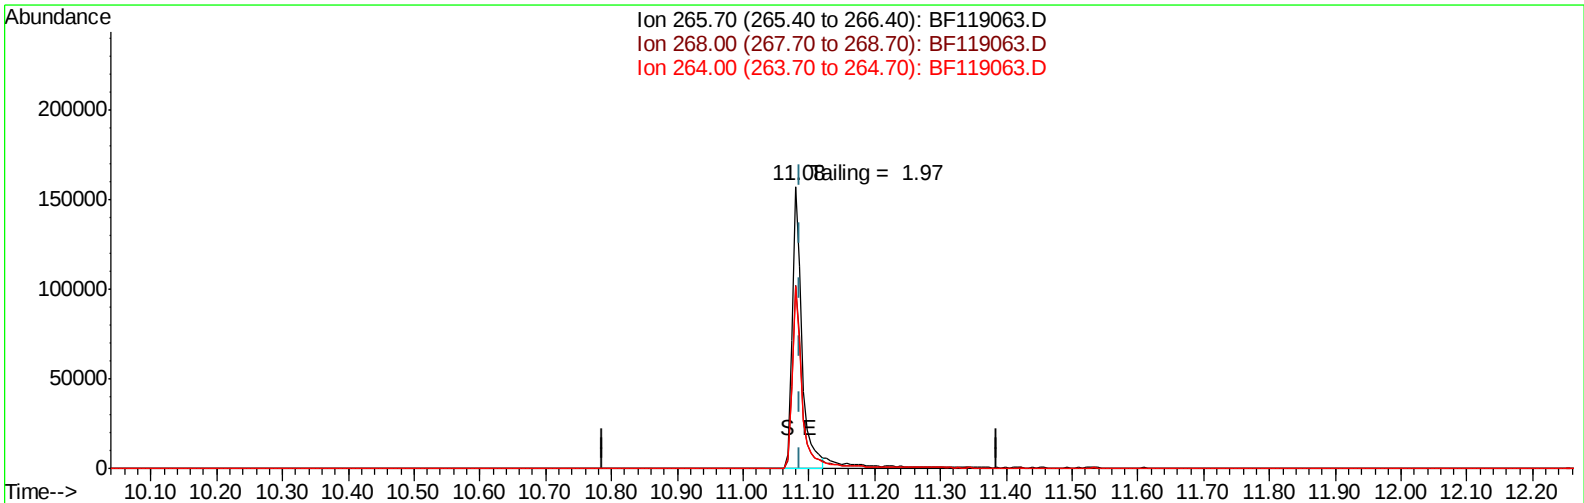

TIC: BF119063.D

(70) Pentachlorophenol (C)




11.080min (-0.006) 215272.02ng

response 175120

Ion	Exp%	Act%
265.70	100	100
268.00	64.20	64.90
264.00	61.90	64.48
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF022520\
 Data File : BF119063.D
 Acq On : 25 Feb 2020 13:56
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 26 06:47:45 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 20 17:40:17 2020
 Response via : Initial Calibration

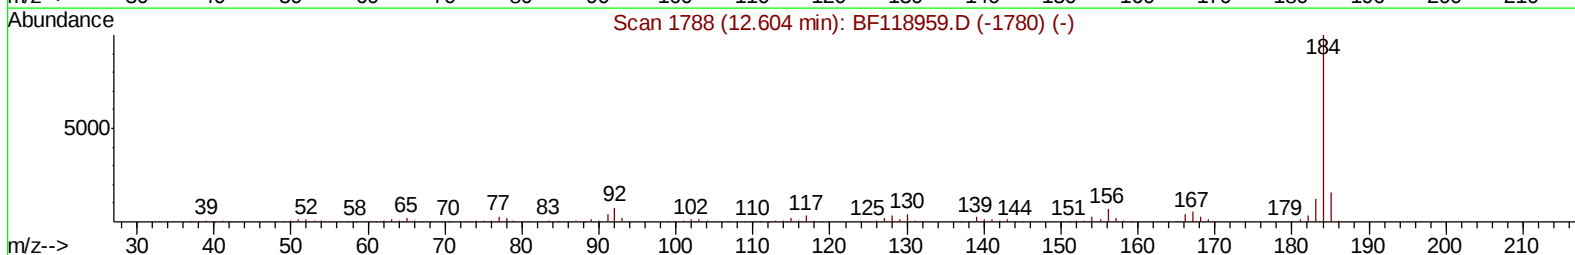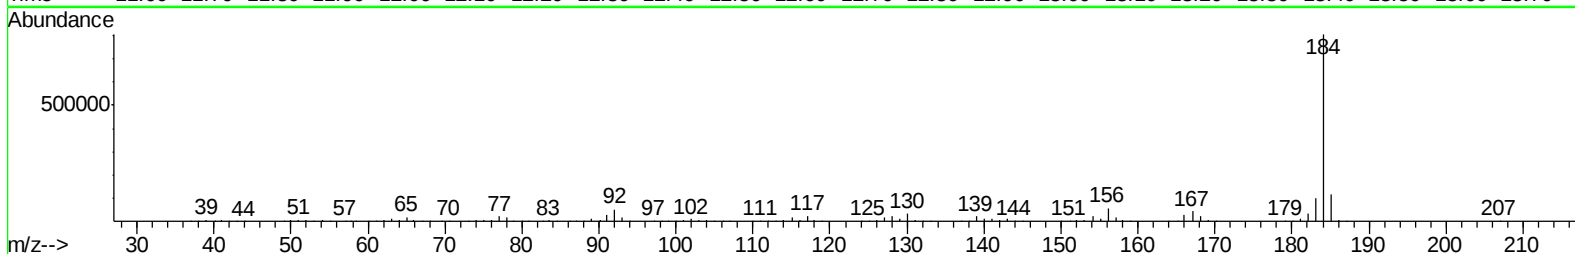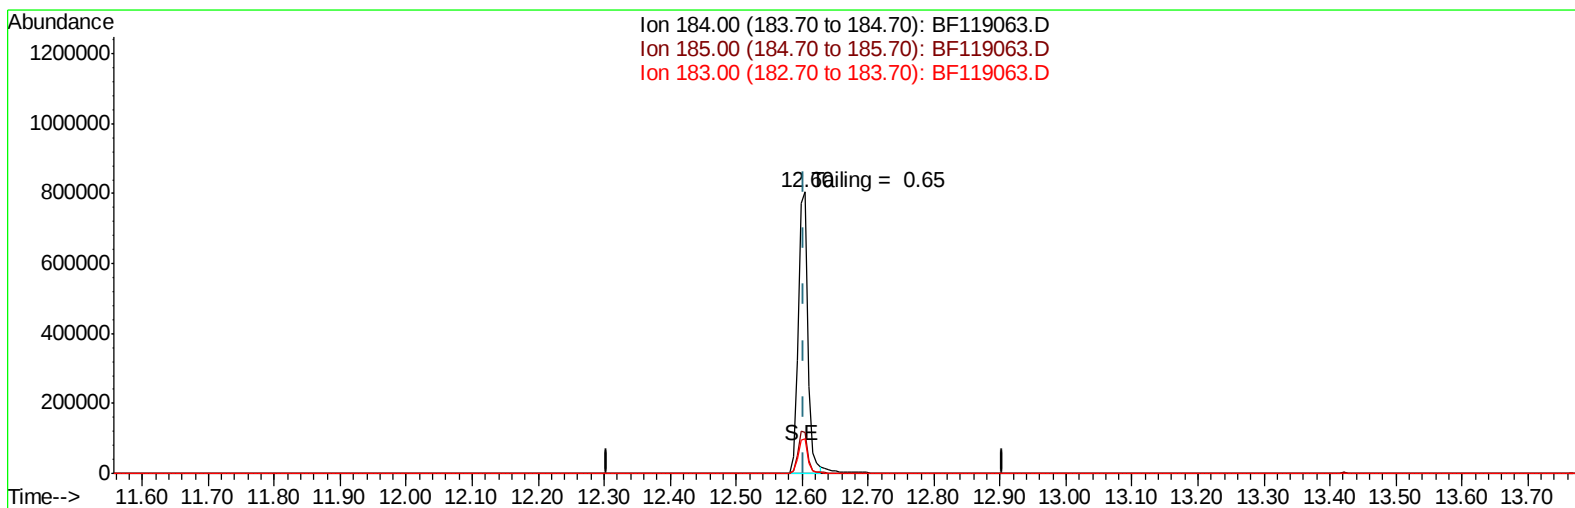

TIC: BF119063.D

(77) Benzidine

12.604min (-0.000) 54318.38ng

response 841661

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	14.37
183.00	12.40	12.10
0.00	0.00	0.00