

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF022520\
 Data File : BF119069.D
 Acq On : 25 Feb 2020 17:19
 Operator : CG/JU
 Sample : L1602-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 0178-COMP-SL-B-ELUTRIATE

Quant Time: Feb 26 02:54:18 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 20 17:40:17 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.75	152	197224	20.00	ng	-0.01
21) Naphthalene-d8	8.03	136	764840	20.00	ng	-0.01
39) Acenaphthene-d10	9.79	164	424887	20.00	ng	0.00
64) Phenanthrene-d10	11.27	188	802649	20.00	ng	0.00
76) Chrysene-d12	13.90	240	657218	20.00	ng	0.00
87) Perylene-d12	15.33	264	557414	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.39	112	547935	46.43	ng	0.00
7) Phenol-d6	6.40	99	134048	9.34	ng	0.00
23) Nitrobenzene-d5	7.32	82	1141797	78.82	ng	-0.01
42) 2,4,6-Tribromophenol	10.58	330	663369	119.35	ng	0.00
45) 2-Fluorobiphenyl	9.11	172	2193551	76.06	ng	-0.01
79) Terphenyl-d14	12.86	244	2415507	63.28	ng	0.00
Target Compounds						
50) Dimethylphthalate	9.50	163	180171	5.545	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF022520\
Data File : BF119069.D
Acq On : 25 Feb 2020 17:19
Operator : CG/JU
Sample : L1602-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
0178-COMP-SL-B-ELUTRIATE

Quant Time: Feb 26 02:54:18 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 20 17:40:17 2020
Response via : Initial Calibration

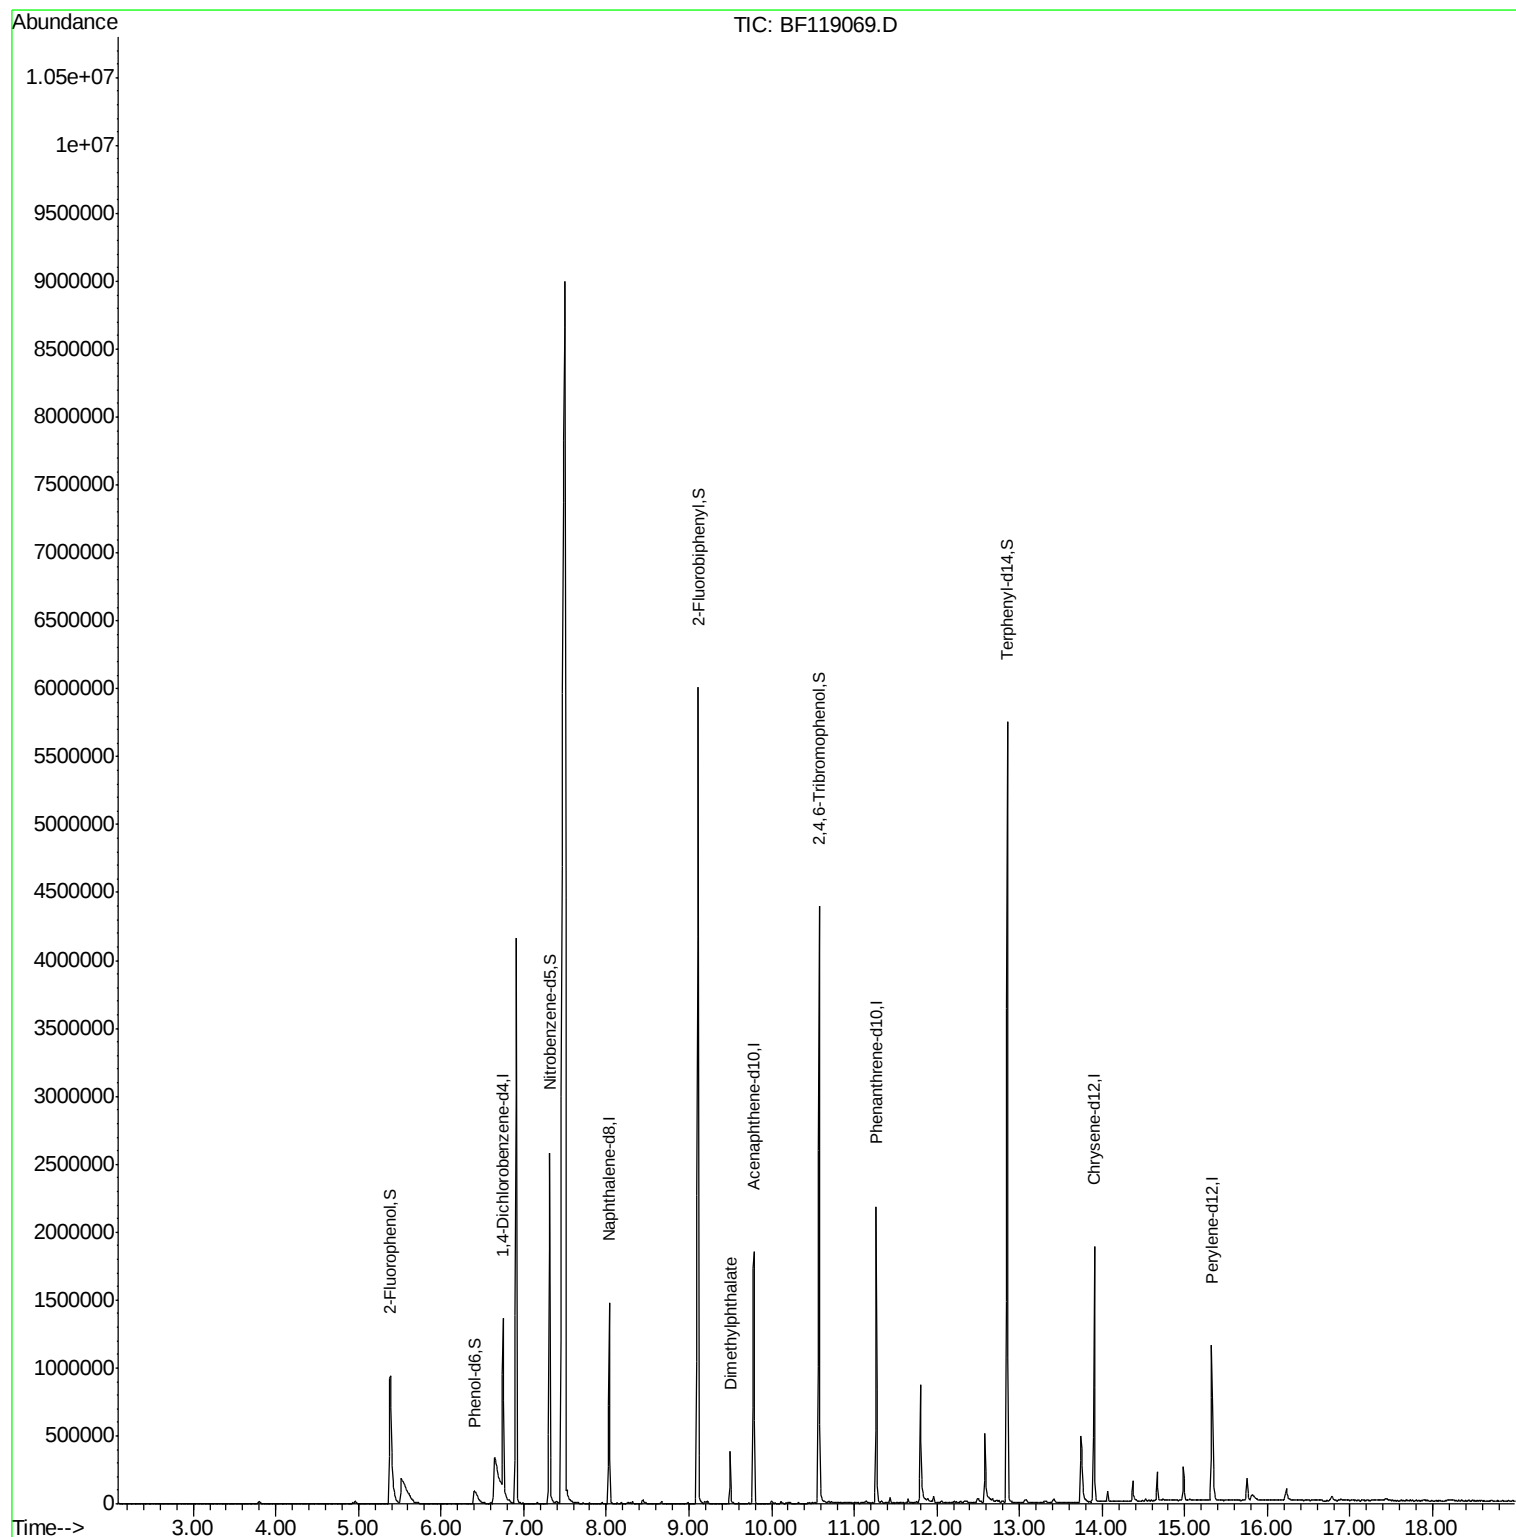

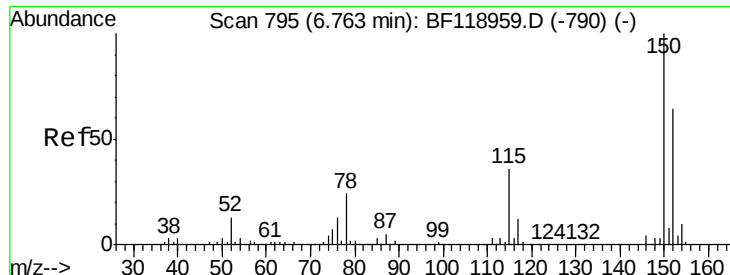


#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.75 min Scan# 793
Delta R.T. -0.01 min
Lab File: BF119069.D
Acq: 25 Feb 2020 17:19

Instrument :
BNA_F
ClientSampleId :
0178-COMP-SL-B-ELUTRIATE

Tot Ion:152 Resp: 197224
Ion Ratio Lower Upper
152 100
150 155.9 124.3 186.5
115 59.7 44.6 67.0

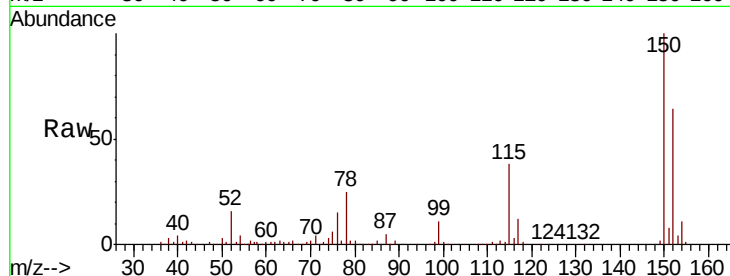


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

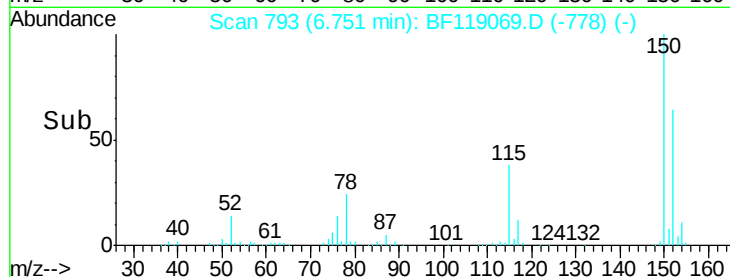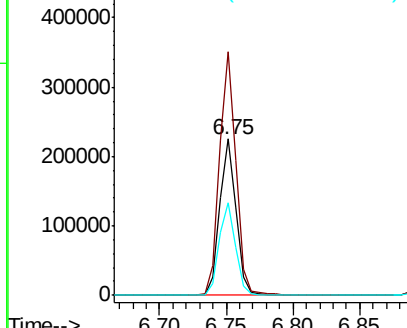



#5

2-Fluorophenol
Concen: 46.429 ng
RT: 5.39 min Scan# 561
Delta R.T. 0.01 min
Lab File: BF119069.D
Acq: 25 Feb 2020 17:19

Tgt Ion:112 Resp: 547935
Ion Ratio Lower Upper
112 100
64 51.6 40.4 60.6
63 27.3 21.3 31.9

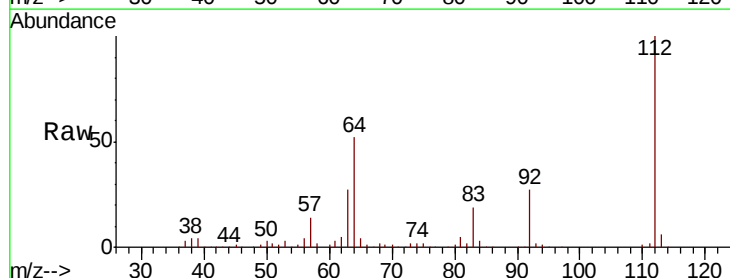

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

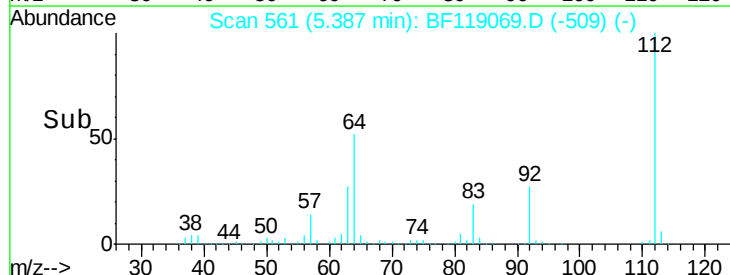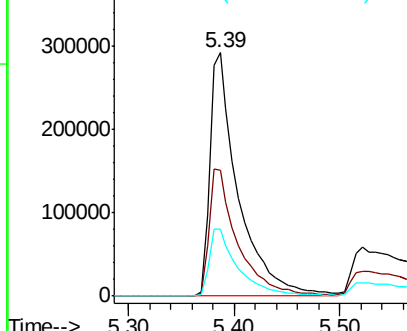



#7

Phenol-d6

Concen: 9.340 ng

RT: 6.40 min Scan# 734

Delta R.T. -0.00 min

Lab File: BF119069.D

Acq: 25 Feb 2020 17:19

Instrument :

BNA_F

ClientSampleId :

0178-COMP-SL-B-ELUTRIATE


Tot Ion: 99 Resp: 134048

Ion Ratio Lower Upper

99 100

42 13.0 11.4 17.0



71 37.5 29.8 44.6

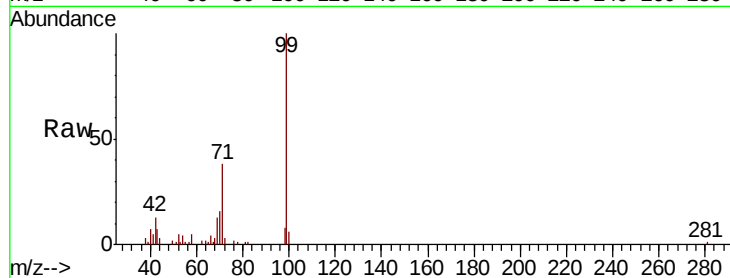

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

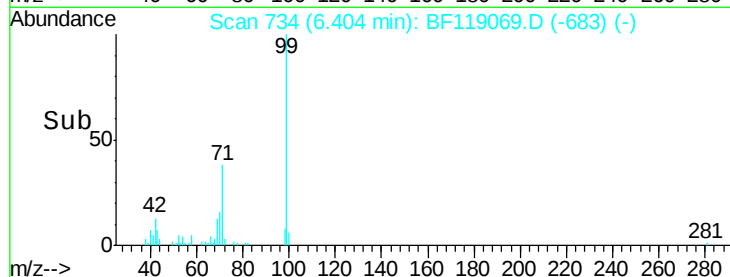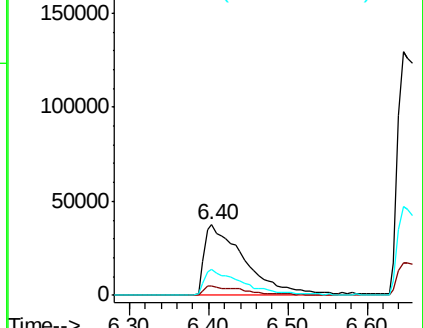

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.03 min Scan# 1011

Delta R.T. -0.01 min

Lab File: BF119069.D

Acq: 25 Feb 2020 17:19

Tgt Ion: 136 Resp: 764840


Ion Ratio Lower Upper

136 100

137 11.4 8.9 13.3

54 5.5 3.8 5.6

68 5.3 4.2 6.2


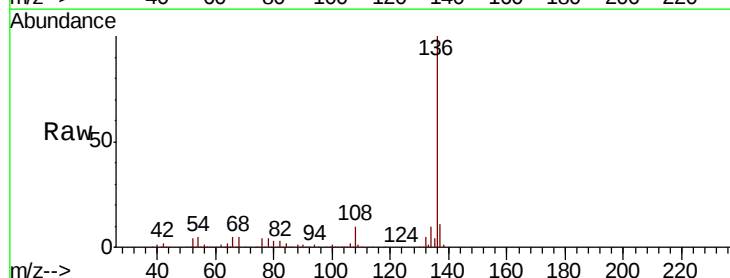


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

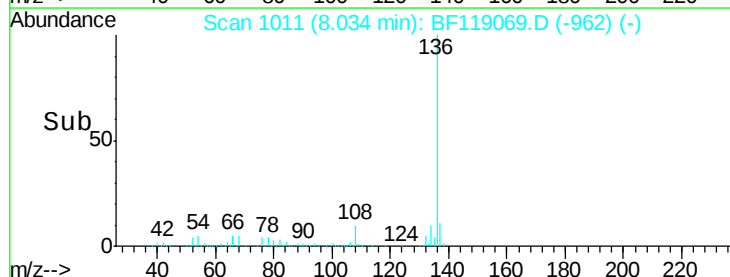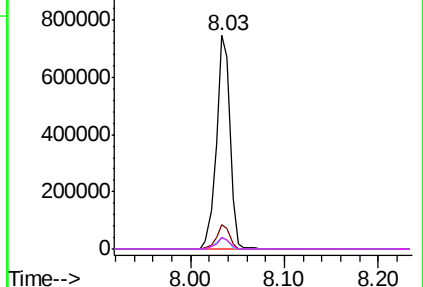




#23
 Nitrobenzene-d5
 Concen: 78.823 ng
 RT: 7.32 min Scan# 889
 Delta R.T. -0.01 min
 Lab File: BF119069.D
 Acq: 25 Feb 2020 17:19




Instrument :
 BNA_F
 ClientSampleId :
 0178-COMP-SL-B-ELUTRIATE

Tot Ion: 82 Resp: 1141797

Ion	Ratio	Lower	Upper
82	100		
128	47.0	38.2	57.2
54	40.4	31.3	46.9

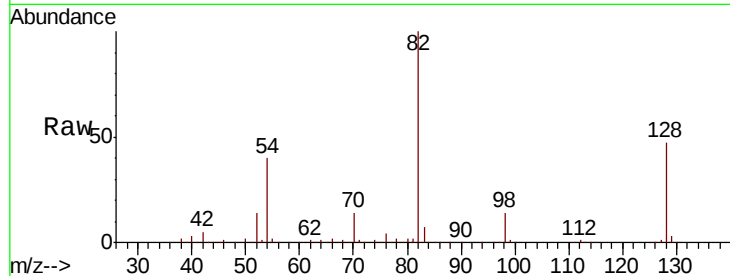


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF1

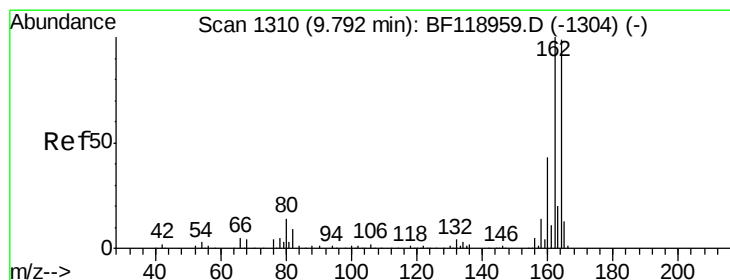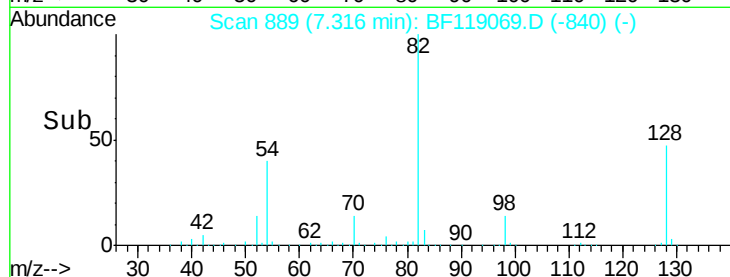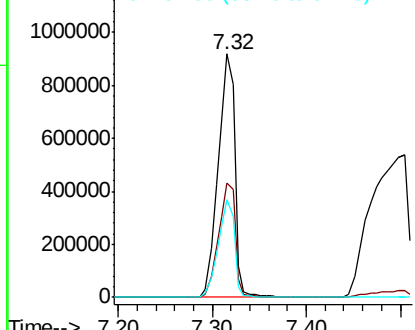



#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.79 min Scan# 1309
 Delta R.T. -0.01 min
 Lab File: BF119069.D
 Acq: 25 Feb 2020 17:19

Tgt Ion: 164 Resp: 424887

Ion	Ratio	Lower	Upper
164	100		
162	102.8	81.2	121.8
160	44.7	35.2	52.8

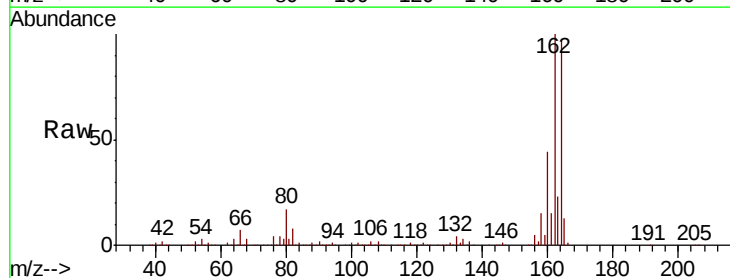

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

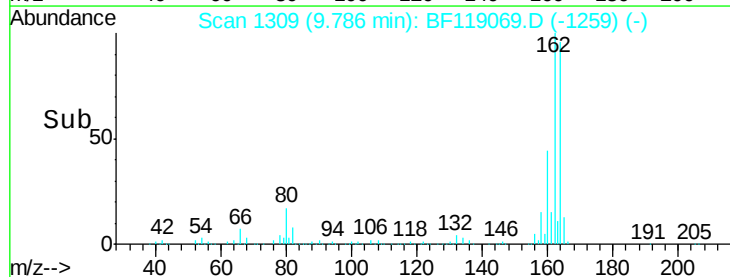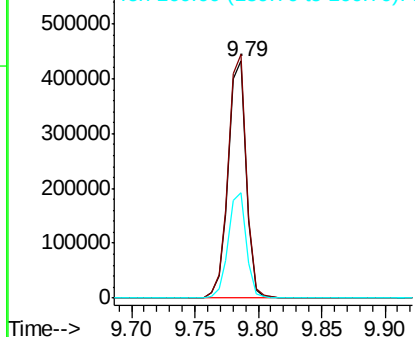







#42
 2,4,6-Tribromophenol
 Concen: 119.349 ng
 RT: 10.58 min Scan# 1444
 Delta R.T. -0.00 min
 Lab File: BF119069.D
 Acq: 25 Feb 2020 17:19

Instrument :
 BNA_F
 ClientSampleId :
 0178-COMP-SL-B-ELUTRIATE

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.9	77.1	115.7
141	28.8	23.0	34.6

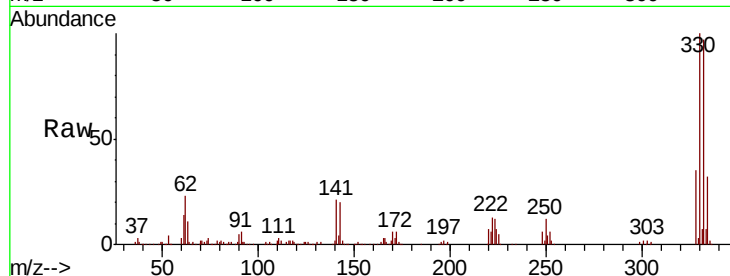


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

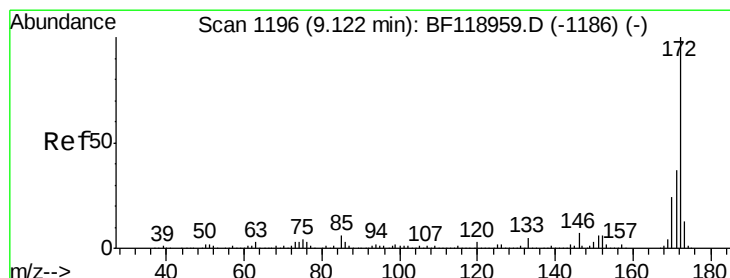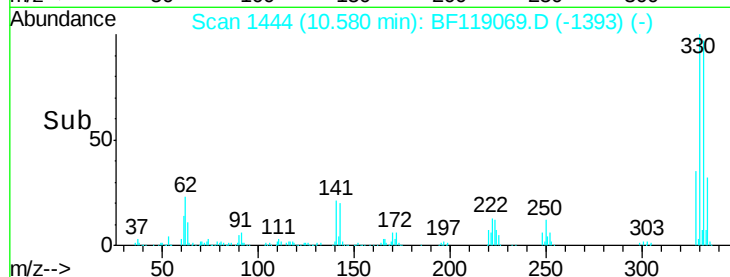
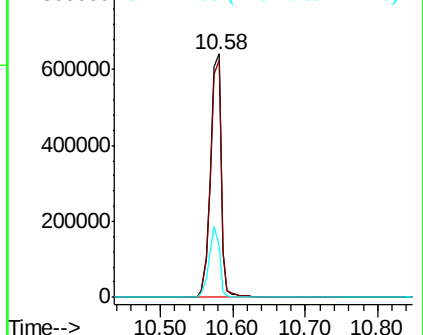



#45
 2-Fluorobiphenyl
 Concen: 76.055 ng
 RT: 9.11 min Scan# 1194
 Delta R.T. -0.01 min
 Lab File: BF119069.D
 Acq: 25 Feb 2020 17:19

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.6	29.4	44.2
170	24.7	19.6	29.4

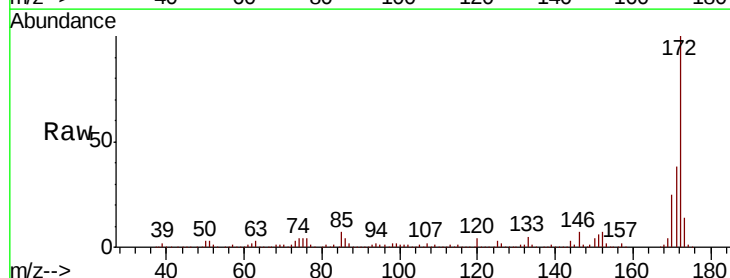

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

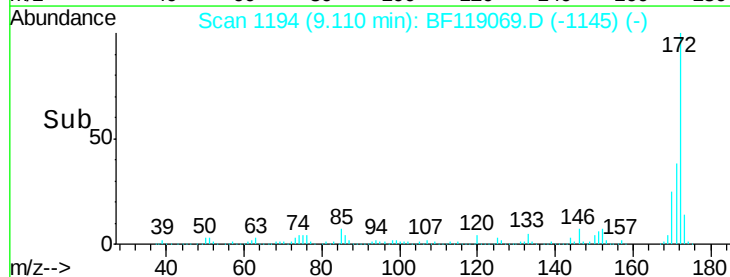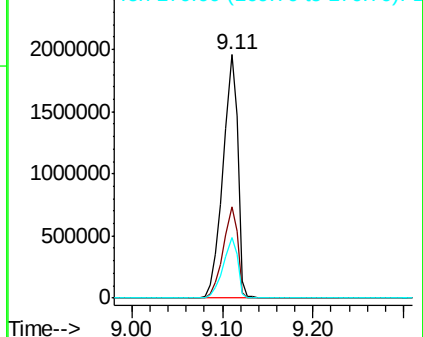

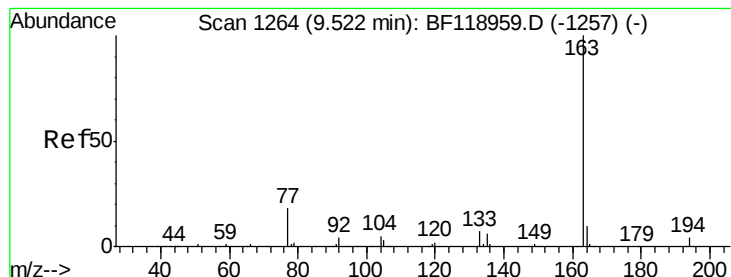

#50

Dimethylphthalate

Concen: 5.545 ng

RT: 9.50 min Scan# 1261

Delta R.T. -0.02 min

Lab File: BF119069.D

Acq: 25 Feb 2020 17:19

Instrument :

BNA_F

ClientSampleId :

0178-COMP-SL-B-ELUTRIATE


Tot Ion:163 Resp: 180171

Ion Ratio Lower Upper

163 100

194 4.4 3.4 5.2




164 9.7 8.2 12.2

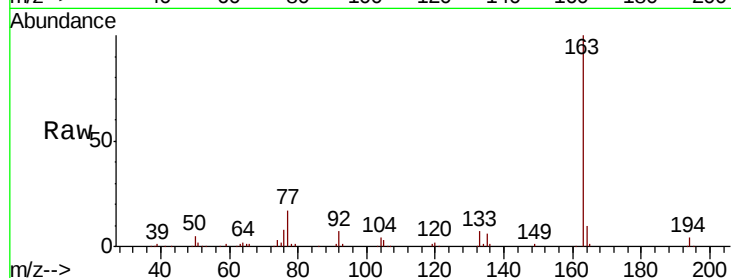

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

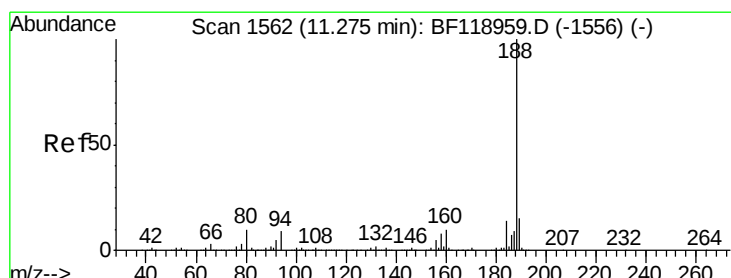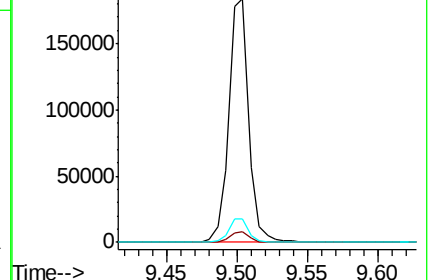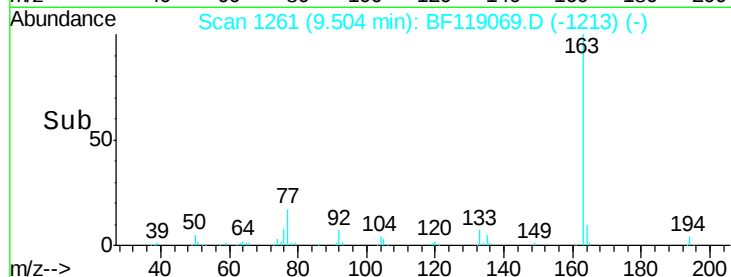

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.27 min Scan# 1561

Delta R.T. -0.01 min

Lab File: BF119069.D

Acq: 25 Feb 2020 17:19


Tgt Ion:188 Resp: 802649

Ion Ratio Lower Upper

188 100

94 8.4 7.0 10.6



80 8.8 7.9 11.9

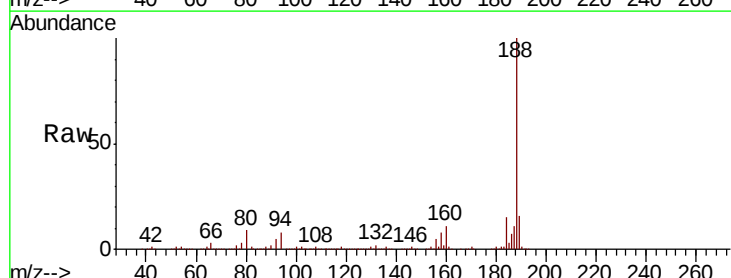

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

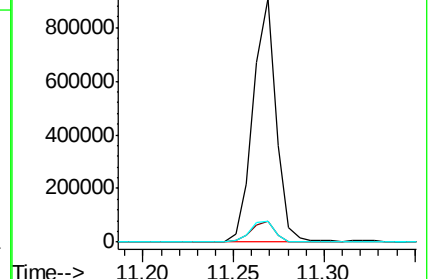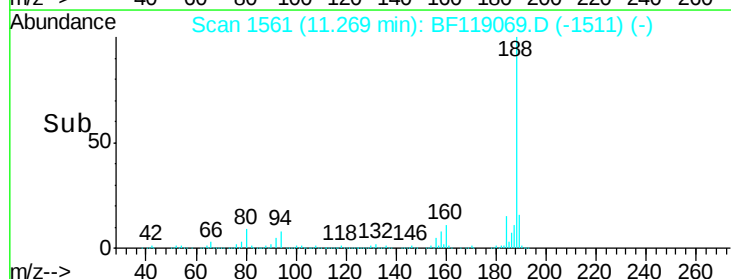



#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.90 min Scan# 2009

Delta R.T. -0.01 min

Lab File: BF119069.D

Acq: 25 Feb 2020 17:19

Instrument :

BNA_F

ClientSampleId :

0178-COMP-SL-B-ELUTRIATE


Tot Ion:240 Resp: 657218

Ion Ratio Lower Upper

240 100

120 9.4 8.9 13.3




236 25.9 20.6 30.8

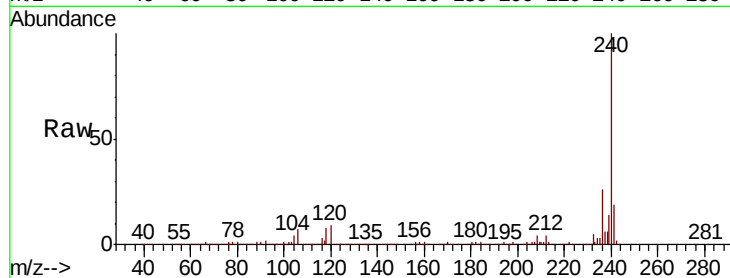

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

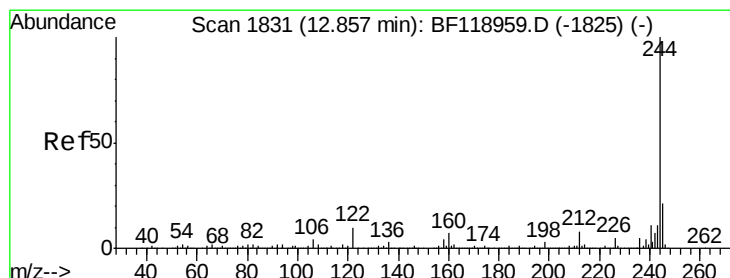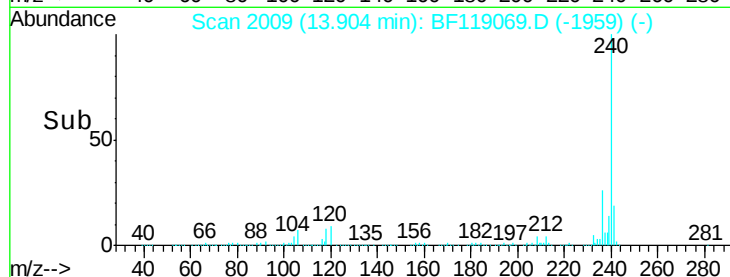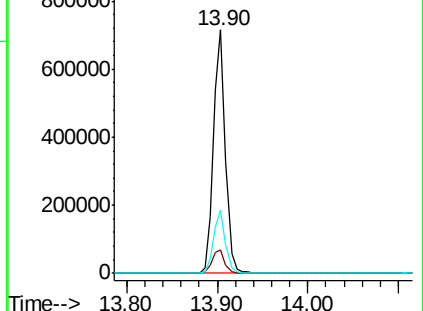

#79

Terphenyl-d14

Concen: 63.278 ng

RT: 12.86 min Scan# 1831

Delta R.T. -0.00 min

Lab File: BF119069.D

Acq: 25 Feb 2020 17:19


Tgt Ion:244 Resp: 2415507

Ion Ratio Lower Upper

244 100

212 7.5 6.3 9.5



122 8.7 8.4 12.6

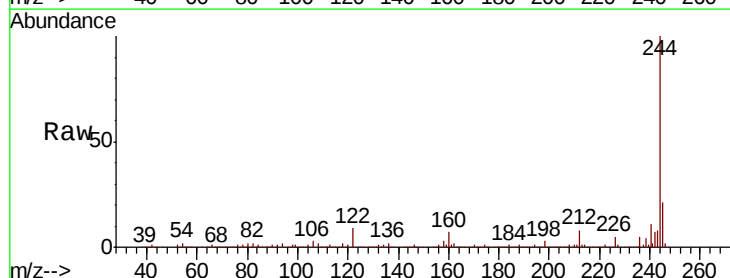


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

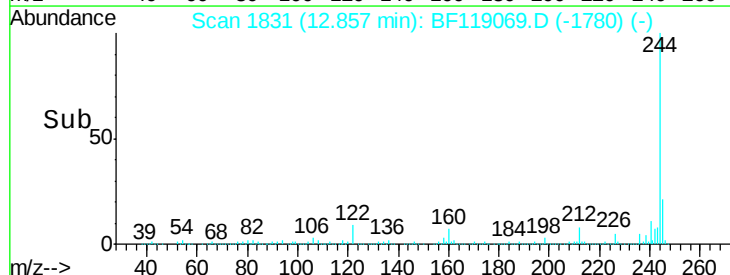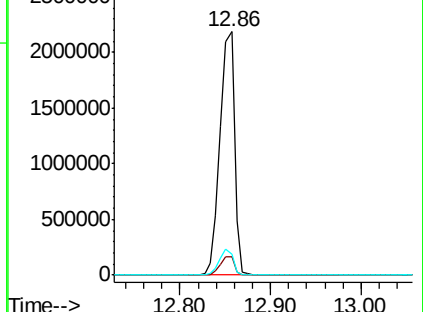


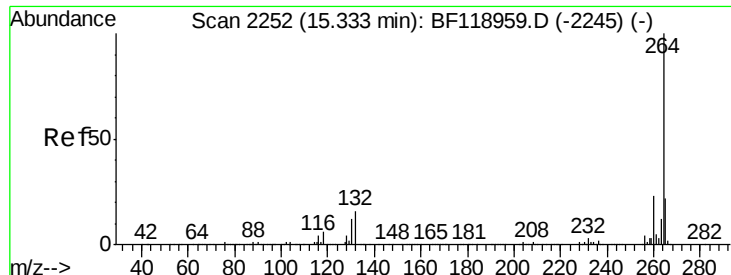

#87
 Pervlene-d12
 Concen: 20.000 ng
 RT: 15.33 min Scan# 2251
 Delta R.T. -0.01 min
 Lab File: BF119069.D
 Acq: 25 Feb 2020 17:19

Instrument :
 BNA_F
 ClientSampleId :
 0178-COMP-SL-B-ELUTRIATE

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.5	18.6	28.0
265	22.4	17.3	25.9

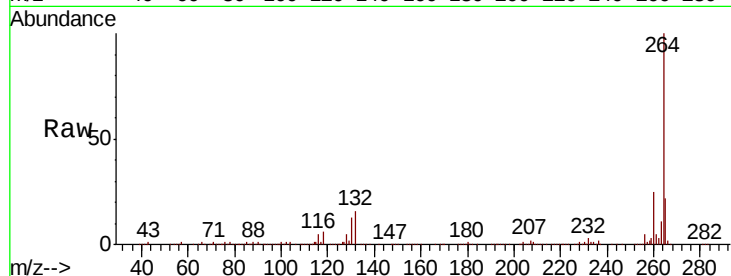

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

