


Data Path : Z:\SVOASRV\HPCHEM1\BNA\_F\DATA\BF022520\  
 Data File : BF119063.D  
 Acq On : 25 Feb 2020 13:56  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF022020.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Thu Feb 20 17:40:17 2020

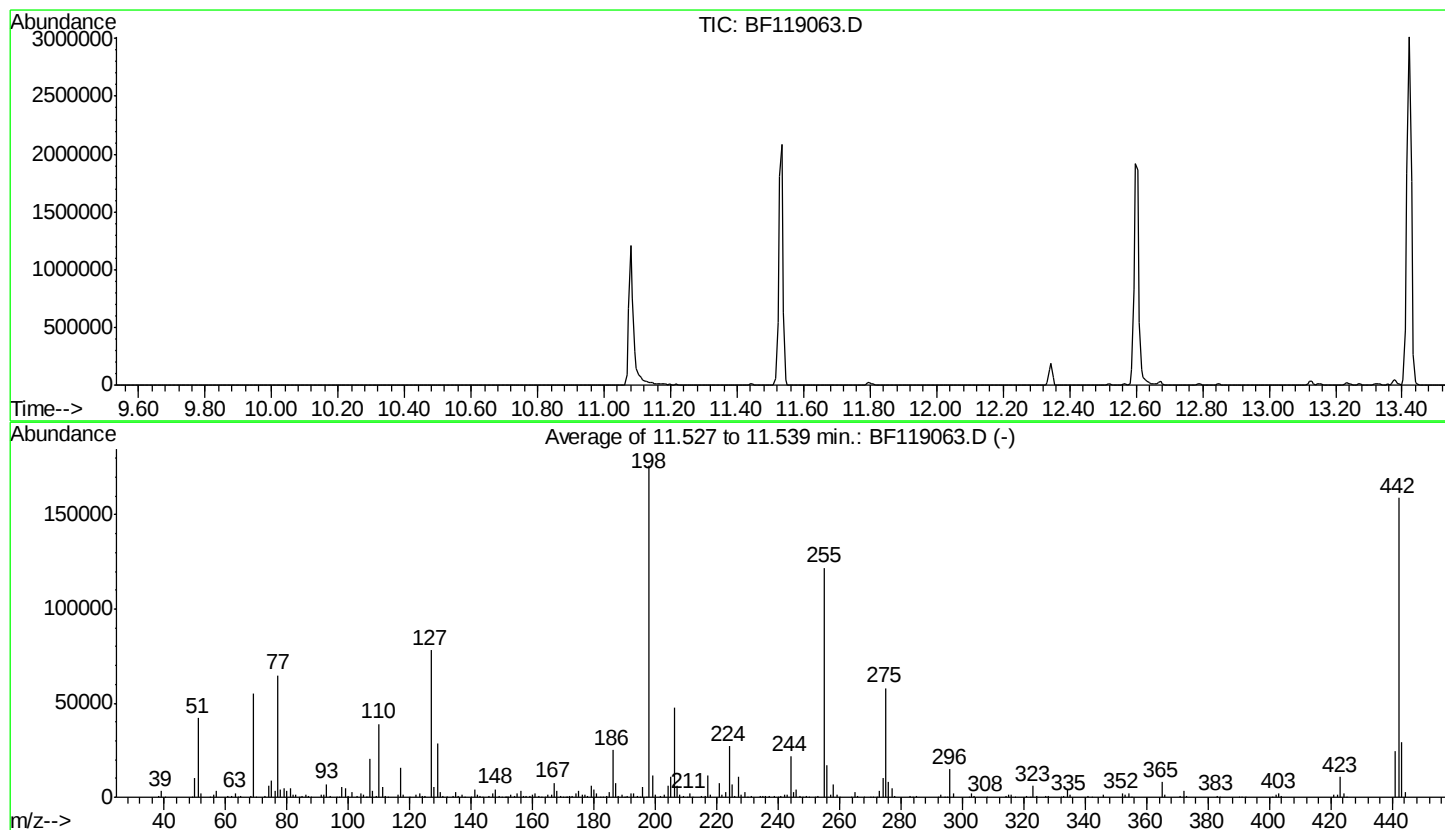

AutoFind: Scans 1605, 1606, 1607; Background Corrected with Scan 1599

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 23.8      | 41926   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.8       | 1023    | PASS             |
| 69          | 198          | 0.00         | 100          | 31.5      | 55433   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.2       | 116     | PASS             |
| 127         | 198          | 10           | 80           | 44.3      | 77992   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.1       | 193     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 176157  | PASS             |
| 199         | 198          | 5            | 9            | 6.5       | 11453   | PASS             |
| 275         | 198          | 10           | 60           | 33.0      | 58101   | PASS             |
| 365         | 198          | 1            | 100          | 4.6       | 8047    | PASS             |
| 441         | 198          | 0.01         | 100          | 13.9      | 24565   | PASS             |
| 442         | 198          | 50           | 100          | 90.2      | 158952  | PASS             |
| 443         | 442          | 15           | 24           | 18.3      | 29165   | PASS             |