


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022522\
Data File : BF127065.D
Acq On : 25 Feb 2022 11:47
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 26 05:25:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 24 02:10:57 2022
Response via : Initial Calibration

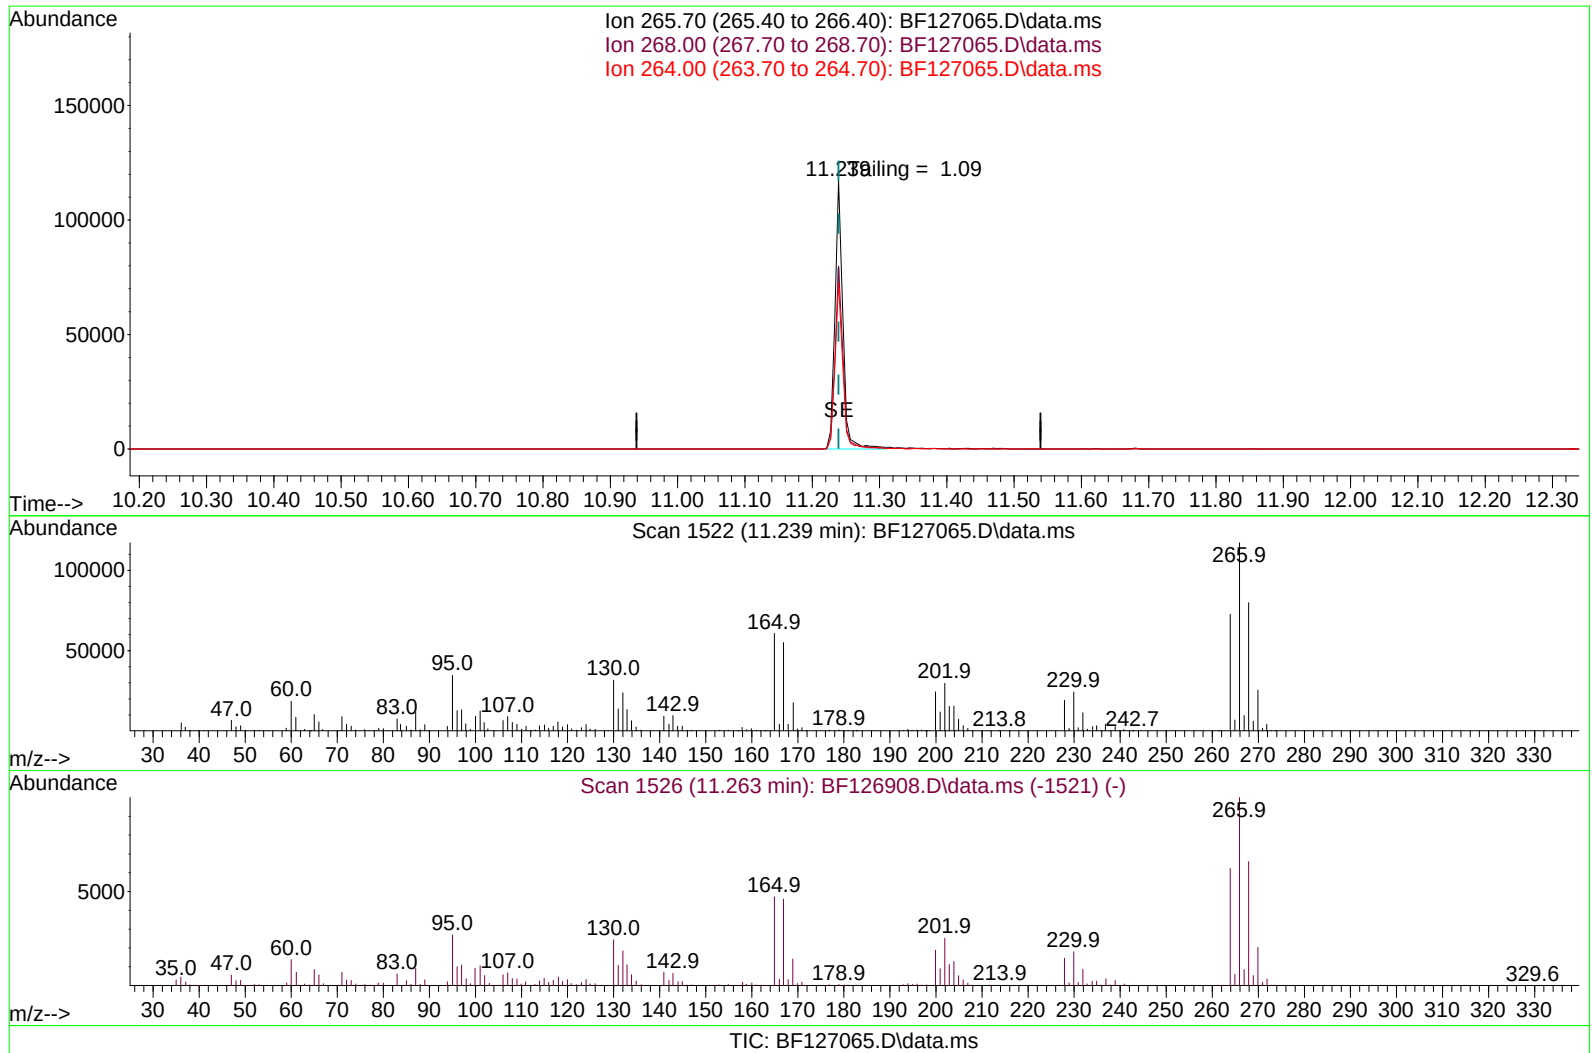

(70) Pentachlorophenol (C)




11.239min (0.000) 24575.57 ng

response 96172

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	68.13
264.00	63.00	62.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022522\
 Data File : BF127065.D
 Acq On : 25 Feb 2022 11:47
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 26 05:25:24 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 24 02:10:57 2022
 Response via : Initial Calibration

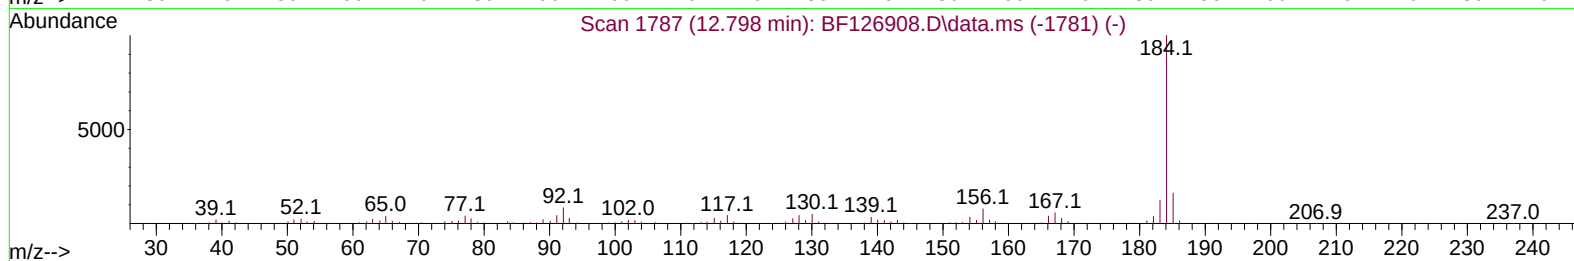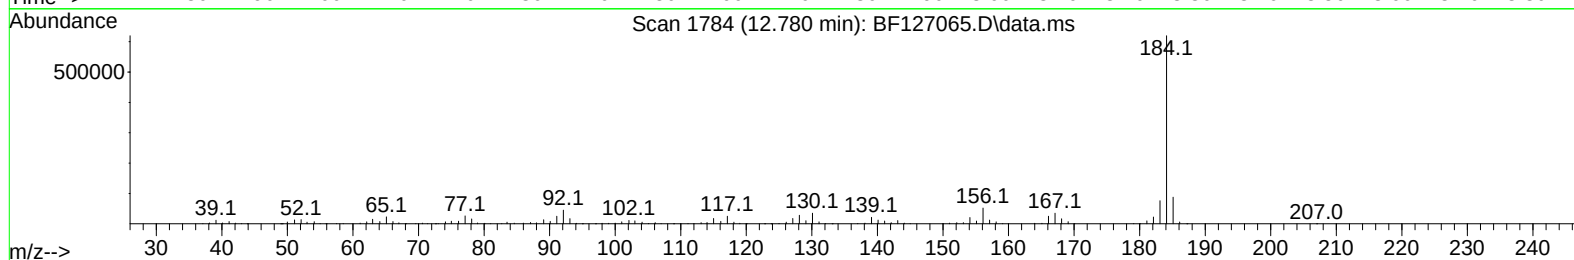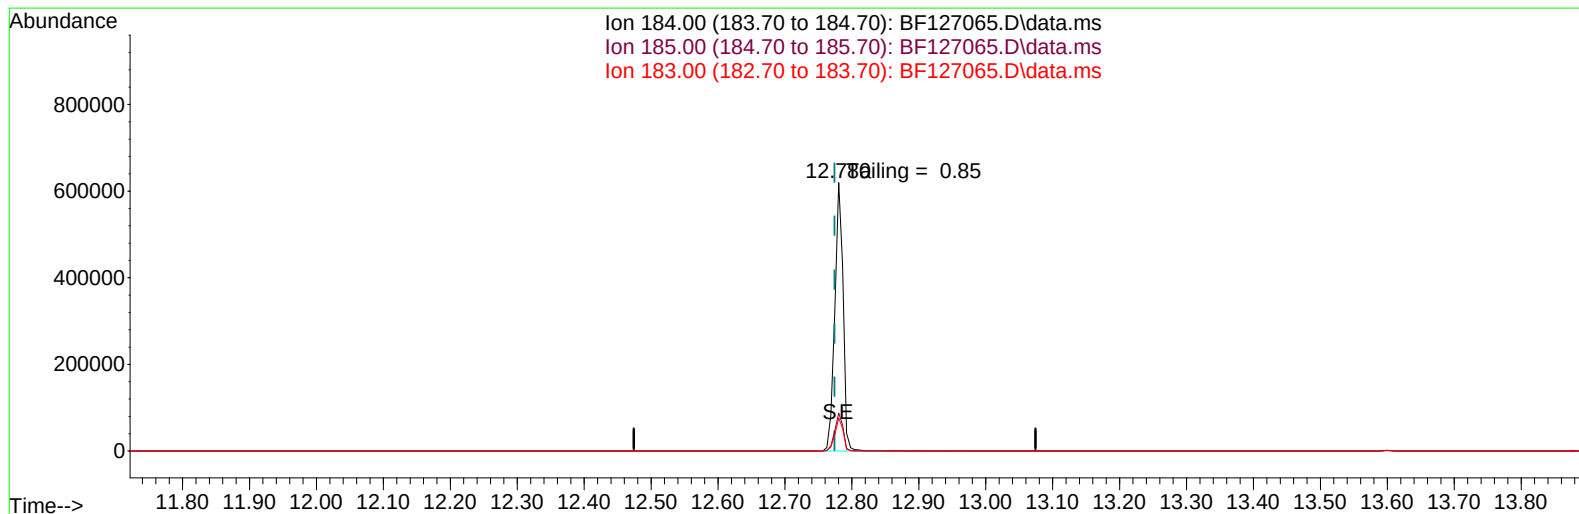

TIC: BF127065.D\data.ms

(77) Benzidine

12.780min (+ 0.006) 0.00 ng

response 538173

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.17
183.00	10.20	12.31#
0.00	0.00	0.00